


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU042220\
 Data File : VU037839.D
 Acq On : 22 Apr 2020 09:12
 Operator : JC/MD
 Sample : BFB18
 Misc : 25mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR041420WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 23 01:37:32 2020

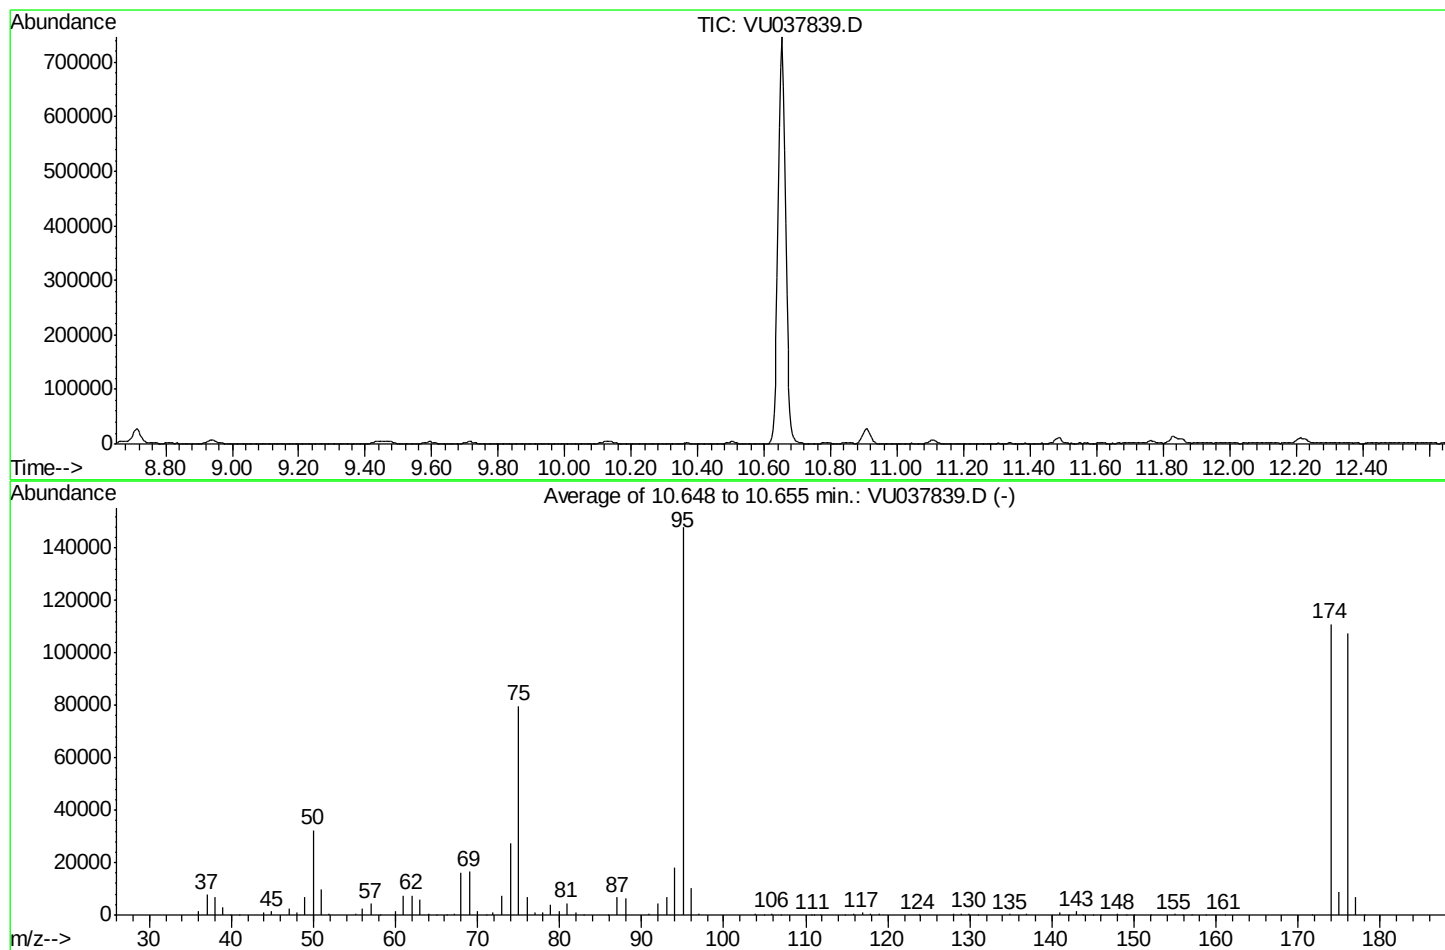

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.9	32365	PASS
75	95	30	80	53.8	79653	PASS
95	95	100	100	100.0	147968	PASS
96	95	5	9	6.9	10172	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.1	111101	PASS
175	174	5	9	8.1	9037	PASS
176	174	95	101	96.8	107562	PASS
177	176	5	9	6.5	6975	PASS

m/z	Abundance
36.00	1517.0
37.00	7687.0
38.00	6660.0
39.00	2860.0
39.90	313.0
40.90	100.0
44.00	1813.0
44.90	1370.0
47.00	2249.0
48.00	1033.0
49.00	6361.0
50.00	31520.0
51.00	9725.0
51.90	404.0
55.10	403.0
56.00	2821.0
57.00	4127.0
60.00	1375.0
61.00	7257.0
62.00	7539.0
63.00	5828.0
64.10	635.0
65.00	191.0
66.20	105.0
68.00	15042.0
69.00	15632.0
70.00	1310.0
71.00	148.0
71.90	878.0
73.00	7184.0
74.00	26336.0
75.00	76328.0
76.00	6881.0
76.90	887.0
78.00	764.0
78.90	3958.0
80.00	1231.0
80.90	4324.0
81.90	936.0
85.80	157.0
87.00	6058.0
88.00	6230.0
90.90	606.0
92.00	3973.0
93.10	6360.0
94.00	17256.0
95.00	141440.0
96.10	10120.0
97.00	285.0
103.90	492.0
104.90	200.0
105.90	679.0
110.70	168.0
114.80	175.0
115.80	564.0
116.90	863.0
117.90	570.0
119.00	539.0
123.80	110.0
127.90	372.0
128.90	301.0
129.90	541.0
131.00	130.0
134.90	241.0
136.90	242.0
141.00	1065.0
142.00	188.0
143.00	1314.0
145.00	207.0
145.90	167.0
148.00	282.0
150.00	114.0
152.00	108.0
155.00	306.0
155.90	110.0
157.00	215.0
158.80	124.0
161.00	138.0
171.60	160.0
174.00	104288.0
175.00	8782.0
176.00	101584.0
177.00	6657.0
178.00	255.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1553.0
37.00	7941.0
38.00	7200.0
39.00	3197.0
39.90	382.0
40.90	103.0
44.00	1814.0
44.90	1466.0
47.00	2651.0
48.00	1033.0
49.00	7024.0
50.00	33568.0
51.00	10076.0
52.00	514.0
55.10	385.0
56.00	2774.0
57.00	4463.0
60.00	1497.0
61.00	7610.0
62.00	7849.0
63.00	6153.0
64.00	720.0
65.10	179.0
66.30	110.0
67.10	593.0
68.00	16432.0
69.00	16904.0
70.00	1446.0
71.00	139.0
71.90	919.0
73.00	7489.0
74.00	28264.0
75.00	82064.0
76.00	7155.0
76.90	965.0
78.00	848.0
78.90	4056.0
80.00	1333.0
80.90	4556.0
81.90	977.0
85.90	191.0
87.00	6916.0
88.00	6529.0
90.90	593.0
92.00	4449.0
93.10	6926.0
94.00	18768.0
95.10	152960.0
96.10	10508.0
97.00	304.0
103.90	575.0
105.00	235.0
105.90	705.0
111.00	161.0
114.80	153.0
115.80	611.0
116.90	913.0
117.80	510.0
119.00	638.0
123.70	134.0
127.90	428.0
128.90	294.0
129.90	540.0
131.00	131.0
134.90	291.0
136.90	312.0
140.90	1114.0
142.00	204.0
143.00	1391.0
143.80	106.0
145.00	160.0
145.90	184.0
148.00	353.0
150.00	105.0
152.00	117.0
154.90	333.0
157.00	197.0
158.80	161.0
161.00	203.0
171.60	180.0
174.00	114680.0
175.00	9383.0
176.00	110872.0
177.00	7184.0
178.00	262.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	1353.0
37.00	7492.0
38.00	6869.0
39.00	3137.0
39.90	403.0
41.00	107.0
44.00	1638.0
44.90	1474.0
47.00	2744.0
48.00	920.0
49.00	6866.0
50.00	32008.0
51.00	9796.0
52.00	519.0
55.10	333.0
56.00	2515.0
57.00	4535.0
58.10	111.0
60.00	1413.0
61.00	7215.0
62.00	7277.0
63.00	5952.0
64.00	669.0
65.00	141.0
67.10	544.0
68.00	16424.0
69.00	16760.0
70.00	1461.0
71.90	909.0
73.00	7156.0
74.00	27416.0
75.00	80568.0
76.00	6834.0
77.00	971.0
78.00	727.0
78.90	3814.0
79.90	1303.0
80.90	4419.0
82.00	928.0
82.90	108.0
85.90	202.0
87.00	7115.0
88.00	6334.0
91.00	552.0
92.00	4527.0
93.10	6652.0
94.00	18368.0
95.00	149504.0
96.10	9888.0
97.00	272.0
103.90	582.0
105.00	241.0
105.90	642.0
106.90	110.0
111.00	188.0
111.80	116.0
114.80	135.0
115.90	584.0
116.90	959.0
117.80	454.0
119.00	716.0
128.00	458.0
128.90	279.0
129.90	495.0
131.00	121.0
134.90	310.0
137.00	286.0
141.00	1093.0
142.00	191.0
143.00	1375.0
143.80	132.0
145.00	102.0
145.90	215.0
148.00	326.0
149.00	107.0
149.90	114.0
154.90	305.0
156.90	190.0
158.80	168.0
161.00	214.0
174.00	114336.0
175.00	8946.0
176.00	110232.0
177.00	7086.0
178.10	197.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

Scan 2882 (10.607 min): VU037839.D
BFB18

m/z	Abundance
39.90	236.0
43.90	629.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18