

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042221\
 Data File : VU043282.D
 Acq On : 22 Apr 2021 16:48
 Operator : SY/MD
 Sample : M2124-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4527

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043282.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	72	82	92	rBV	28158	33000	6.48%	0.967%
2	1.922	172	181	189	rBV	27576	35258	6.93%	1.033%
3	2.575	373	384	397	rBV	67694	111148	21.84%	3.258%
4	4.655	1013	1031	1064	rBV	56391	209989	41.26%	6.155%
5	5.076	1147	1162	1189	rVB	73789	171813	33.76%	5.036%
6	5.735	1345	1367	1384	rBV3	135459	357095	70.16%	10.466%
7	6.256	1515	1529	1549	rBV	122461	229966	45.19%	6.740%
8	6.552	1610	1621	1630	rVB7	7021	12718	2.50%	0.373%
9	6.700	1654	1667	1682	rBV2	89245	170995	33.60%	5.012%
10	7.571	1926	1938	1956	rVB	39531	69921	13.74%	2.049%
11	7.906	2029	2042	2059	rBV	149826	253471	49.80%	7.429%
12	8.186	2114	2129	2142	rBV	25964	43172	8.48%	1.265%
13	8.478	2208	2220	2233	rBV2	3050	5299	1.04%	0.155%
14	8.558	2233	2245	2259	rBV	149303	254914	50.09%	7.471%
15	8.645	2259	2272	2302	rBV2	259030	508940	100.00%	14.917%
16	9.423	2502	2514	2529	rBV	181772	302614	59.46%	8.869%
17	10.764	2919	2931	2945	rVB2	73375	116421	22.88%	3.412%
18	10.896	2964	2972	2980	rBV5	3584	5494	1.08%	0.161%
19	11.819	3248	3259	3276	rBV	175383	271895	53.42%	7.969%
20	12.198	3364	3377	3392	rBV	155427	247803	48.69%	7.263%




Sum of corrected areas: 3411926

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042221\
Data File : VU043282.D
Acq On : 22 Apr 2021 16:48
Operator : SY/MD
Sample : M2124-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4527

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

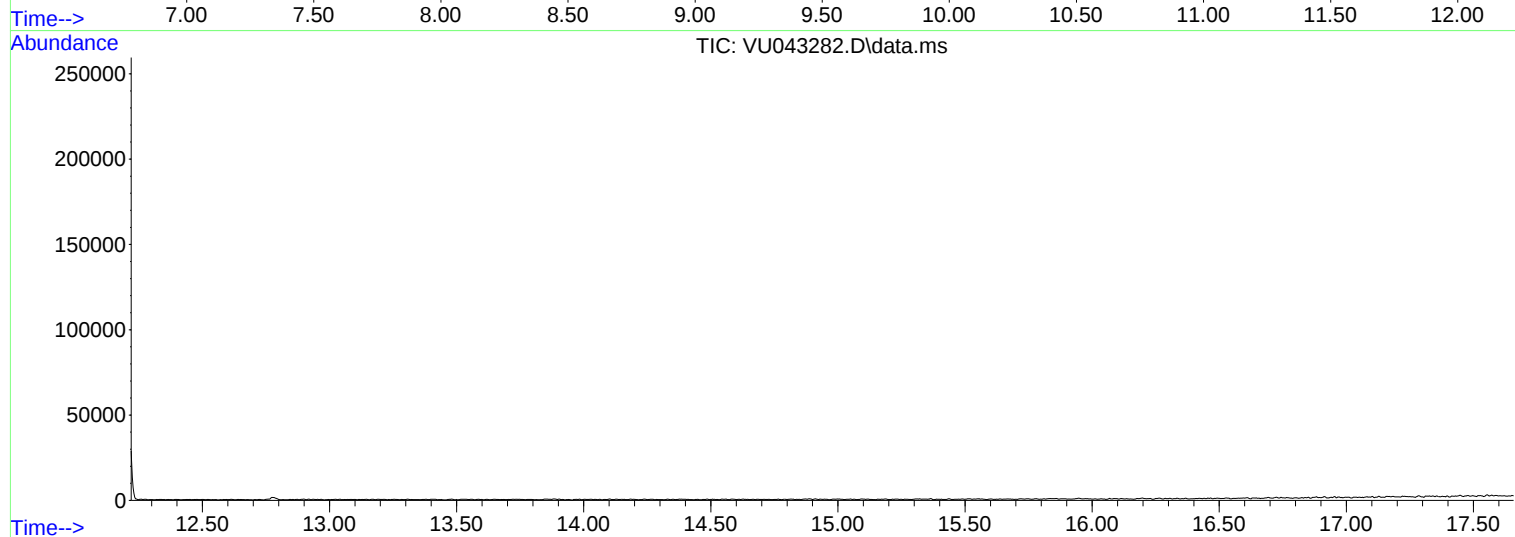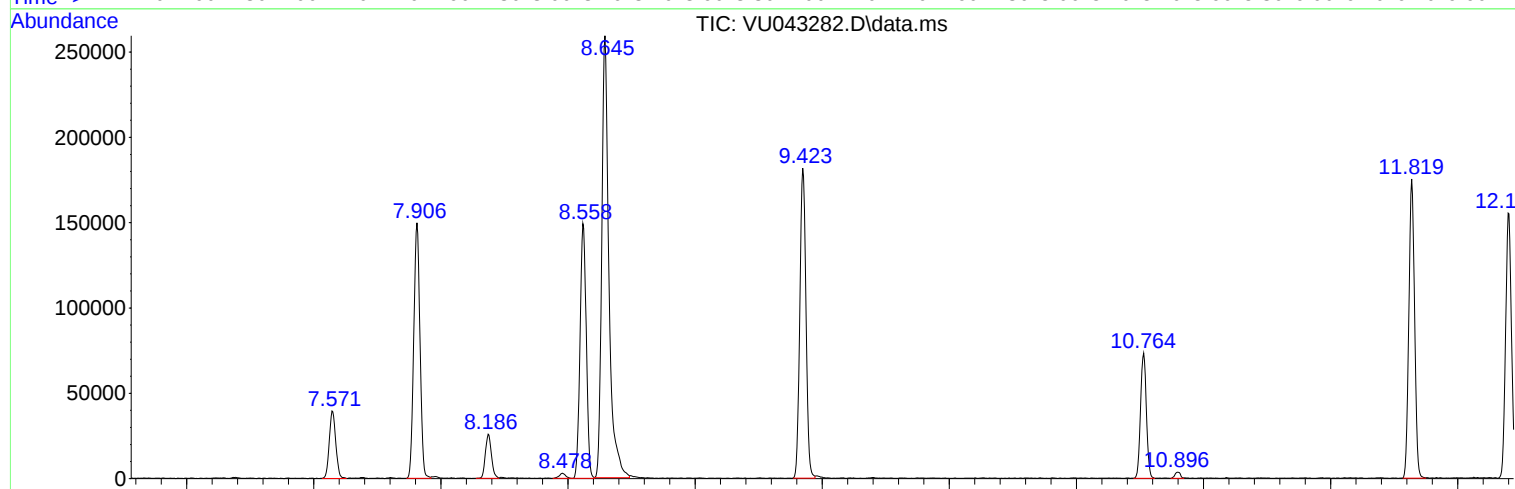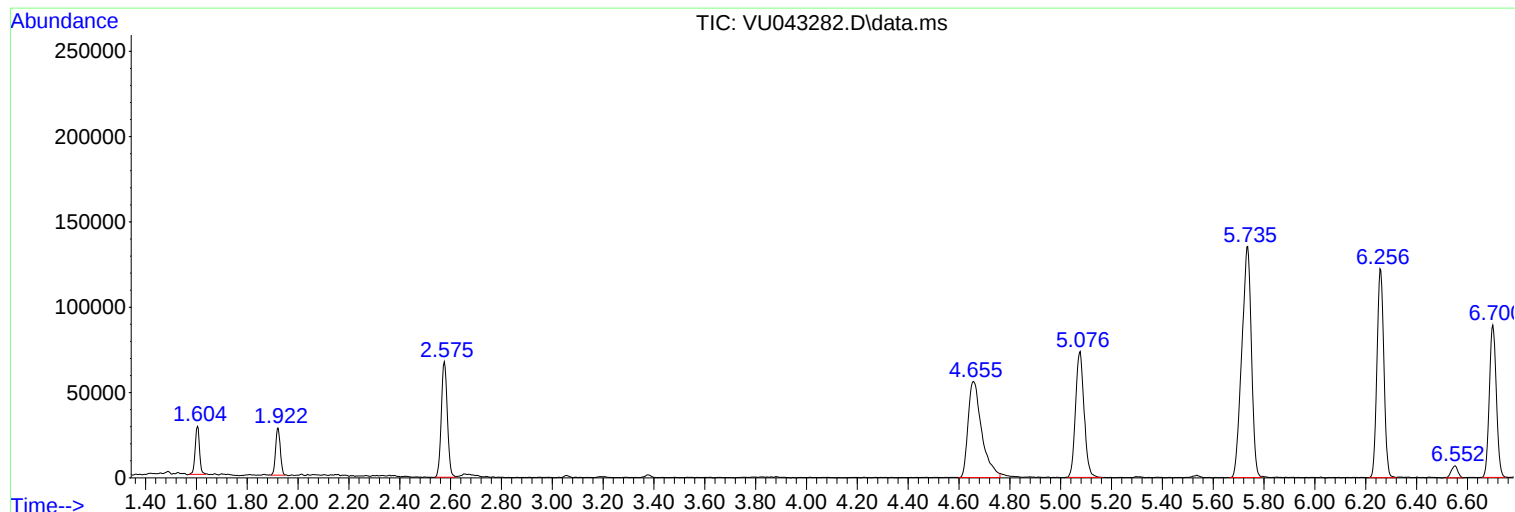

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042221\
Data File : VU043282.D
Acq On : 22 Apr 2021 16:48
Operator : SY/MD
Sample : M2124-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4527

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042221\
Data File : VU043282.D
Acq On : 22 Apr 2021 16:48
Operator : SY/MD
Sample : M2124-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4527

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
