


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042221\
Data File : VU043266.D
Acq On : 22 Apr 2021 09:09
Operator : SY/MD
Sample : BFB34
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB134

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 22 23:39:31 2021

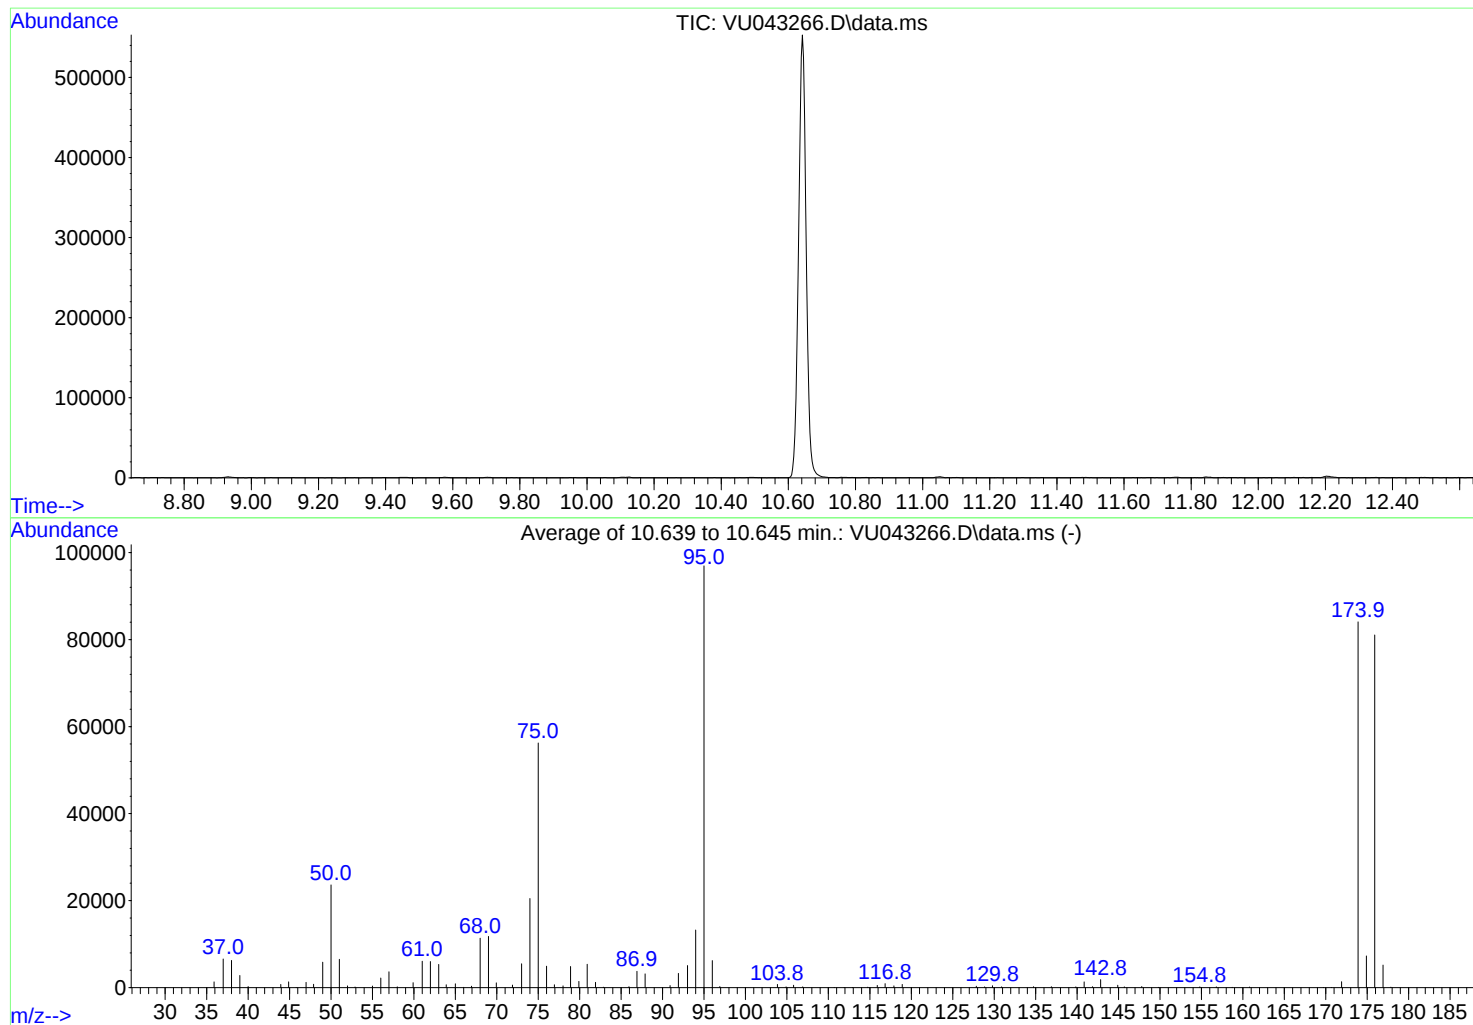

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.3	23600	PASS
75	95	30	80	58.0	56227	PASS
95	95	100	100	100.0	96952	PASS
96	95	5	9	6.4	6232	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.7	84083	PASS
175	174	5	9	8.7	7280	PASS
176	174	95	101	96.4	81059	PASS
177	176	5	9	6.4	5179	PASS

m/z	Abundance
43.90	211.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1410.0
37.00	6723.0
38.00	6074.0
39.00	2789.0
40.00	227.0
44.00	959.0
44.90	1308.0
45.80	105.0
47.00	1351.0
47.90	856.0
49.00	5993.0
50.00	23512.0
51.00	6193.0
52.00	333.0
52.90	148.0
55.00	453.0
56.00	2220.0
57.00	3758.0
58.00	155.0
59.90	1094.0
61.00	6094.0
62.00	5993.0
63.00	5310.0
63.90	704.0
65.00	924.0
66.00	143.0
67.00	283.0
68.00	11078.0
69.00	11714.0
69.90	1078.0
71.90	705.0
73.00	5490.0
74.00	20424.0
75.00	56184.0
76.00	5084.0
76.90	573.0
78.00	457.0
78.90	4876.0
79.90	1402.0
80.90	5372.0
81.90	1237.0
86.00	220.0
86.90	3923.0
87.90	3337.0
90.90	508.0
91.90	3270.0
93.00	5194.0
94.00	12971.0
95.00	95688.0
96.00	6330.0
96.90	284.0
103.80	729.0
104.90	229.0
105.80	551.0
106.90	186.0
110.70	106.0
112.90	100.0
114.70	136.0
115.90	485.0
116.90	851.0
117.90	334.0
118.90	681.0
127.80	311.0
128.90	204.0
129.80	441.0
130.90	150.0
134.80	257.0
136.90	206.0
139.80	165.0
140.90	1364.0
141.80	210.0
142.90	1721.0
144.90	538.0
145.70	198.0
147.80	232.0
154.80	190.0
156.80	173.0
160.80	115.0
171.90	1445.0
173.90	80360.0
174.90	7174.0
175.90	77584.0
176.90	5076.0
177.90	130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1399.0
37.00	6689.0
38.00	6465.0
39.00	2860.0
40.00	271.0
44.00	982.0
44.90	1386.0
47.00	1270.0
47.90	789.0
49.00	6120.0
50.00	24456.0
51.00	6695.0
52.00	459.0
52.90	173.0
55.00	402.0
56.00	2286.0
57.00	3756.0
58.00	201.0
59.90	1214.0
61.00	6258.0
62.00	6158.0
63.00	5558.0
63.90	670.0
65.00	873.0
66.00	110.0
67.00	340.0
68.00	11826.0
69.00	12171.0
69.90	1129.0
71.90	588.0
73.00	5660.0
74.00	21208.0
75.00	58424.0
76.00	5066.0
77.00	695.0
78.00	414.0
78.90	5003.0
79.90	1482.0
80.90	5546.0
81.90	1249.0
82.80	134.0
86.00	222.0
86.90	3915.0
87.90	3207.0
90.90	503.0
91.90	3341.0
93.00	5221.0
94.00	13820.0
95.00	100312.0
96.00	6417.0
96.90	274.0
103.90	760.0
104.90	197.0
105.80	593.0
106.90	196.0
114.70	111.0
115.90	548.0
116.80	949.0
117.90	441.0
118.90	799.0
127.90	326.0
128.90	197.0
129.80	457.0
130.90	196.0
134.70	227.0
136.90	247.0
139.80	174.0
140.90	1345.0
141.90	234.0
142.90	1903.0
144.90	599.0
145.70	194.0
147.80	262.0
149.80	114.0
154.80	193.0
156.80	193.0
158.70	115.0
160.80	161.0
171.90	1425.0
173.90	86976.0
174.90	7541.0
175.90	84024.0
176.90	5406.0
177.90	128.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134

m/z	Abundance
35.90	1192.0
37.00	6383.0
38.00	6175.0
39.00	2717.0
40.00	267.0
44.00	937.0
44.90	1265.0
47.00	989.0
47.90	702.0
49.00	5458.0
50.00	22832.0
51.00	6695.0
52.00	472.0
52.90	144.0
55.00	303.0
56.00	2111.0
57.00	3368.0
58.00	177.0
59.90	1164.0
61.00	5827.0
62.00	5878.0
63.00	5180.0
63.90	609.0
65.00	813.0
66.90	351.0
68.00	11194.0
69.00	11386.0
70.00	1073.0
71.90	470.0
73.00	5287.0
74.00	19816.0
75.00	54072.0
76.00	4679.0
76.90	704.0
78.00	338.0
78.90	4726.0
79.90	1445.0
80.90	5164.0
81.90	1167.0
82.90	159.0
85.90	183.0
86.90	3447.0
87.90	3004.0
90.90	421.0
91.90	3266.0
93.00	4810.0
94.00	12955.0
95.00	94856.0
96.00	5948.0
96.90	191.0
103.90	686.0
104.90	133.0
105.80	537.0
106.90	178.0
111.90	103.0
114.80	114.0
115.90	514.0
116.80	930.0
117.90	480.0
118.90	784.0
127.90	368.0
128.70	181.0
129.80	402.0
130.90	197.0
134.70	185.0
136.90	249.0
139.90	173.0
140.80	1238.0
141.90	186.0
142.80	1895.0
144.90	510.0
145.70	174.0
147.80	257.0
149.80	117.0
154.80	201.0
156.80	194.0
158.70	119.0
160.80	163.0
169.70	110.0
170.70	160.0
171.90	1238.0
173.90	84912.0
174.90	7125.0
175.90	81568.0
176.90	5054.0
177.80	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB134