
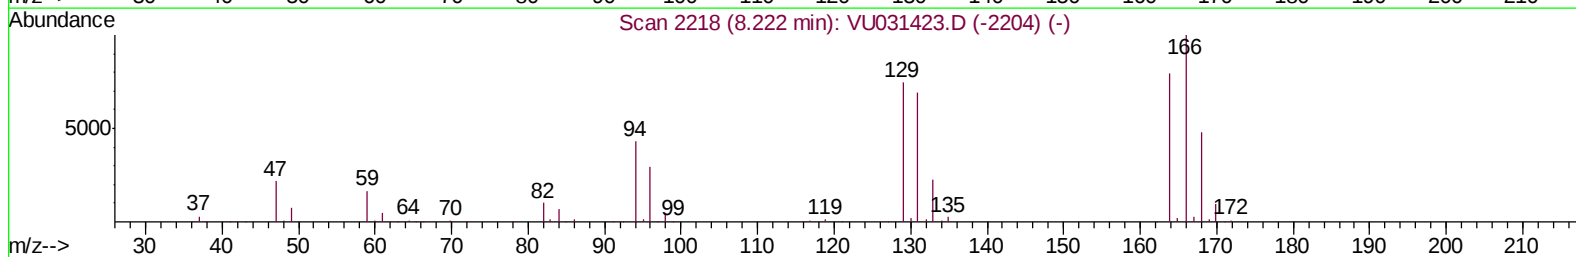
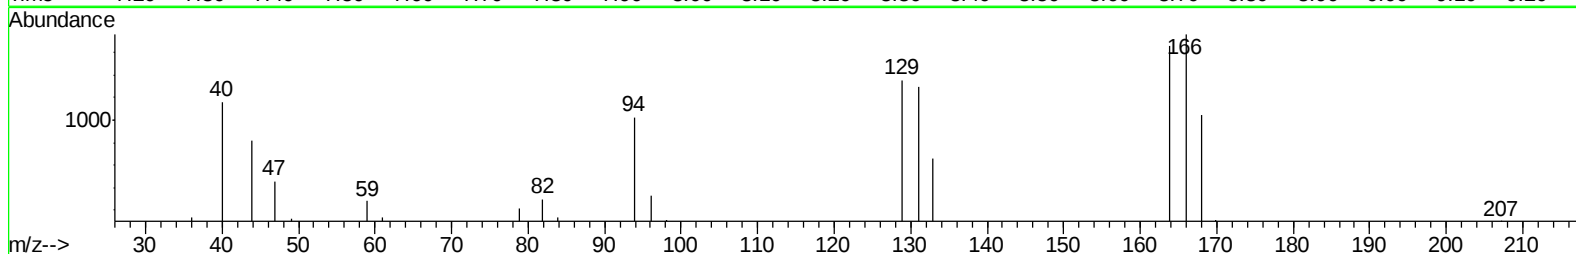


Data File : VU031427.D
Acq On : 23 Apr 2019 10:57
Operator : JC/SP
Sample : K2478-07DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Quant Time: Apr 24 06:03:39 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

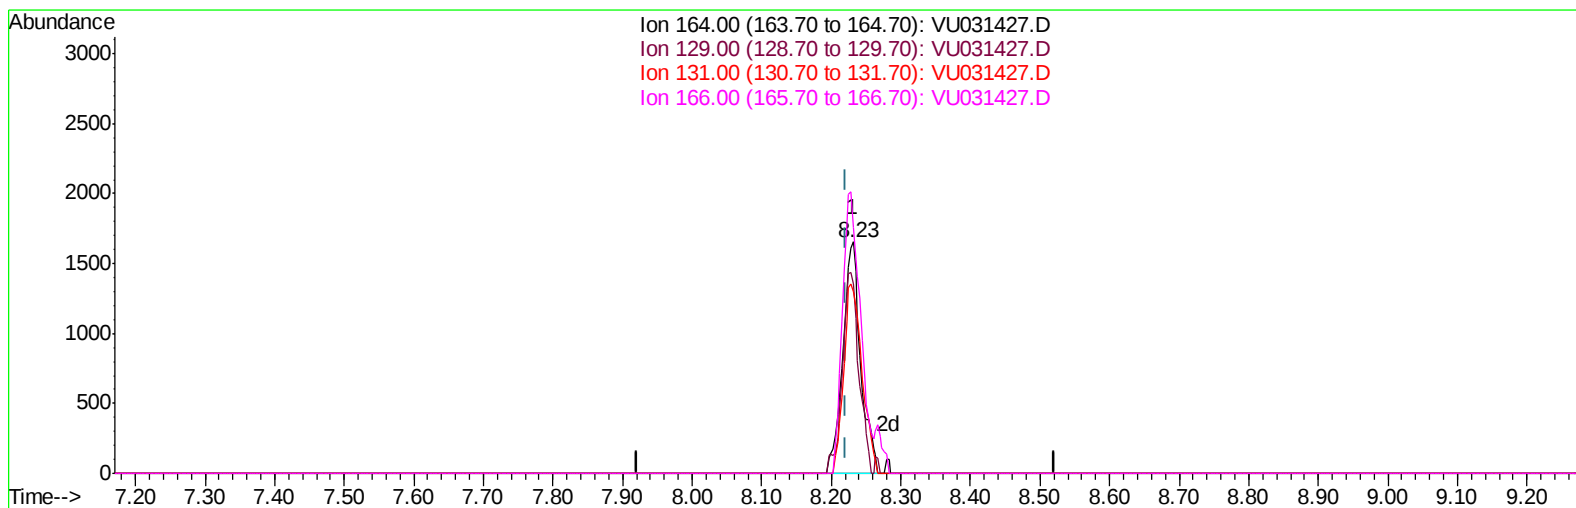

TIC: VU031427.D

(46) Tetrachloroethene (T)

8.231min (+0.010) 0.87ug/L m

response 2931

Ion	Exp%	Act%
164.00	100	100
129.00	93.10	81.70
131.00	87.70	78.20
166.00	127.40	106.34