
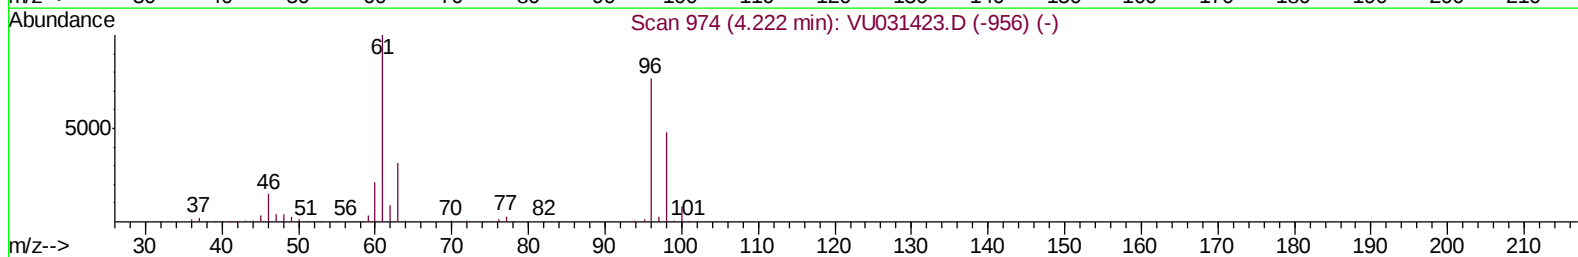
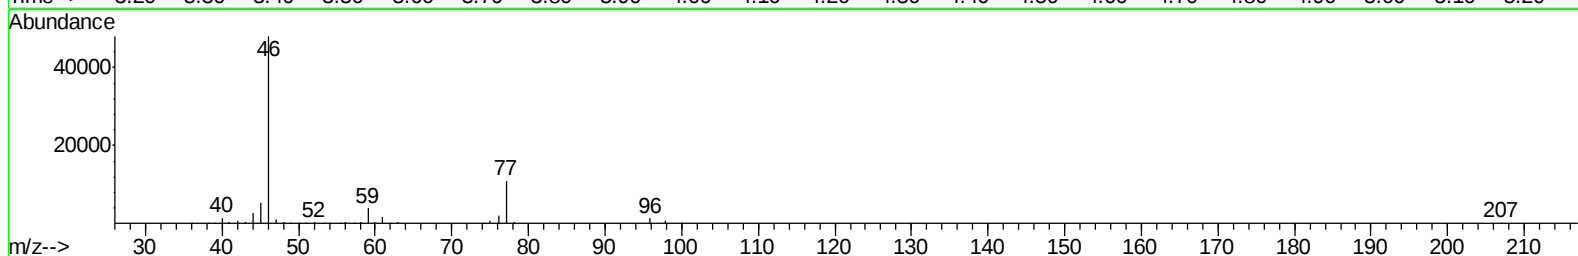


Data File : VU031441.D
Acq On : 23 Apr 2019 16:22
Operator : JC/SP
Sample : K2536-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Apr 24 06:05:34 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

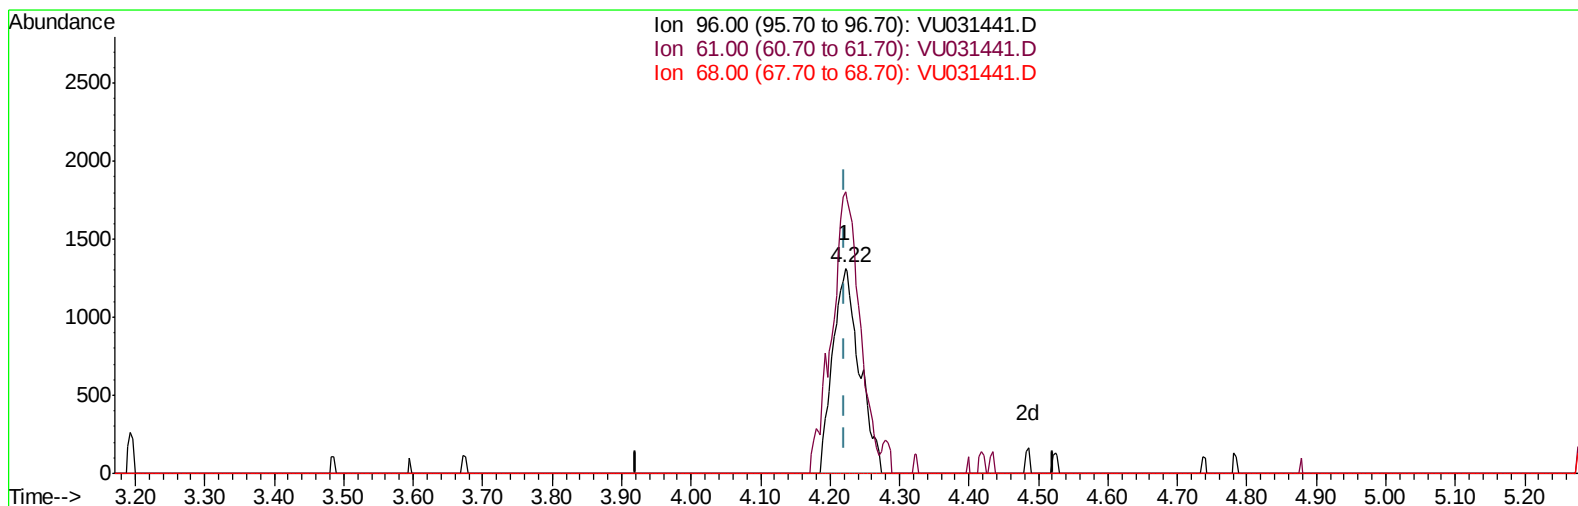

TIC: VU031441.D

(20) cis-1,2-Dichloroethene (T)

4.222min (0.000) 0.68ug/L m

response 3479

Ion	Exp%	Act%
96.00	100	100
61.00	131.30	137.29
68.00	0.00	0.00
0.00	0.00	0.00