
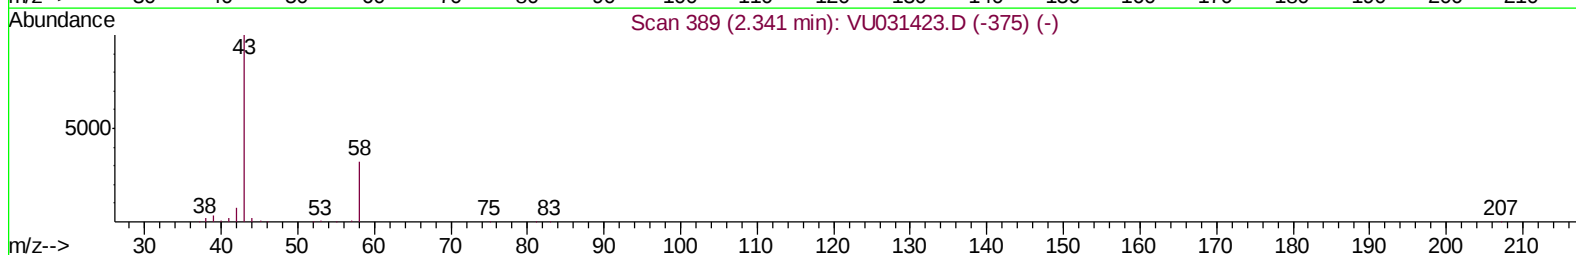
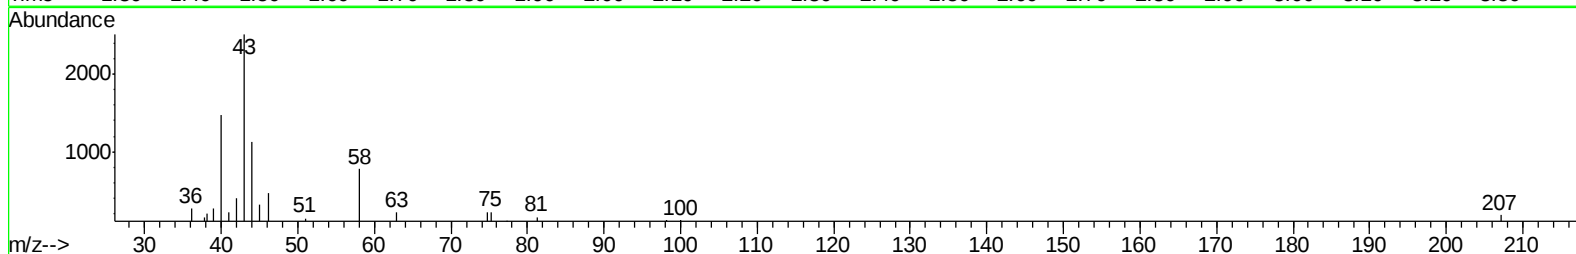


Data File : VU031443.D
Acq On : 23 Apr 2019 17:09
Operator : JC/SP
Sample : K2536-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Apr 24 06:05:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

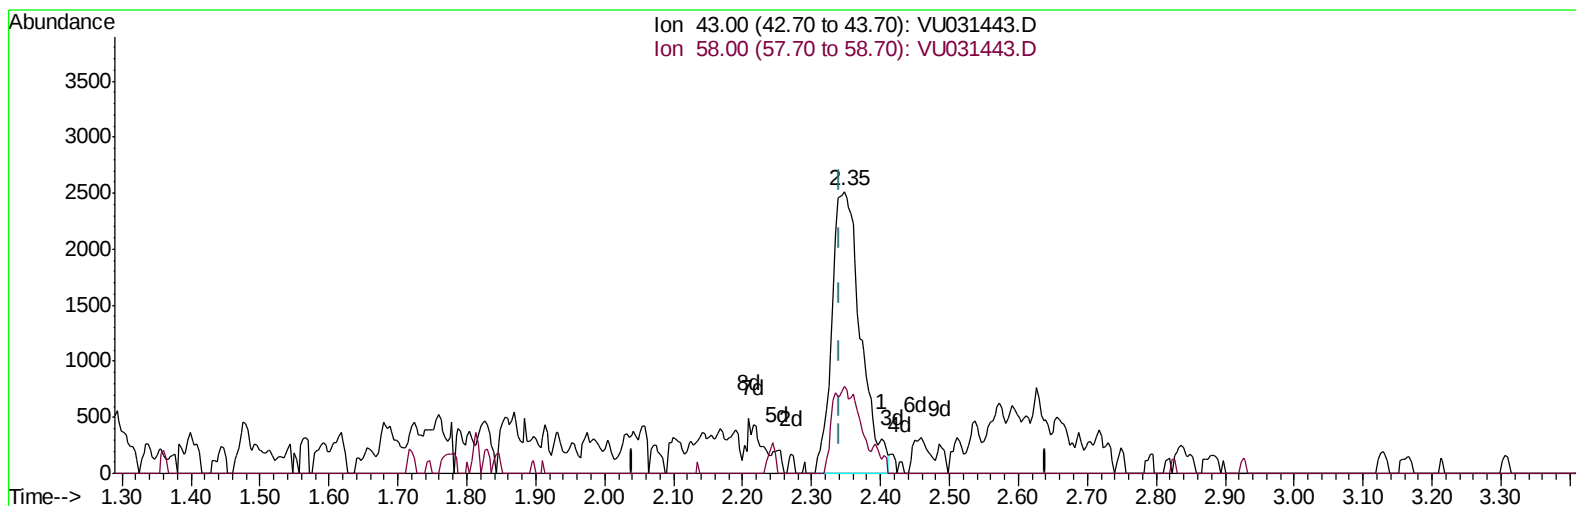

TIC: VU031443.D

(13) Acetone (T)

2.347min (+0.006) 2.01ug/L m

response 7306

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	0.77
0.00	0.00	0.00
0.00	0.00	0.00