
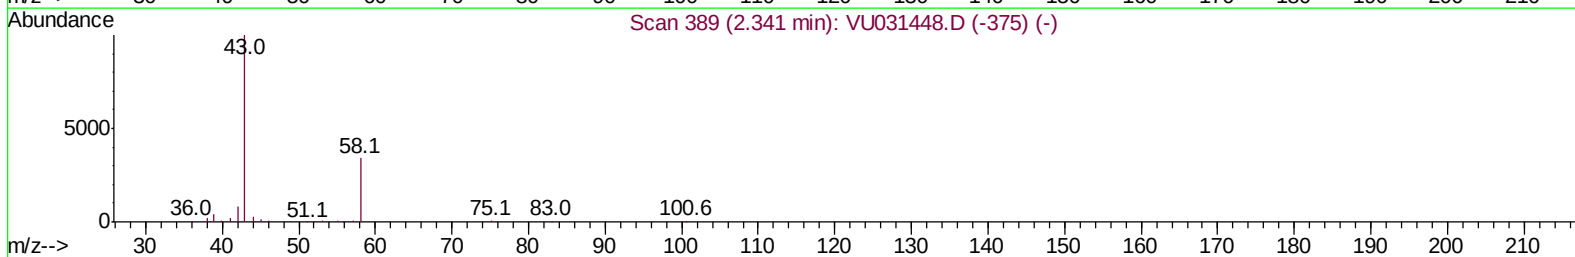
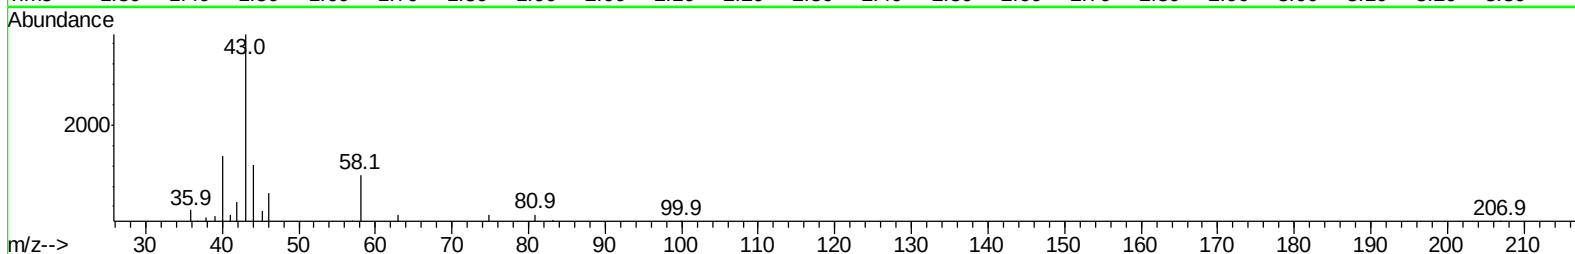


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031453.D
Acq On : 23 Apr 2019 21:49
Operator : JC/SP
Sample : K2536-04DL 4X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 24 08:45:00 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 08:41:52 2019
Response via : Initial Calibration

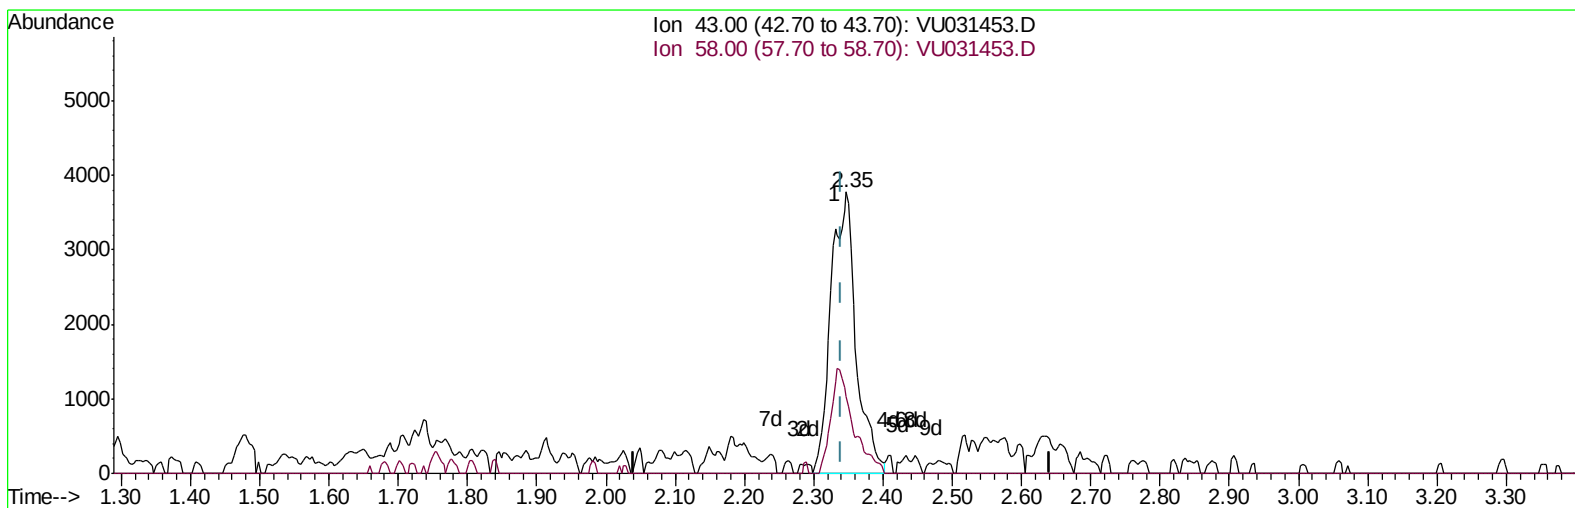

TIC: VU031453.D

(13) Acetone (T)

2.347min (+0.007) 2.78ug/L m

response 9420

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	26.96
0.00	0.00	0.00
0.00	0.00	0.00