

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Quantitation Report (QT Reviewed)


Data File : VU031443.D
Acq On : 23 Apr 2019 17:09
Operator : JC/SP
Sample : K2536-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X21DL

Manual Integrations
APPROVED

MMDadoda
4/24/2019 10:46:32 AM

Quant Time: Apr 24 08:15:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

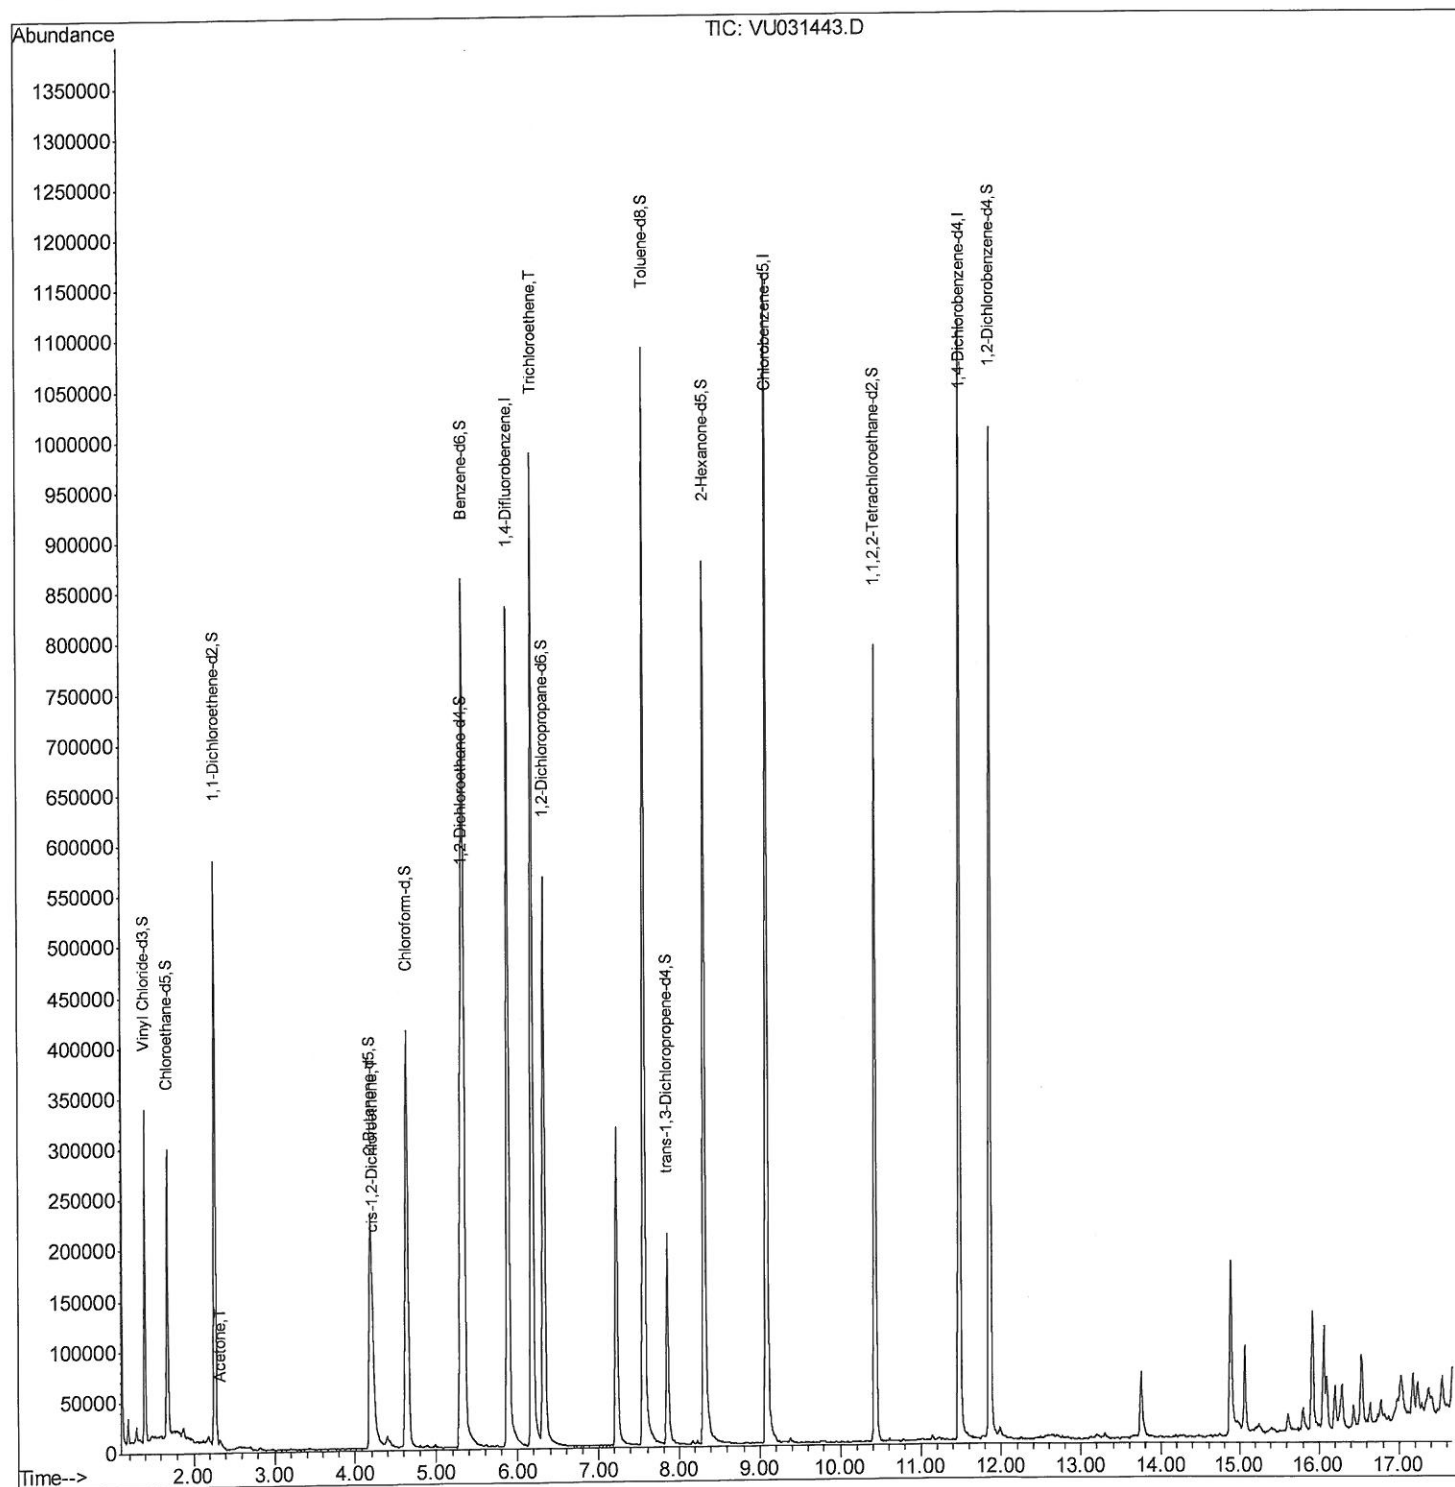

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Quantitation Report (Qedit)




Data File : VU031443.D
Acq On : 23 Apr 2019 17:09
Operator : JC/SP
Sample : K2536-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X21DL

Manual Integrations
APPROVED

MMDadoda
4/24/2019 10:46:32 AM

Quant Time: Apr 24 06:05:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

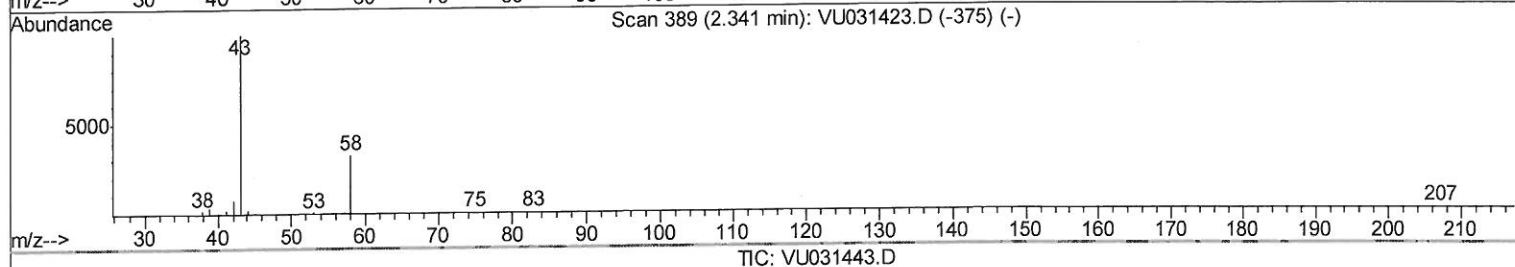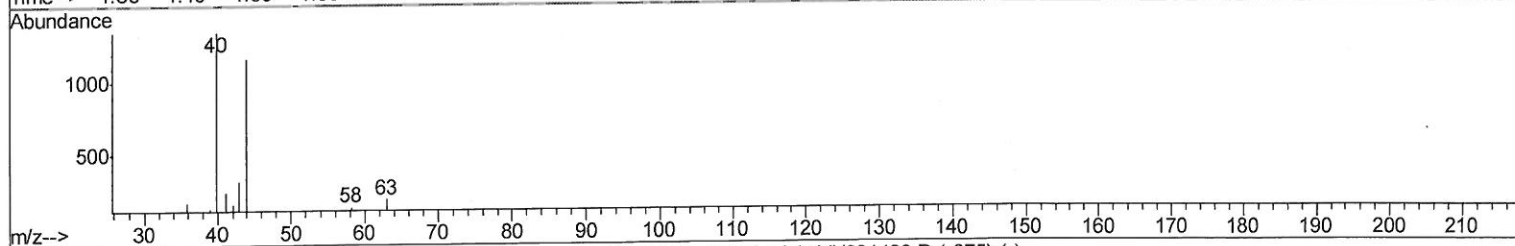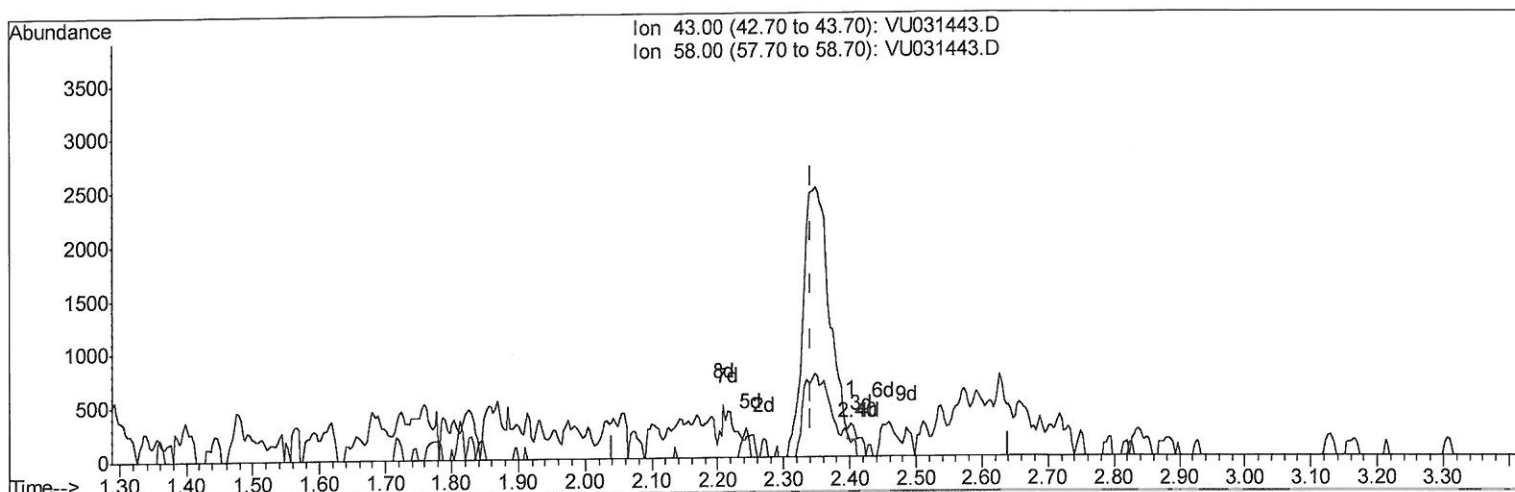

(13) Acetone (T)
2.402min (+0.061) 0.02ug/L
response 87

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	64.37
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Quantitation Report (Qedit)




Data File : VU031443.D
Acq On : 23 Apr 2019 17:09
Operator : JC/SP
Sample : K2536-01DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X21DL

Manual Integrations
APPROVED

MMDadoda
4/24/2019 10:46:32 AM

Quant Time: Apr 24 06:05:49 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Apr 24 06:00:22 2019
Response via : Initial Calibration

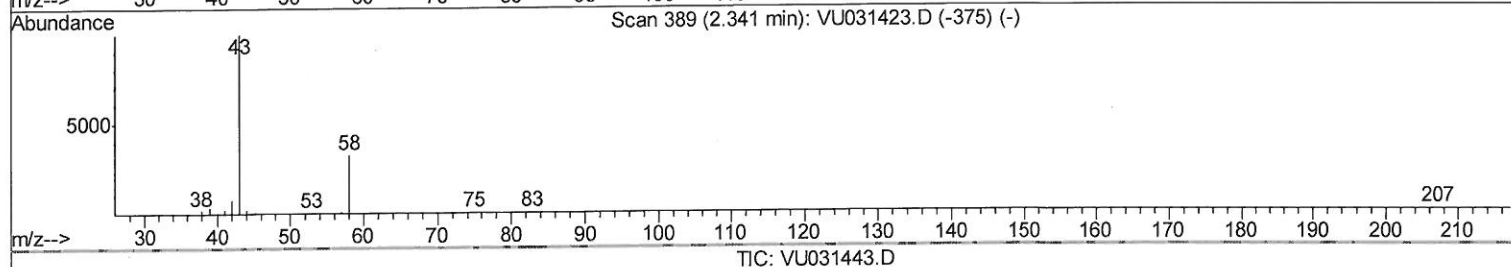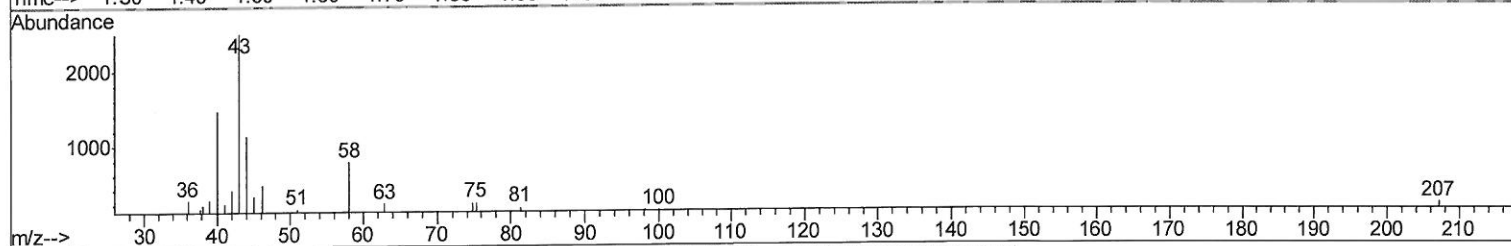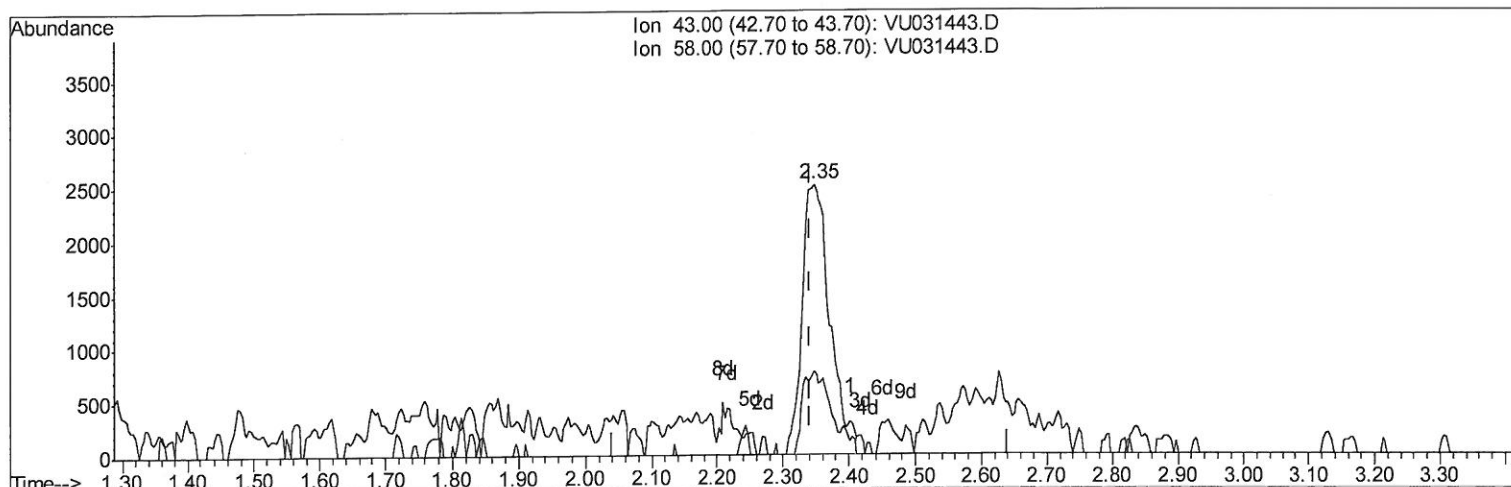

(13) Acetone (T)

2.347min (+0.006) 2.01ug/L m

response 7306

Ion	Exp%	Act%
43.00	100	100
58.00	33.20	0.77
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
 Quantitation Report (QT Reviewed)

Data File : VU031443.D
 Acq On : 23 Apr 2019 17:09
 Operator : JC/SP
 Sample : K2536-01DL 5X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X21DL

Manual Integrations
 APPROVED

MMDadoda
 4/24/2019 10:46:32 AM

Quant Time: Apr 24 08:15:37 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Apr 24 06:00:22 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	763747	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	683186	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	306932	50.00	ug/L	0.00

System Monitoring Compounds						
4) Vinyl Chloride-d3	1.40	65	229055	37.01	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	74.02%		
7) Chloroethane-d5	1.68	69	195608	41.51	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.02%		
11) 1,1-Dichloroethene-d2	2.27	63	332712	30.90	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	61.80%		
21) 2-Butanone-d5	4.19	46	467898	101.13	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.13%		
24) Chloroform-d	4.64	84	415152	42.10	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	84.20%		
26) 1,2-Dichloroethane-d4	5.31	65	266802	45.16	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.32%		
32) Benzene-d6	5.34	84	891891	45.19	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.38%		
36) 1,2-Dichloropropane-d6	6.33	67	304896	48.01	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	96.02%		
41) Toluene-d8	7.56	98	783409	44.44	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.88%		
43) trans-1,3-Dichloropropene-	7.85	79	130318	45.03	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.06%		
47) 2-Hexanone-d5	8.31	63	336139	105.64	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.64%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	410003	47.59	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	95.18%		
64) 1,2-Dichlorobenzene-d4	11.86	152	283208	45.14	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.28%		

Target Compounds						Qvalue
13) Acetone	2.35	43	7306m	2.011	ug/L	88
20) cis-1,2-Dichloroethene	4.23	96	17818	3.272	ug/L	98
34) Trichloroethene	6.18	95	361141	68.971	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed