

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031405.D
 Acq On : 22 Apr 2019 21:43
 Operator : JC/SP
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rVB3	16655	15510	0.59%	0.078%
2	1.396	87	95	109	rBV	402022	435658	16.47%	2.186%
3	1.682	176	184	197	rBV	309632	391073	14.78%	1.962%
4	2.270	355	367	380	rBV	658261	1015770	38.40%	5.096%
5	2.441	417	420	422	rBV3	715	513	0.02%	0.003%
6	2.473	422	430	439	rVB4	3560	6108	0.23%	0.031%
7	2.534	445	449	451	rBV2	794	749	0.03%	0.004%
8	2.698	491	500	510	rBV6	3183	5318	0.20%	0.027%
9	2.981	582	588	592	rVV6	988	1213	0.05%	0.006%
10	3.026	598	602	607	rBV2	842	805	0.03%	0.004%
11	3.277	676	680	683	rBV2	703	637	0.02%	0.003%
12	3.347	698	702	707	rBV3	552	525	0.02%	0.003%
13	3.588	772	777	780	rBV4	934	929	0.04%	0.005%
14	3.624	785	788	793	rVB3	1316	1066	0.04%	0.005%
15	3.682	799	806	808	rBV3	837	1065	0.04%	0.005%
16	3.698	808	811	814	rVB2	841	627	0.02%	0.003%
17	3.810	844	846	852	rVV2	846	675	0.03%	0.003%
18	3.849	852	858	863	rVV4	675	705	0.03%	0.004%
19	4.186	951	963	996	rBV	211407	673470	25.46%	3.379%
20	4.527	1066	1069	1071	rBV3	924	616	0.02%	0.003%
21	4.643	1088	1105	1132	rBV	418242	997551	37.71%	5.004%
22	4.878	1172	1178	1180	rBV4	1356	1566	0.06%	0.008%
23	4.981	1203	1210	1211	rBV3	2443	2120	0.08%	0.011%
24	5.100	1240	1247	1249	rBV3	515	632	0.02%	0.003%
25	5.125	1251	1255	1258	rVV4	817	650	0.02%	0.003%
26	5.215	1278	1283	1286	rBV4	1361	1449	0.05%	0.007%
27	5.334	1297	1320	1353	rBV3	887290	2645501	100.00%	13.272%
28	5.637	1409	1414	1417	rVB6	1039	815	0.03%	0.004%
29	5.666	1420	1423	1425	rBV2	1165	741	0.03%	0.004%
30	5.749	1442	1449	1451	rBV2	955	893	0.03%	0.004%
31	5.881	1476	1490	1519	rBV	761405	1566873	59.23%	7.860%
32	6.090	1552	1555	1557	rBV3	1192	948	0.04%	0.005%
33	6.180	1573	1583	1598	rVB3	10335	26265	0.99%	0.132%
34	6.247	1602	1604	1608	rVB4	837	509	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031405.D
 Acq On : 22 Apr 2019 21:43
 Operator : JC/SP
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	6.270	1608	1611	1613	rBV2	737	514	0.02%	0.003%
36	6.325	1613	1628	1651	rBV	560681	1167496	44.13%	5.857%
37	6.495	1678	1681	1682	rBV3	959	575	0.02%	0.003%
38	6.559	1698	1701	1707	rVB4	1247	989	0.04%	0.005%
39	6.656	1727	1731	1737	rVB4	1275	1323	0.05%	0.007%
40	6.685	1737	1740	1744	rBV2	629	560	0.02%	0.003%
41	6.743	1755	1758	1763	rVB3	1001	850	0.03%	0.004%
42	7.064	1856	1858	1863	rVB2	699	537	0.02%	0.003%
43	7.128	1872	1878	1883	rBV4	648	628	0.02%	0.003%
44	7.225	1895	1908	1931	rBV	306635	588596	22.25%	2.953%
45	7.428	1968	1971	1975	rVB4	1068	896	0.03%	0.004%
46	7.450	1975	1978	1981	rVV3	859	610	0.02%	0.003%
47	7.469	1981	1984	1988	rVB3	1059	778	0.03%	0.004%
48	7.563	1999	2013	2035	rBV	1158838	2080004	78.62%	10.435%
49	7.849	2090	2102	2126	rBV	204471	387739	14.66%	1.945%
50	7.984	2142	2144	2147	rVB3	1090	592	0.02%	0.003%
51	8.000	2147	2149	2156	rVB3	871	786	0.03%	0.004%
52	8.087	2174	2176	2180	rVB4	967	715	0.03%	0.004%
53	8.228	2214	2220	2227	rBV9	2173	3326	0.13%	0.017%
54	8.312	2234	2246	2283	rBV	810107	1528519	57.78%	7.668%
55	8.624	2340	2343	2346	rVB2	862	560	0.02%	0.003%
56	8.768	2385	2388	2391	rBV3	699	551	0.02%	0.003%
57	8.845	2409	2412	2414	rBV3	1256	875	0.03%	0.004%
58	8.977	2451	2453	2458	rVB2	757	651	0.02%	0.003%
59	9.006	2458	2462	2466	rBV4	962	723	0.03%	0.004%
60	9.087	2473	2487	2515	rBV	1068345	1849344	69.91%	9.278%
61	9.325	2558	2561	2563	rBV2	953	541	0.02%	0.003%
62	9.363	2571	2573	2575	rBV	1298	819	0.03%	0.004%
63	9.437	2593	2596	2600	rBV2	1292	1154	0.04%	0.006%
64	9.495	2610	2614	2616	rBV2	959	722	0.03%	0.004%
65	9.553	2628	2632	2633	rBV3	906	607	0.02%	0.003%
66	9.701	2675	2678	2681	rVB	886	562	0.02%	0.003%
67	9.720	2681	2684	2689	rBV2	890	1039	0.04%	0.005%
68	9.759	2694	2696	2700	rBV2	681	521	0.02%	0.003%
69	9.791	2700	2706	2711	rBV5	1538	2226	0.08%	0.011%
70	9.971	2756	2762	2764	rBV2	696	701	0.03%	0.004%
71	10.093	2796	2800	2805	rVB3	1159	1044	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031405.D
 Acq On : 22 Apr 2019 21:43
 Operator : JC/SP
 Sample : VU0423WBL01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.132	2805	2812	2817	rBV3	1118	1644	0.06%	0.008%
73	10.167	2818	2823	2827	rBV5	1115	1206	0.05%	0.006%
74	10.241	2843	2846	2851	rBV3	1123	813	0.03%	0.004%
75	10.263	2851	2853	2858	rVB3	796	512	0.02%	0.003%
76	10.427	2889	2904	2925	rBV	775904	1263695	47.77%	6.340%
77	10.591	2952	2955	2960	rVB2	1576	1514	0.06%	0.008%
78	10.736	2996	3000	3004	rBV4	789	659	0.02%	0.003%
79	10.868	3039	3041	3043	rBV2	944	565	0.02%	0.003%
80	10.996	3079	3081	3087	rVB3	720	596	0.02%	0.003%
81	11.212	3143	3148	3151	rBV3	1040	1114	0.04%	0.006%
82	11.331	3183	3185	3189	rVB2	725	537	0.02%	0.003%
83	11.411	3207	3210	3211	rBV2	1762	1001	0.04%	0.005%
84	11.479	3220	3231	3254	rBV	953354	1563763	59.11%	7.845%
85	11.855	3336	3348	3368	rBV	985585	1653590	62.51%	8.296%
86	12.279	3477	3480	3485	rVB3	890	819	0.03%	0.004%
87	12.427	3524	3526	3529	rBV2	806	565	0.02%	0.003%
88	12.479	3540	3542	3545	rBV3	982	675	0.03%	0.003%
89	12.771	3630	3633	3635	rBV2	779	624	0.02%	0.003%
90	13.048	3715	3719	3722	rBV3	953	946	0.04%	0.005%
91	13.199	3763	3766	3768	rVB2	1057	538	0.02%	0.003%
92	13.244	3777	3780	3783	rBV2	980	827	0.03%	0.004%
93	13.730	3926	3931	3935	rBV4	938	1261	0.05%	0.006%
94	14.090	4041	4043	4046	rBV2	908	561	0.02%	0.003%
95	14.238	4087	4089	4092	rVB	975	527	0.02%	0.003%
96	14.289	4102	4105	4109	rBV3	1446	1198	0.05%	0.006%
97	14.791	4258	4261	4266	rBV4	1758	1602	0.06%	0.008%
98	14.945	4305	4309	4311	rBV2	1581	1147	0.04%	0.006%
99	15.160	4371	4376	4379	rBV4	1924	1676	0.06%	0.008%
100	15.456	4466	4468	4472	rBV4	1311	1140	0.04%	0.006%


Sum of corrected areas: 19933533

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031405.D
Acq On : 22 Apr 2019 21:43
Operator : JC/SP
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

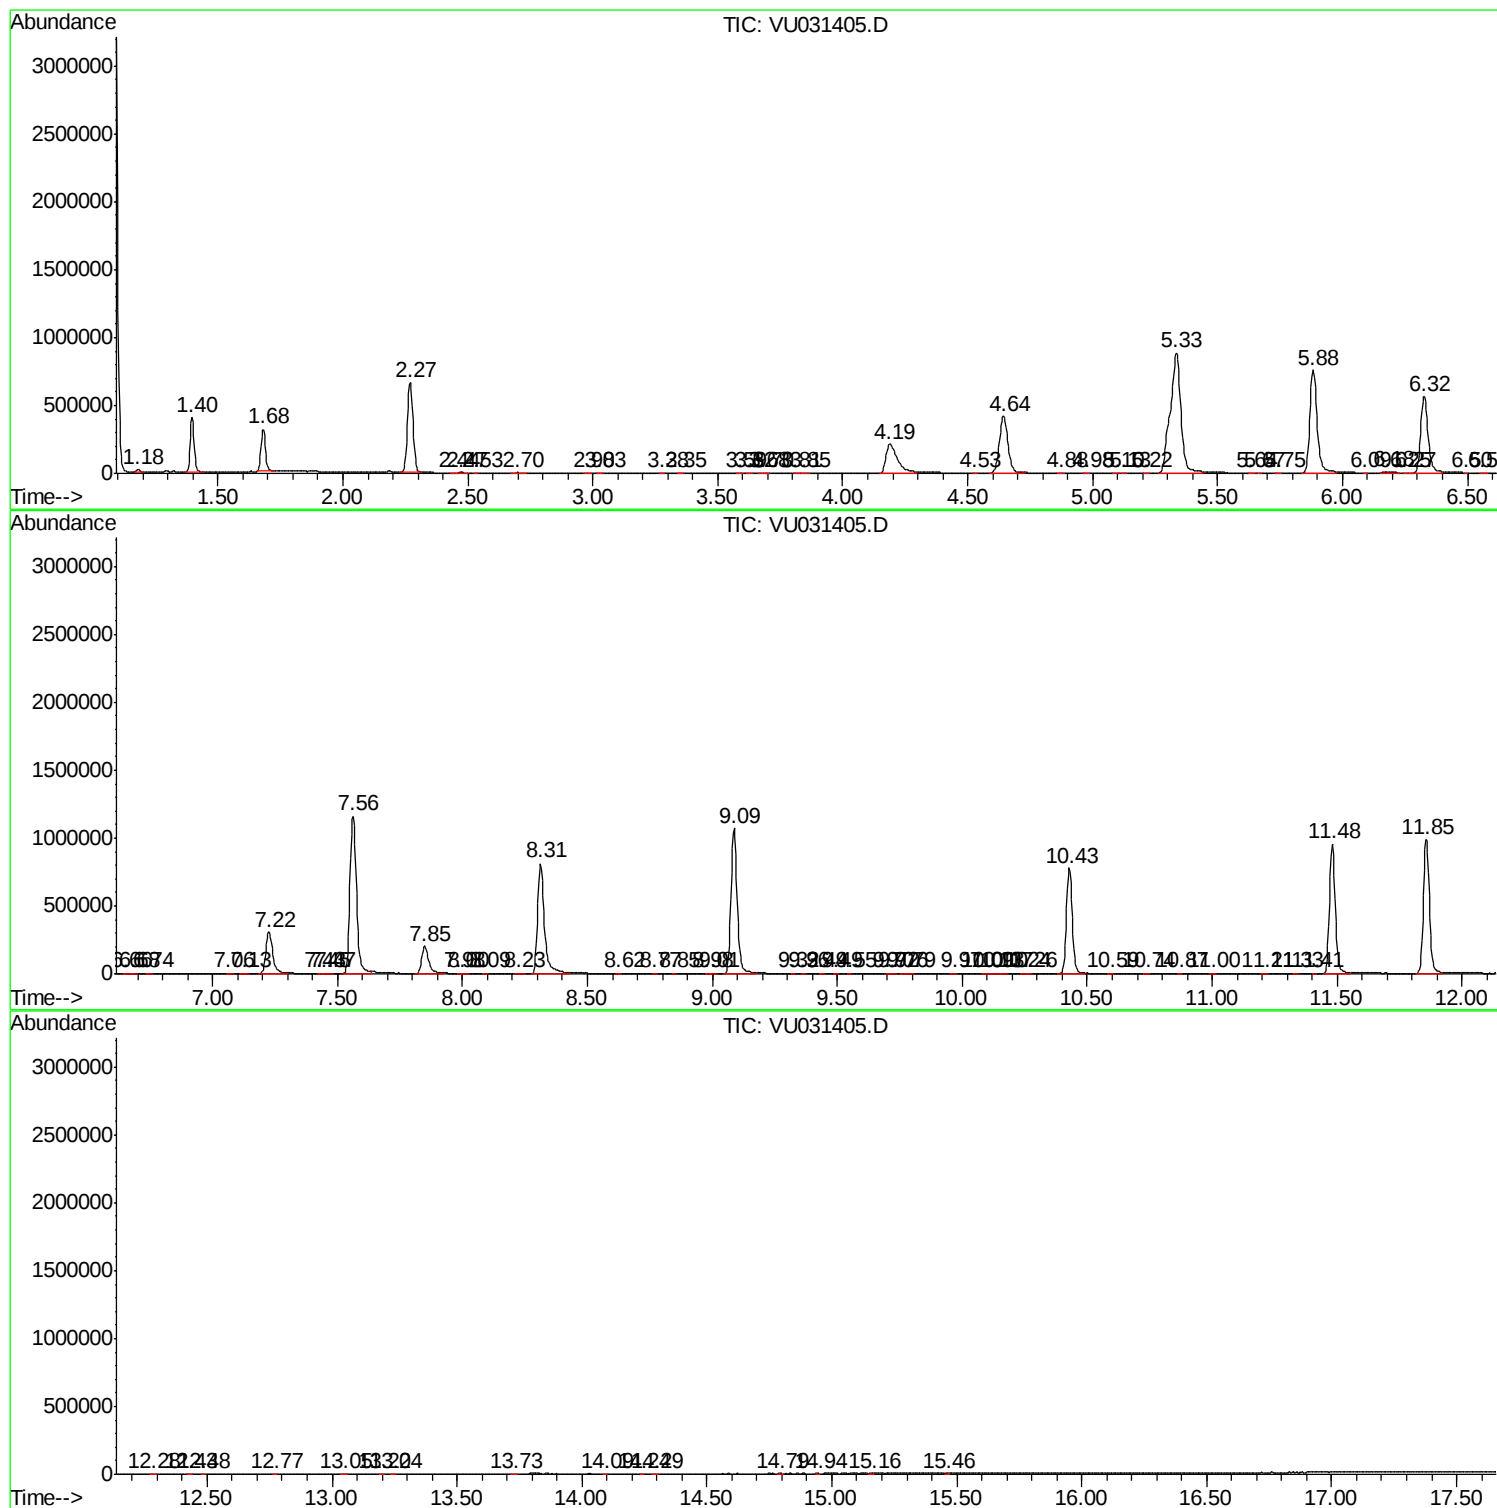

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031405.D
Acq On : 22 Apr 2019 21:43
Operator : JC/SP
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031405.D
Acq On : 22 Apr 2019 21:43
Operator : JC/SP
Sample : VU0423WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc