

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031407.D
 Acq On : 22 Apr 2019 22:29
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB	16602	16168	0.67%	0.081%
2	1.396	88	95	111	rVB	307050	340594	14.03%	1.704%
3	1.682	176	184	196	rBV	255516	326118	13.43%	1.632%
4	1.881	241	246	258	rVB2	29554	40582	1.67%	0.203%
5	2.267	356	366	381	rVB	557214	849491	34.99%	4.251%
6	2.640	479	482	485	rBV3	1214	835	0.03%	0.004%
7	2.701	492	501	504	rBV7	2614	3653	0.15%	0.018%
8	2.717	504	506	513	rVB6	1796	1431	0.06%	0.007%
9	2.836	535	543	547	rBV5	1412	2042	0.08%	0.010%
10	2.926	567	571	574	rBV3	964	737	0.03%	0.004%
11	3.196	652	655	659	rBV3	745	670	0.03%	0.003%
12	3.338	692	699	701	rBV3	595	742	0.03%	0.004%
13	3.457	726	736	740	rVB4	1060	1351	0.06%	0.007%
14	3.550	763	765	771	rVB3	652	467	0.02%	0.002%
15	3.585	771	776	778	rBV3	510	541	0.02%	0.003%
16	3.627	784	789	794	rVB4	752	827	0.03%	0.004%
17	3.662	794	800	801	rBV	730	649	0.03%	0.003%
18	3.711	809	815	818	rBV3	624	747	0.03%	0.004%
19	3.939	879	886	889	rBV2	579	545	0.02%	0.003%
20	4.077	925	929	934	rVB	1293	1023	0.04%	0.005%
21	4.190	948	964	991	rBV	214795	681361	28.06%	3.409%
22	4.643	1088	1105	1133	rBV2	394917	946711	38.99%	4.737%
23	4.842	1163	1167	1171	rBV2	879	894	0.04%	0.004%
24	4.878	1176	1178	1184	rVV5	1616	1917	0.08%	0.010%
25	4.916	1187	1190	1194	rVB4	820	613	0.03%	0.003%
26	4.955	1199	1202	1204	rBV3	925	650	0.03%	0.003%
27	4.984	1207	1211	1214	rVV3	1110	1096	0.05%	0.005%
28	5.000	1214	1216	1220	rVB3	1377	829	0.03%	0.004%
29	5.083	1237	1242	1246	rVB3	893	923	0.04%	0.005%
30	5.112	1246	1251	1252	rBV2	717	648	0.03%	0.003%
31	5.334	1297	1320	1351	rBV2	804297	2428133	100.00%	12.149%
32	5.665	1420	1423	1425	rBV3	1121	594	0.02%	0.003%
33	5.736	1442	1445	1449	rVB4	1112	759	0.03%	0.004%
34	5.884	1476	1491	1521	rBV	715509	1474724	60.73%	7.379%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031407.D
 Acq On : 22 Apr 2019 22:29
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	6.183	1568	1584	1615	rBV	657325	1343196	55.32%	6.721%
36	6.328	1616	1629	1650	rVV	526065	1071570	44.13%	5.362%
37	6.601	1707	1714	1717	rBV7	848	1040	0.04%	0.005%
38	6.633	1721	1724	1726	rVV3	734	543	0.02%	0.003%
39	6.820	1779	1782	1785	rVB	622	450	0.02%	0.002%
40	6.836	1785	1787	1791	rBV2	983	654	0.03%	0.003%
41	6.855	1791	1793	1796	rBV3	865	512	0.02%	0.003%
42	6.903	1800	1808	1811	rBV3	1253	1479	0.06%	0.007%
43	6.945	1819	1821	1825	rVB3	876	603	0.02%	0.003%
44	6.974	1825	1830	1832	rBV2	838	716	0.03%	0.004%
45	7.009	1836	1841	1847	rVB3	922	915	0.04%	0.005%
46	7.067	1851	1859	1863	rBV3	1305	1365	0.06%	0.007%
47	7.225	1895	1908	1933	rBV	278808	533561	21.97%	2.670%
48	7.437	1971	1974	1977	rBV3	871	542	0.02%	0.003%
49	7.562	1999	2013	2034	rBV	1023364	1867723	76.92%	9.345%
50	7.849	2091	2102	2132	rBV2	179063	346038	14.25%	1.731%
51	7.984	2142	2144	2148	rBV3	1085	585	0.02%	0.003%
52	8.225	2208	2219	2235	rBV2	101101	180771	7.44%	0.905%
53	8.312	2235	2246	2279	rBV	805792	1530009	63.01%	7.656%
54	9.086	2474	2487	2512	rBV	1002224	1725851	71.08%	8.636%
55	9.257	2536	2540	2543	rBV3	1070	952	0.04%	0.005%
56	9.347	2563	2568	2569	rBV3	957	660	0.03%	0.003%
57	9.373	2573	2576	2578	rBV2	1135	732	0.03%	0.004%
58	9.488	2610	2612	2614	rBV	759	508	0.02%	0.003%
59	9.550	2626	2631	2636	rBV3	959	1077	0.04%	0.005%
60	9.701	2675	2678	2685	rBV4	1004	995	0.04%	0.005%
61	9.736	2685	2689	2692	rVV3	696	539	0.02%	0.003%
62	9.794	2705	2707	2709	rVV3	731	445	0.02%	0.002%
63	9.816	2711	2714	2721	rVB7	1069	1069	0.04%	0.005%
64	9.865	2726	2729	2733	rBV	835	662	0.03%	0.003%
65	9.890	2733	2737	2742	rVV3	811	968	0.04%	0.005%
66	9.913	2742	2744	2748	rVV	772	449	0.02%	0.002%
67	9.932	2748	2750	2756	rVB3	538	498	0.02%	0.002%
68	10.016	2774	2776	2781	rVB2	1025	849	0.03%	0.004%
69	10.045	2781	2785	2787	rBV	1125	875	0.04%	0.004%
70	10.167	2817	2823	2824	rBV2	758	820	0.03%	0.004%
71	10.331	2869	2874	2878	rBV3	989	706	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031407.D
 Acq On : 22 Apr 2019 22:29
 Operator : JC/SP
 Sample : K2428-15DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X16DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2928	rBV	778667	1252291	51.57%	6.266%
73	10.556	2941	2944	2948	rVB3	912	693	0.03%	0.003%
74	10.701	2985	2989	2991	rVB3	594	475	0.02%	0.002%
75	10.787	3013	3016	3019	rVB2	733	524	0.02%	0.003%
76	10.848	3031	3035	3036	rBV	830	534	0.02%	0.003%
77	10.922	3055	3058	3062	rBV2	553	453	0.02%	0.002%
78	11.003	3078	3083	3087	rVB4	1025	951	0.04%	0.005%
79	11.083	3104	3108	3115	rVB7	814	960	0.04%	0.005%
80	11.151	3122	3129	3132	rBV3	861	925	0.04%	0.005%
81	11.215	3144	3149	3152	rBV	823	773	0.03%	0.004%
82	11.276	3165	3168	3171	rVV2	654	489	0.02%	0.002%
83	11.363	3192	3195	3199	rBV2	627	454	0.02%	0.002%
84	11.395	3200	3205	3207	rBV2	839	744	0.03%	0.004%
85	11.479	3219	3231	3259	rBV	870977	1438023	59.22%	7.195%
86	11.765	3317	3320	3327	rVB4	1088	909	0.04%	0.005%
87	11.855	3335	3348	3372	rBV	899565	1521394	62.66%	7.612%
88	12.472	3536	3540	3546	rBV4	2058	2662	0.11%	0.013%
89	12.562	3565	3568	3570	rBV3	694	449	0.02%	0.002%
90	12.601	3577	3580	3584	rBV3	970	773	0.03%	0.004%
91	12.720	3612	3617	3618	rBV3	1227	1007	0.04%	0.005%
92	12.906	3672	3675	3679	rBV3	1617	1105	0.05%	0.006%
93	13.041	3714	3717	3719	rBV2	823	462	0.02%	0.002%
94	13.212	3767	3770	3773	rBV2	885	651	0.03%	0.003%
95	13.414	3830	3833	3840	rBV2	861	774	0.03%	0.004%
96	13.466	3847	3849	3854	rBV3	718	644	0.03%	0.003%
97	14.112	4046	4050	4057	rBV5	1761	2035	0.08%	0.010%
98	14.196	4072	4076	4081	rBV3	1708	2251	0.09%	0.011%
99	14.331	4115	4118	4121	rBV2	1163	741	0.03%	0.004%
100	15.016	4328	4331	4335	rBV4	1419	1350	0.06%	0.007%


Sum of corrected areas: 19985488

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031407.D
Acq On : 22 Apr 2019 22:29
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X16DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

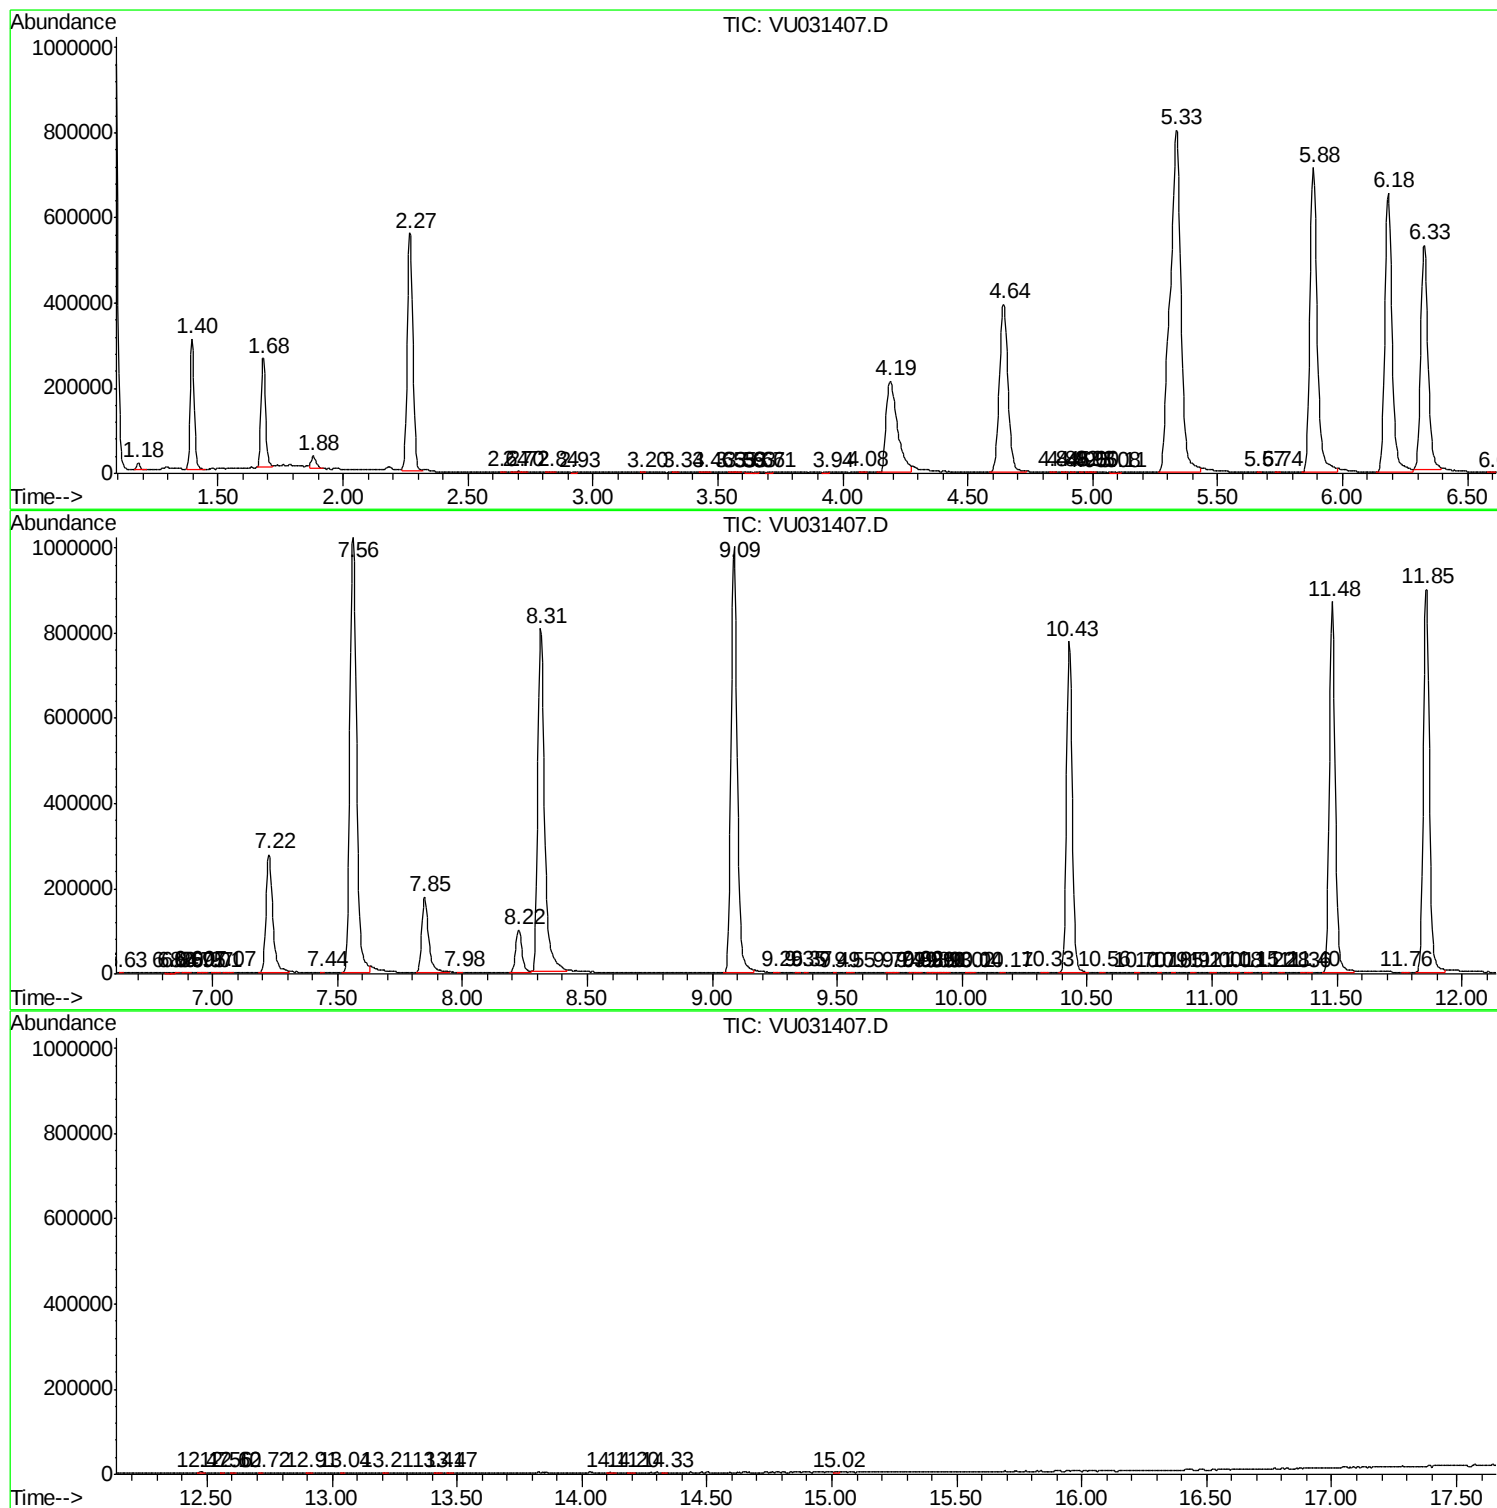

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031407.D
Acq On : 22 Apr 2019 22:29
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X16DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031407.D
Acq On : 22 Apr 2019 22:29
Operator : JC/SP
Sample : K2428-15DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X16DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc