

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031412.D
 Acq On : 23 Apr 2019 00:25
 Operator : JC/SP
 Sample : K2477-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB3	16971	16130	0.03%	0.019%
2	1.395	88	95	107	rBV	400464	432361	0.70%	0.506%
3	1.682	176	184	198	rVB	319357	392246	0.64%	0.459%
4	1.884	238	247	266	rVB	520186	721158	1.17%	0.844%
5	2.270	356	367	381	rVB	677213	1024655	1.66%	1.200%
6	2.473	425	430	435	rBV6	2779	3864	0.01%	0.005%
7	2.833	530	542	554	rBV2	13887	32920	0.05%	0.039%
8	2.977	583	587	599	rVB6	3784	7331	0.01%	0.009%
9	3.048	606	609	613	rBV3	1116	930	0.00%	0.001%
10	3.083	618	620	625	rVB2	542	434	0.00%	0.001%
11	3.157	639	643	644	rBV3	811	482	0.00%	0.001%
12	3.305	684	689	691	rBV2	652	599	0.00%	0.001%
13	3.382	708	713	715	rBV2	1041	977	0.00%	0.001%
14	3.395	715	717	720	rVV	1211	786	0.00%	0.001%
15	3.427	723	727	733	rBV5	1059	1208	0.00%	0.001%
16	3.479	740	743	747	rBV3	938	773	0.00%	0.001%
17	3.546	761	764	768	rVV3	611	537	0.00%	0.001%
18	3.608	775	783	786	rBV2	619	694	0.00%	0.001%
19	3.653	794	797	800	rBV2	720	444	0.00%	0.001%
20	3.717	813	817	819	rBV2	596	506	0.00%	0.001%
21	3.736	820	823	827	rVB2	767	557	0.00%	0.001%
22	3.781	832	837	840	rVB2	990	838	0.00%	0.001%
23	3.807	840	845	846	rBV2	736	638	0.00%	0.001%
24	3.936	883	885	889	rBV2	850	453	0.00%	0.001%
25	3.955	889	891	895	rVB3	716	507	0.00%	0.001%
26	4.022	909	912	916	rBV3	547	430	0.00%	0.001%
27	4.093	932	934	938	rVB	775	491	0.00%	0.001%
28	4.135	942	947	950	rBV3	493	440	0.00%	0.001%
29	4.186	950	963	1003	rBV	238713	805797	1.31%	0.943%
30	4.508	1060	1063	1065	rBV4	925	547	0.00%	0.001%
31	4.524	1065	1068	1072	rVV2	1140	978	0.00%	0.001%
32	4.643	1088	1105	1135	rBV	436066	1041222	1.69%	1.219%
33	4.977	1206	1209	1211	rBV3	1150	742	0.00%	0.001%
34	5.128	1246	1256	1274	rVV3	12167	28721	0.05%	0.034%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031412.D
 Acq On : 23 Apr 2019 00:25
 Operator : JC/SP
 Sample : K2477-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.222	1282	1285	1288	rVB3	766	478	0.00%	0.001%
36	5.334	1295	1320	1349	rBV2	923065	2735989	4.44%	3.203%
37	5.730	1437	1443	1444	rBV	1074	902	0.00%	0.001%
38	5.775	1455	1457	1462	rVB3	954	483	0.00%	0.001%
39	5.881	1475	1490	1529	rBV2	750208	1556716	2.53%	1.823%
40	6.183	1566	1584	1618	rBV	31449928	61603149	100.00%	72.127%
41	6.328	1620	1629	1668	rVB	625243	1431138	2.32%	1.676%
42	6.714	1745	1749	1751	rBV3	1538	1159	0.00%	0.001%
43	6.771	1764	1767	1772	rVV5	918	1032	0.00%	0.001%
44	6.865	1793	1796	1797	rBV2	1117	503	0.00%	0.001%
45	6.929	1812	1816	1819	rVB3	1366	959	0.00%	0.001%
46	7.022	1842	1845	1848	rVB3	786	563	0.00%	0.001%
47	7.103	1866	1870	1873	rVB4	852	567	0.00%	0.001%
48	7.225	1896	1908	1935	rBV	333133	621963	1.01%	0.728%
49	7.562	1994	2013	2047	rBV	1221704	2212335	3.59%	2.590%
50	7.849	2091	2102	2129	rBV2	217939	397052	0.64%	0.465%
51	8.070	2164	2171	2184	rVB8	6941	11584	0.02%	0.014%
52	8.177	2193	2204	2207	rBV2	16702	26004	0.04%	0.030%
53	8.222	2207	2218	2235	rVV	1177569	2046891	3.32%	2.397%
54	8.308	2236	2245	2275	rVB	875923	1602803	2.60%	1.877%
55	8.562	2321	2324	2328	rBV4	920	668	0.00%	0.001%
56	8.617	2339	2341	2345	rBV2	809	480	0.00%	0.001%
57	8.877	2420	2422	2424	rBV2	834	509	0.00%	0.001%
58	8.945	2439	2443	2446	rBV4	1293	974	0.00%	0.001%
59	8.987	2453	2456	2459	rVB3	735	565	0.00%	0.001%
60	9.012	2459	2464	2467	rVB4	605	504	0.00%	0.001%
61	9.035	2467	2471	2474	rBV4	1063	780	0.00%	0.001%
62	9.086	2474	2487	2522	rBV	1071338	1851453	3.01%	2.168%
63	9.466	2602	2605	2608	rBV3	797	715	0.00%	0.001%
64	9.508	2613	2618	2621	rBV3	985	944	0.00%	0.001%
65	9.684	2668	2673	2677	rBV5	1529	1587	0.00%	0.002%
66	9.755	2691	2695	2697	rBV2	683	456	0.00%	0.001%
67	10.009	2771	2774	2776	rBV	832	514	0.00%	0.001%
68	10.029	2776	2780	2781	rVV	709	544	0.00%	0.001%
69	10.196	2830	2832	2837	rVB3	673	461	0.00%	0.001%
70	10.244	2845	2847	2852	rBV	749	565	0.00%	0.001%
71	10.308	2864	2867	2868	rBV2	878	479	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031412.D
 Acq On : 23 Apr 2019 00:25
 Operator : JC/SP
 Sample : K2477-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.318	2868	2870	2873	rVV2	1148	552	0.00%	0.001%
73	10.334	2873	2875	2882	rVB4	708	690	0.00%	0.001%
74	10.427	2891	2904	2929	rBV	809114	1318896	2.14%	1.544%
75	10.604	2950	2959	2969	rVB3	19266	28794	0.05%	0.034%
76	10.729	2996	2998	3001	rVB3	1138	561	0.00%	0.001%
77	10.758	3001	3007	3015	rBV5	1178	1376	0.00%	0.002%
78	10.861	3037	3039	3045	rVB3	679	527	0.00%	0.001%
79	10.893	3045	3049	3050	rBV3	810	605	0.00%	0.001%
80	11.080	3102	3107	3113	rBV8	1300	1558	0.00%	0.002%
81	11.128	3117	3122	3125	rBV4	890	791	0.00%	0.001%
82	11.202	3143	3145	3148	rVB	1194	623	0.00%	0.001%
83	11.225	3149	3152	3154	rBV3	940	601	0.00%	0.001%
84	11.324	3181	3183	3188	rVB3	1095	744	0.00%	0.001%
85	11.398	3203	3206	3208	rBV3	1063	732	0.00%	0.001%
86	11.479	3219	3231	3260	rBV	961340	1585709	2.57%	1.857%
87	11.855	3336	3348	3371	rBV	1043699	1743193	2.83%	2.041%
88	12.167	3443	3445	3448	rBV4	779	485	0.00%	0.001%
89	12.437	3527	3529	3532	rVB4	1015	486	0.00%	0.001%
90	12.475	3532	3541	3552	rVB6	4484	8362	0.01%	0.010%
91	12.543	3560	3562	3566	rBV3	715	464	0.00%	0.001%
92	12.623	3584	3587	3591	rVB2	772	474	0.00%	0.001%
93	12.649	3591	3595	3597	rBV2	1124	828	0.00%	0.001%
94	12.665	3597	3600	3604	rBV4	1109	889	0.00%	0.001%
95	13.543	3867	3873	3877	rBV5	1396	1826	0.00%	0.002%
96	13.778	3937	3946	3952	rBV7	5326	10299	0.02%	0.012%
97	14.099	4044	4046	4048	rBV2	911	500	0.00%	0.001%
98	14.369	4128	4130	4134	rBV3	1355	1018	0.00%	0.001%
99	14.893	4284	4293	4316	rBV2	20419	53216	0.09%	0.062%
100	15.070	4344	4348	4353	rBV5	7718	8201	0.01%	0.010%


Sum of corrected areas: 85408864

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031412.D
Acq On : 23 Apr 2019 00:25
Operator : JC/SP
Sample : K2477-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

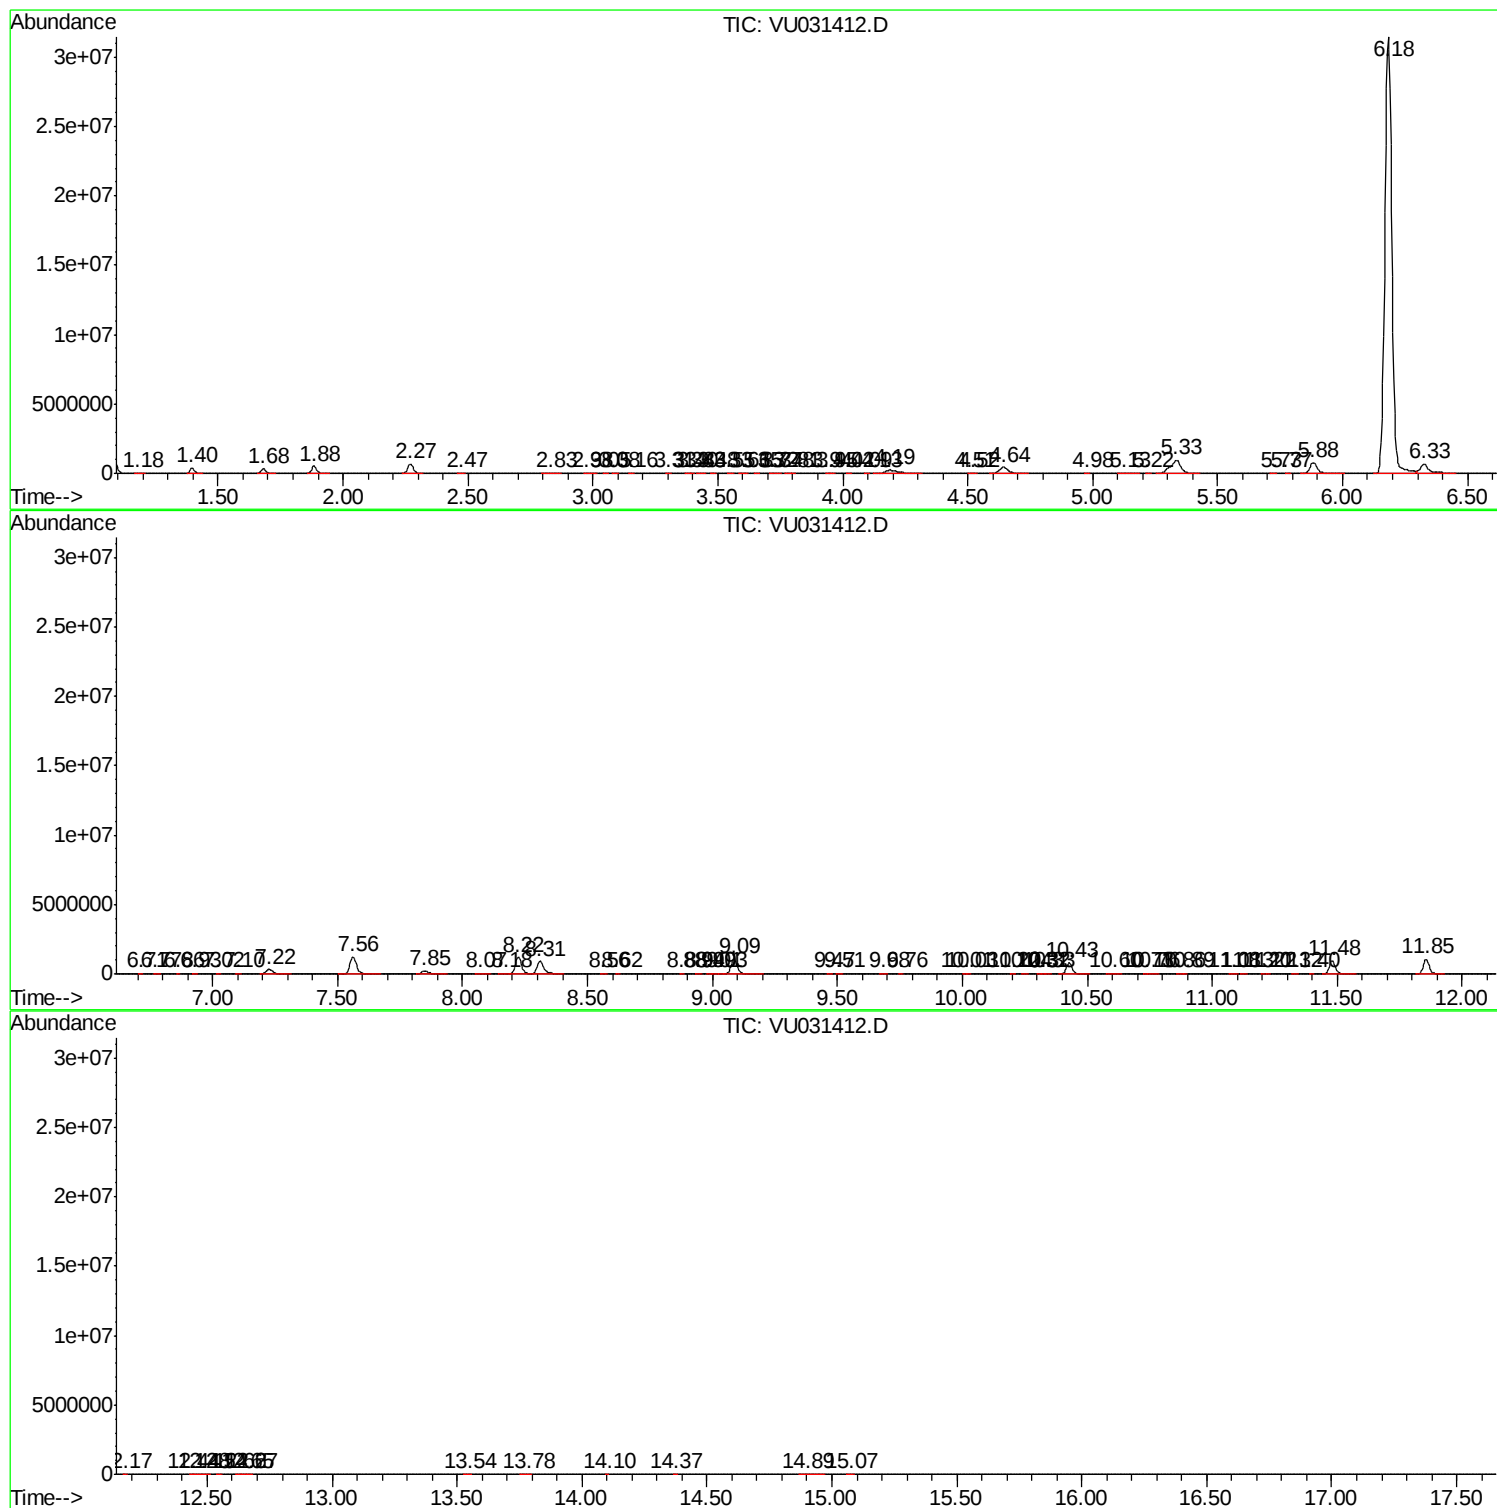

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031412.D
Acq On : 23 Apr 2019 00:25
Operator : JC/SP
Sample : K2477-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031412.D
Acq On : 23 Apr 2019 00:25
Operator : JC/SP
Sample : K2477-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc