

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031416.D
 Acq On : 23 Apr 2019 01:58
 Operator : JC/SP
 Sample : K2478-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	37	rVB	17128	17799	0.23%	0.066%
2	1.396	88	95	108	rVB	392229	422358	5.40%	1.562%
3	1.678	176	183	201	rVB	299134	378429	4.84%	1.400%
4	1.830	225	230	240	rVB	29191	35579	0.45%	0.132%
5	1.884	241	247	256	rVB	24225	32227	0.41%	0.119%
6	2.270	356	367	381	rBV	648005	991016	12.67%	3.665%
7	2.331	381	386	402	rVB7	11134	22797	0.29%	0.084%
8	2.469	426	429	433	rBV3	1096	920	0.01%	0.003%
9	2.524	441	446	447	rBV3	2270	2031	0.03%	0.008%
10	2.772	521	523	528	rBV4	832	801	0.01%	0.003%
11	2.833	531	542	559	rVV2	14565	31163	0.40%	0.115%
12	3.125	626	633	636	rVV4	652	807	0.01%	0.003%
13	3.183	649	651	655	rVB2	936	530	0.01%	0.002%
14	3.225	661	664	667	rVB2	838	556	0.01%	0.002%
15	3.293	681	685	688	rVB2	871	605	0.01%	0.002%
16	3.318	688	693	697	rBV4	743	814	0.01%	0.003%
17	3.530	756	759	763	rBV2	530	526	0.01%	0.002%
18	3.592	775	778	781	rBV3	779	601	0.01%	0.002%
19	3.765	828	832	835	rBV2	758	654	0.01%	0.002%
20	3.868	859	864	866	rBV2	659	715	0.01%	0.003%
21	3.974	894	897	902	rBV3	1054	802	0.01%	0.003%
22	4.083	928	931	941	rVB5	899	1354	0.02%	0.005%
23	4.190	950	964	967	rBV	229316	435452	5.57%	1.610%
24	4.643	1087	1105	1131	rVV2	403374	966878	12.36%	3.576%
25	4.768	1143	1144	1150	rVB4	1780	967	0.01%	0.004%
26	4.987	1204	1212	1214	rBV4	1309	1218	0.02%	0.005%
27	5.042	1226	1229	1235	rVB5	882	769	0.01%	0.003%
28	5.083	1238	1242	1247	rVB5	948	991	0.01%	0.004%
29	5.119	1249	1253	1255	rBV2	792	667	0.01%	0.002%
30	5.337	1296	1321	1349	rBV2	861226	2540566	32.49%	9.396%
31	5.636	1411	1414	1416	rBV3	1166	656	0.01%	0.002%
32	5.881	1477	1490	1508	rBV	685955	1389183	17.76%	5.138%
33	6.180	1568	1583	1616	rBV	3934070	7819915	100.00%	28.920%
34	6.325	1617	1628	1665	rVB2	557482	1201719	15.37%	4.444%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031416.D
 Acq On : 23 Apr 2019 01:58
 Operator : JC/SP
 Sample : K2478-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	6.624	1719	1721	1726	rVB4	795	542	0.01%	0.002%
36	6.681	1735	1739	1742	rVB3	755	564	0.01%	0.002%
37	6.723	1747	1752	1757	rBV5	1154	1432	0.02%	0.005%
38	6.813	1775	1780	1783	rBV3	1826	1664	0.02%	0.006%
39	6.833	1783	1786	1790	rVV3	933	844	0.01%	0.003%
40	7.103	1867	1870	1873	rVB2	1175	688	0.01%	0.003%
41	7.225	1896	1908	1940	rBV	314306	604664	7.73%	2.236%
42	7.472	1980	1985	1989	rBV4	1224	1340	0.02%	0.005%
43	7.562	2000	2013	2055	rBV	1153863	2143666	27.41%	7.928%
44	7.784	2079	2082	2089	rVB6	1012	1098	0.01%	0.004%
45	7.849	2090	2102	2125	rBV	204210	373159	4.77%	1.380%
46	8.054	2162	2166	2169	rBV5	1393	897	0.01%	0.003%
47	8.132	2187	2190	2191	rBV2	978	640	0.01%	0.002%
48	8.177	2193	2204	2209	rVV3	13123	20430	0.26%	0.076%
49	8.225	2211	2219	2235	rVV3	66206	115102	1.47%	0.426%
50	8.312	2235	2246	2287	rVV	840705	1599407	20.45%	5.915%
51	8.707	2363	2369	2373	rVB6	1755	1770	0.02%	0.007%
52	8.739	2376	2379	2381	rVB3	1039	569	0.01%	0.002%
53	8.829	2401	2407	2409	rBV3	877	849	0.01%	0.003%
54	8.968	2446	2450	2453	rBV	963	759	0.01%	0.003%
55	9.086	2474	2487	2507	rBV	969788	1644605	21.03%	6.082%
56	9.331	2558	2563	2568	rVB5	1833	2013	0.03%	0.007%
57	9.376	2573	2577	2579	rBV4	1082	785	0.01%	0.003%
58	9.517	2615	2621	2622	rBV	766	586	0.01%	0.002%
59	9.553	2628	2632	2636	rBV3	1198	913	0.01%	0.003%
60	9.630	2652	2656	2657	rBV3	941	625	0.01%	0.002%
61	9.775	2694	2701	2704	rVV3	608	695	0.01%	0.003%
62	9.797	2704	2708	2711	rVV3	655	555	0.01%	0.002%
63	9.826	2711	2717	2722	rVB5	783	1008	0.01%	0.004%
64	9.894	2735	2738	2740	rBV2	936	578	0.01%	0.002%
65	10.003	2768	2772	2780	rVB3	1288	1975	0.03%	0.007%
66	10.048	2780	2786	2788	rBV2	857	914	0.01%	0.003%
67	10.096	2797	2801	2803	rBV2	963	767	0.01%	0.003%
68	10.122	2803	2809	2815	rVB3	1166	1741	0.02%	0.006%
69	10.151	2815	2818	2823	rBV3	1193	1173	0.02%	0.004%
70	10.180	2823	2827	2833	rVB5	1071	1490	0.02%	0.006%
71	10.215	2833	2838	2841	rBV4	1084	1026	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031416.D
 Acq On : 23 Apr 2019 01:58
 Operator : JC/SP
 Sample : K2478-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.241	2841	2846	2851	rBV3	845	976	0.01%	0.004%
73	10.427	2891	2904	2926	rBV	726989	1186679	15.18%	4.389%
74	10.604	2949	2959	2970	rVB3	12917	23038	0.29%	0.085%
75	10.652	2970	2974	2977	rBV2	963	798	0.01%	0.003%
76	10.668	2977	2979	2984	rVB3	839	699	0.01%	0.003%
77	11.144	3124	3127	3132	rBV2	907	814	0.01%	0.003%
78	11.218	3147	3150	3154	rBV4	809	742	0.01%	0.003%
79	11.241	3154	3157	3163	rVV2	791	825	0.01%	0.003%
80	11.405	3205	3208	3214	rVV5	1132	1125	0.01%	0.004%
81	11.479	3219	3231	3251	rBV	859112	1402463	17.93%	5.187%
82	11.855	3335	3348	3373	rBV	935372	1565655	20.02%	5.790%
83	12.064	3410	3413	3414	rBV3	1499	880	0.01%	0.003%
84	12.154	3438	3441	3443	rBV4	1265	867	0.01%	0.003%
85	12.221	3459	3462	3464	rBV2	1308	656	0.01%	0.002%
86	12.482	3531	3543	3550	rBV7	3656	6429	0.08%	0.024%
87	12.517	3550	3554	3556	rBV3	1036	915	0.01%	0.003%
88	12.562	3566	3568	3572	rVB2	847	566	0.01%	0.002%
89	12.585	3572	3575	3580	rBV2	1025	701	0.01%	0.003%
90	12.672	3598	3602	3603	rBV2	860	636	0.01%	0.002%
91	12.900	3669	3673	3677	rBV3	1128	1027	0.01%	0.004%
92	12.938	3680	3685	3689	rBV4	1156	1418	0.02%	0.005%
93	13.080	3727	3729	3733	rVB3	912	692	0.01%	0.003%
94	13.765	3939	3942	3945	rVB	1346	956	0.01%	0.004%
95	13.791	3945	3950	3951	rBV2	1598	1345	0.02%	0.005%
96	14.385	4132	4135	4141	rBV5	1299	1234	0.02%	0.005%
97	14.414	4141	4144	4147	rBV	1014	869	0.01%	0.003%
98	14.495	4166	4169	4172	rBV3	1653	1205	0.02%	0.004%
99	14.514	4172	4175	4180	rVV3	1102	1245	0.02%	0.005%
100	14.559	4185	4189	4192	rVV3	1218	868	0.01%	0.003%


Sum of corrected areas: 27039921

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031416.D
Acq On : 23 Apr 2019 01:58
Operator : JC/SP
Sample : K2478-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

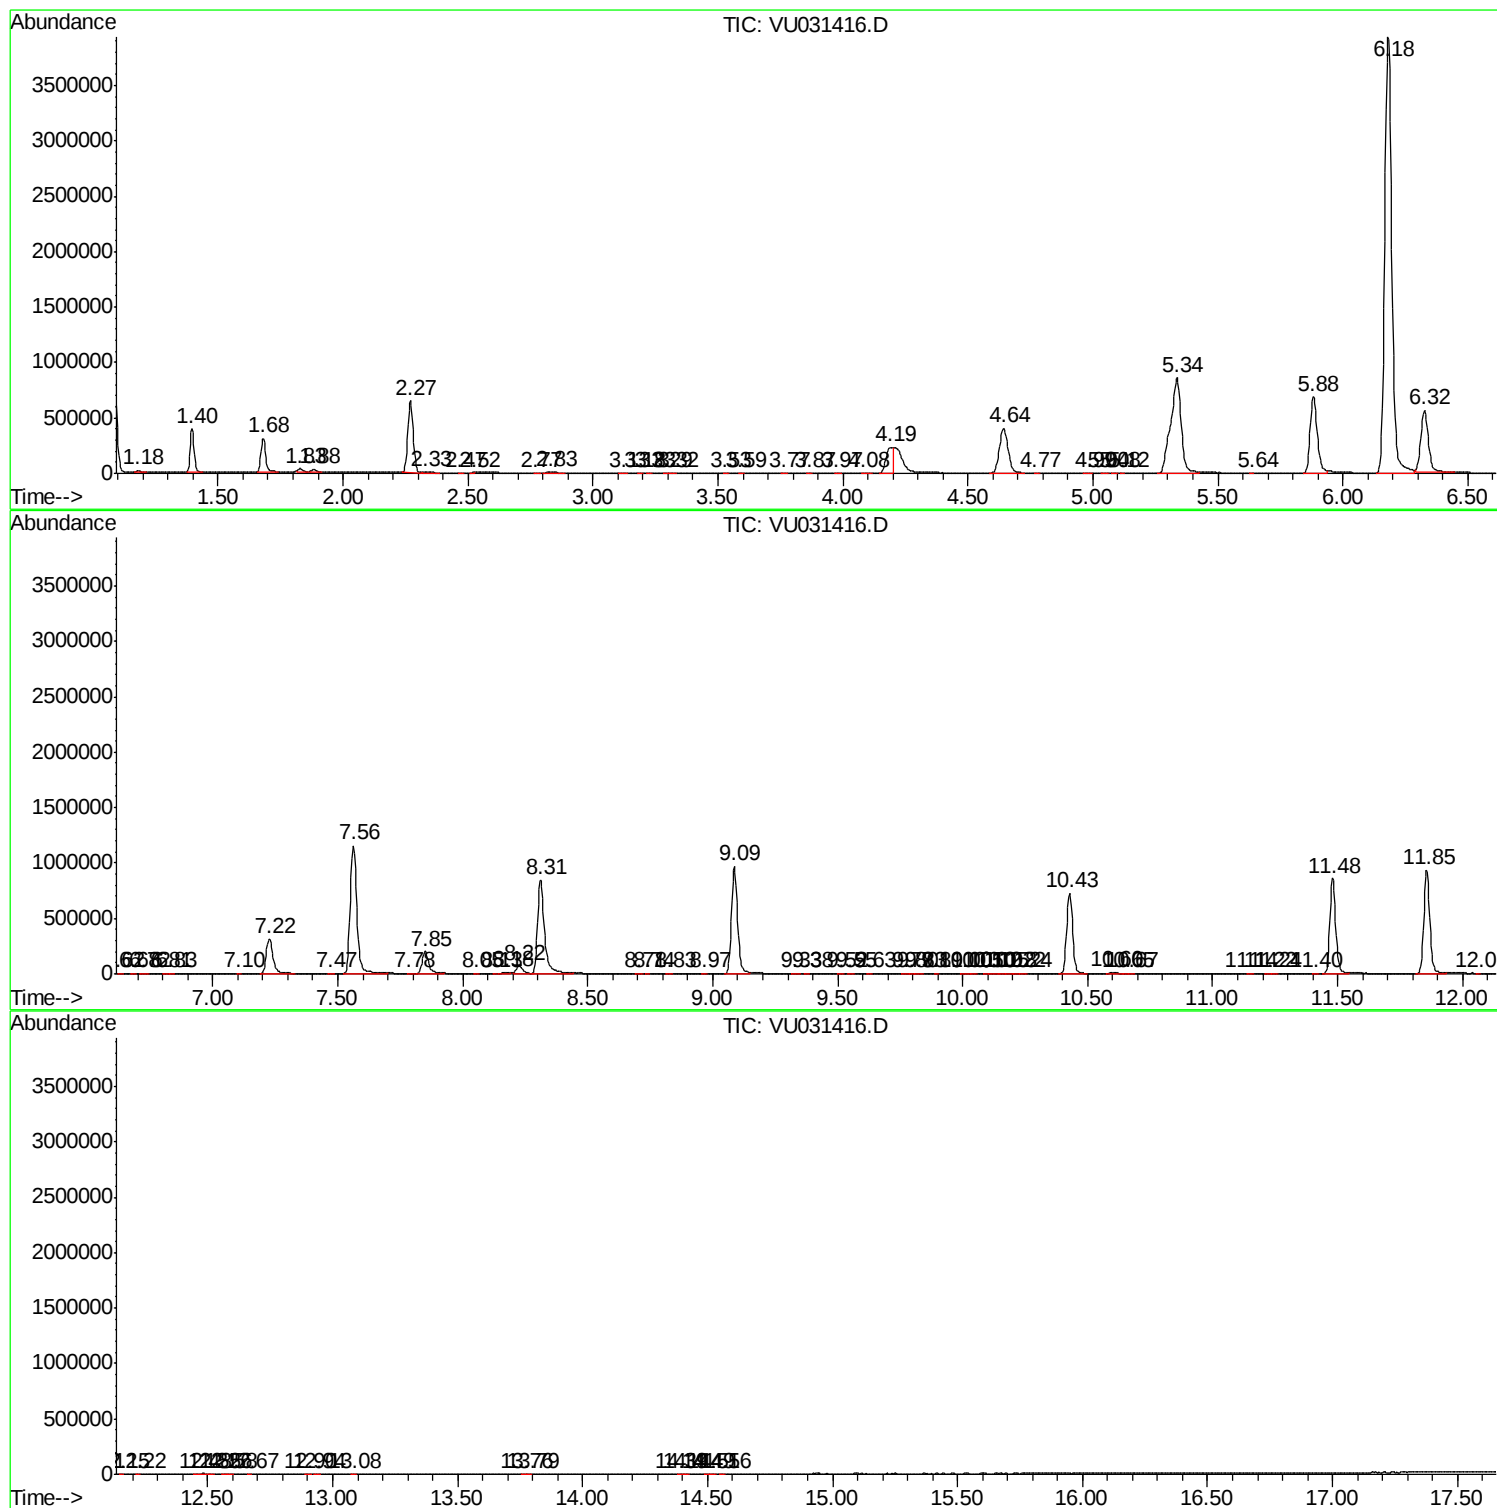

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031416.D
Acq On : 23 Apr 2019 01:58
Operator : JC/SP
Sample : K2478-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031416.D
Acq On : 23 Apr 2019 01:58
Operator : JC/SP
Sample : K2478-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc