

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031417.D
 Acq On : 23 Apr 2019 02:21
 Operator : JC/SP
 Sample : K2478-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	40	rBV	17267	18249	0.01%	0.008%
2	1.293	59	63	68	rBV	5939	6399	0.00%	0.003%
3	1.395	88	95	107	rBV	406722	437979	0.23%	0.197%
4	1.682	176	184	198	rVB	321959	397962	0.21%	0.179%
5	1.833	224	231	237	rBV	52789	68718	0.04%	0.031%
6	1.884	238	247	263	rVB	837921	1150345	0.60%	0.517%
7	2.270	355	367	380	rBV	675716	1042612	0.54%	0.469%
8	2.540	444	451	453	rBV5	1695	2205	0.00%	0.001%
9	2.755	515	518	523	rVB3	1132	1007	0.00%	0.000%
10	2.784	523	527	529	rBV2	865	653	0.00%	0.000%
11	2.836	529	543	555	rVV3	13319	30570	0.02%	0.014%
12	2.923	568	570	575	rVV3	718	649	0.00%	0.000%
13	2.984	579	589	601	rVV3	10839	22244	0.01%	0.010%
14	3.038	604	606	610	rVB2	837	557	0.00%	0.000%
15	3.087	618	621	625	rVB2	935	777	0.00%	0.000%
16	3.128	631	634	638	rBV3	649	625	0.00%	0.000%
17	3.222	659	663	666	rBV2	816	718	0.00%	0.000%
18	3.260	672	675	683	rVB4	995	1089	0.00%	0.000%
19	3.305	683	689	692	rBV3	1014	1031	0.00%	0.000%
20	3.427	723	727	729	rBV3	886	702	0.00%	0.000%
21	3.476	740	742	745	rVB	850	492	0.00%	0.000%
22	3.492	745	747	752	rVB	925	645	0.00%	0.000%
23	3.569	767	771	773	rBV2	690	465	0.00%	0.000%
24	3.656	792	798	803	rVB3	914	834	0.00%	0.000%
25	3.923	877	881	885	rBV3	1031	790	0.00%	0.000%
26	3.974	894	897	901	rVB3	930	645	0.00%	0.000%
27	4.000	901	905	907	rBV3	745	546	0.00%	0.000%
28	4.132	941	946	951	rVB2	780	627	0.00%	0.000%
29	4.199	951	967	1011	rBV3	236933	980435	0.51%	0.441%
30	4.556	1074	1078	1082	rBV6	1195	1303	0.00%	0.001%
31	4.643	1089	1105	1133	rBV	433430	1066529	0.56%	0.480%
32	4.913	1187	1189	1195	rVB4	1740	1169	0.00%	0.001%
33	4.980	1207	1210	1218	rVV5	1606	2137	0.00%	0.001%
34	5.070	1230	1238	1239	rBV4	547	551	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031417.D
 Acq On : 23 Apr 2019 02:21
 Operator : JC/SP
 Sample : K2478-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.135	1245	1258	1273	rBV4	12647	29713	0.02%	0.013%
36	5.231	1286	1288	1293	rVB	1400	926	0.00%	0.000%
37	5.337	1293	1321	1342	rBV2	932602	2716846	1.42%	1.222%
38	5.675	1421	1426	1428	rBV3	752	749	0.00%	0.000%
39	5.717	1436	1439	1442	rBV2	788	621	0.00%	0.000%
40	5.755	1448	1451	1454	rVB3	1382	767	0.00%	0.000%
41	5.781	1455	1459	1465	rVB5	786	859	0.00%	0.000%
42	5.884	1477	1491	1532	rBV	754999	1561203	0.81%	0.702%
43	6.193	1566	1587	1619	rBV4	91732722	191706014	100.00%	86.201%
44	6.749	1757	1760	1763	rBV4	1614	1095	0.00%	0.000%
45	7.032	1845	1848	1852	rBV3	1171	1202	0.00%	0.001%
46	7.090	1863	1866	1869	rBV	1471	1355	0.00%	0.001%
47	7.225	1897	1908	1932	rBV	341154	632387	0.33%	0.284%
48	7.456	1977	1980	1982	rBV3	872	598	0.00%	0.000%
49	7.562	1999	2013	2058	rBV	1236373	2268456	1.18%	1.020%
50	7.849	2091	2102	2127	rBV	218821	397612	0.21%	0.179%
51	8.070	2162	2171	2185	rBV2	21221	38293	0.02%	0.017%
52	8.138	2189	2192	2193	rBV3	972	497	0.00%	0.000%
53	8.176	2193	2204	2205	rBV4	21816	27700	0.01%	0.012%
54	8.221	2206	2218	2236	rVV	5312140	9197877	4.80%	4.136%
55	8.312	2237	2246	2289	rVB	895069	1792877	0.94%	0.806%
56	8.543	2315	2318	2320	rBV3	1543	706	0.00%	0.000%
57	8.707	2367	2369	2375	rVB8	1270	1281	0.00%	0.001%
58	8.800	2395	2398	2402	rBV3	1366	1287	0.00%	0.001%
59	8.829	2403	2407	2410	rVV4	867	719	0.00%	0.000%
60	8.890	2422	2426	2431	rBV6	1393	1257	0.00%	0.001%
61	8.929	2434	2438	2442	rVV5	906	821	0.00%	0.000%
62	9.086	2472	2487	2522	rBV	1100019	1928837	1.01%	0.867%
63	9.360	2570	2572	2575	rBV3	911	586	0.00%	0.000%
64	9.382	2576	2579	2580	rBV3	1107	645	0.00%	0.000%
65	9.498	2613	2615	2619	rBV3	714	504	0.00%	0.000%
66	9.540	2625	2628	2635	rBV5	1338	1215	0.00%	0.001%
67	9.578	2635	2640	2644	rVV3	993	1020	0.00%	0.000%
68	9.604	2644	2648	2651	rBV4	703	647	0.00%	0.000%
69	9.639	2656	2659	2661	rBV2	1011	708	0.00%	0.000%
70	9.668	2666	2668	2672	rVB3	764	509	0.00%	0.000%
71	9.720	2681	2684	2690	rBV3	1376	1056	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031417.D
 Acq On : 23 Apr 2019 02:21
 Operator : JC/SP
 Sample : K2478-08
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	9.771	2697	2700	2702	rVB3	1177	695	0.00%	0.000%
73	9.794	2702	2707	2708	rBV3	939	766	0.00%	0.000%
74	10.028	2777	2780	2786	rBV3	666	606	0.00%	0.000%
75	10.057	2787	2789	2794	rVB3	857	668	0.00%	0.000%
76	10.173	2821	2825	2830	rBV2	977	980	0.00%	0.000%
77	10.221	2837	2840	2842	rBV2	675	485	0.00%	0.000%
78	10.321	2866	2871	2874	rBV6	1037	1179	0.00%	0.001%
79	10.427	2890	2904	2925	rBV	832400	1353115	0.71%	0.608%
80	10.604	2951	2959	2971	rVB4	23395	38002	0.02%	0.017%
81	10.697	2985	2988	2995	rBV6	753	1020	0.00%	0.000%
82	10.774	3006	3012	3015	rBV4	1377	1402	0.00%	0.001%
83	10.945	3057	3065	3074	rBV5	937	1709	0.00%	0.001%
84	10.983	3074	3077	3080	rBV2	759	647	0.00%	0.000%
85	11.479	3219	3231	3249	rBV	1000415	1621212	0.85%	0.729%
86	11.855	3335	3348	3372	rBV	1072290	1788239	0.93%	0.804%
87	12.196	3451	3454	3456	rBV3	1086	740	0.00%	0.000%
88	12.353	3501	3503	3506	rBV2	843	464	0.00%	0.000%
89	12.427	3522	3526	3531	rBV3	1470	1536	0.00%	0.001%
90	12.475	3533	3541	3549	rVV4	6805	11242	0.01%	0.005%
91	12.639	3589	3592	3595	rBV	1321	1000	0.00%	0.000%
92	13.093	3726	3733	3735	rBV4	1292	1594	0.00%	0.001%
93	13.205	3766	3768	3770	rBV2	902	504	0.00%	0.000%
94	13.237	3775	3778	3781	rVV4	978	620	0.00%	0.000%
95	13.257	3782	3784	3788	rVB4	1090	767	0.00%	0.000%
96	13.733	3928	3932	3934	rBV3	956	716	0.00%	0.000%
97	13.884	3976	3979	3982	rBV4	1031	700	0.00%	0.000%
98	14.163	4064	4066	4069	rBV3	1029	708	0.00%	0.000%
99	14.443	4151	4153	4155	rBV3	1233	651	0.00%	0.000%
100	14.630	4209	4211	4213	rBV2	1274	685	0.00%	0.000%


Sum of corrected areas: 222394356

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031417.D
Acq On : 23 Apr 2019 02:21
Operator : JC/SP
Sample : K2478-08
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

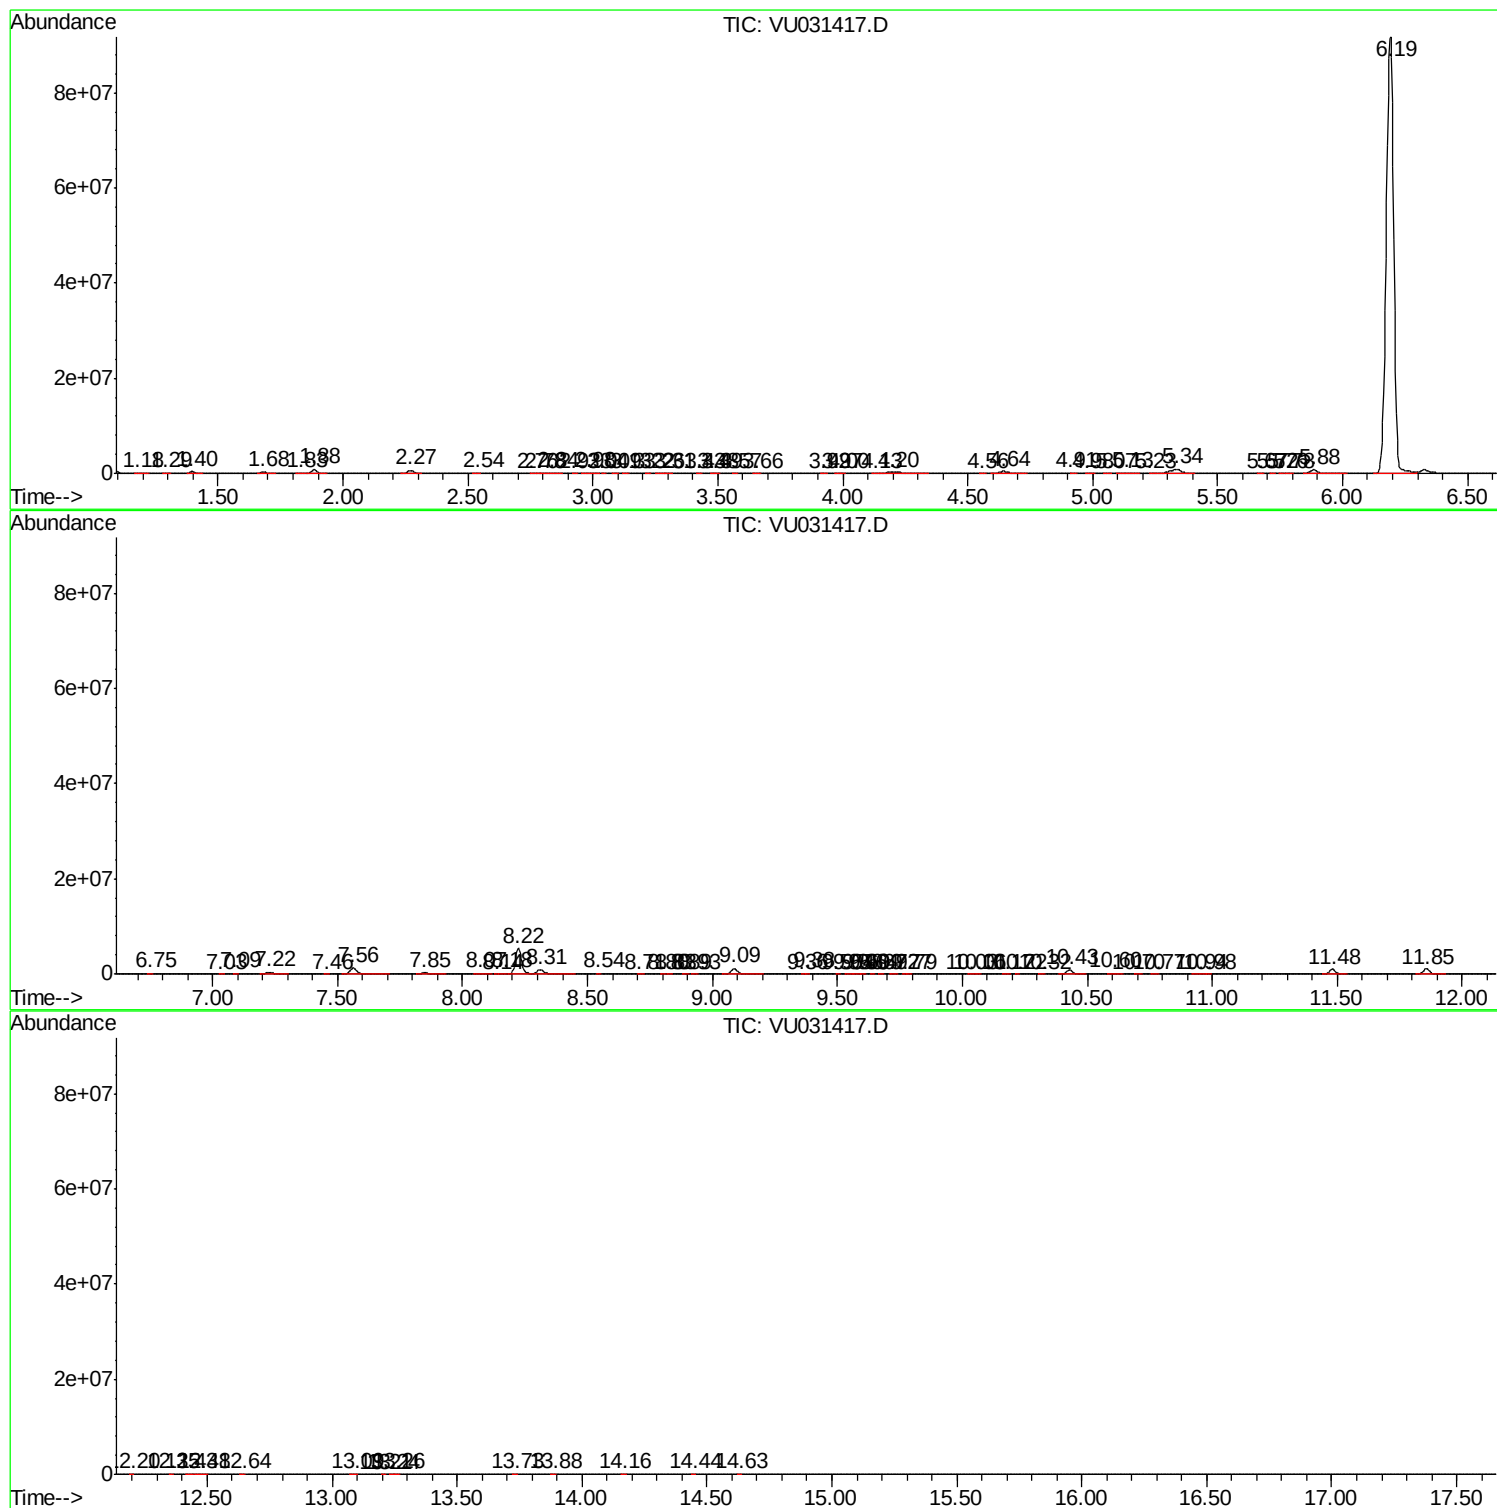

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031417.D
Acq On : 23 Apr 2019 02:21
Operator : JC/SP
Sample : K2478-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031417.D
Acq On : 23 Apr 2019 02:21
Operator : JC/SP
Sample : K2478-08
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc