

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031429.D
 Acq On : 23 Apr 2019 11:43
 Operator : JC/SP
 Sample : K2477-06DL 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB	17306	17764	0.67%	0.080%
2	1.283	54	60	69	rBV3	34259	37829	1.44%	0.170%
3	1.395	88	95	107	rBV	378176	407989	15.50%	1.836%
4	1.682	176	184	198	rBV	303258	378944	14.40%	1.705%
5	1.884	241	247	259	rVB2	30989	45697	1.74%	0.206%
6	2.270	356	367	380	rBV	634298	965508	36.68%	4.345%
7	2.434	415	418	422	rVB5	1329	948	0.04%	0.004%
8	2.456	422	425	429	rBV3	1193	1226	0.05%	0.006%
9	2.505	437	440	445	rVB4	704	614	0.02%	0.003%
10	2.543	450	452	455	rBV	735	611	0.02%	0.003%
11	2.575	458	462	463	rBV2	1171	890	0.03%	0.004%
12	2.611	470	473	477	rBV3	916	614	0.02%	0.003%
13	2.649	483	485	489	rVB3	1052	504	0.02%	0.002%
14	2.704	493	502	509	rVB10	2974	5536	0.21%	0.025%
15	2.794	527	530	534	rBV	636	552	0.02%	0.002%
16	2.907	563	565	569	rVB3	1108	609	0.02%	0.003%
17	3.061	609	613	618	rBV4	619	683	0.03%	0.003%
18	3.379	708	712	715	rBV4	651	579	0.02%	0.003%
19	3.472	734	741	744	rVB3	698	793	0.03%	0.004%
20	3.508	749	752	757	rVB3	643	609	0.02%	0.003%
21	3.624	784	788	789	rBV	679	562	0.02%	0.003%
22	3.733	819	822	824	rBV	709	534	0.02%	0.002%
23	3.823	847	850	853	rBV2	915	580	0.02%	0.003%
24	3.871	863	865	869	rVV2	616	505	0.02%	0.002%
25	3.897	869	873	875	rVV2	633	565	0.02%	0.003%
26	3.939	880	886	888	rBV2	713	624	0.02%	0.003%
27	3.968	892	895	900	rBV2	776	515	0.02%	0.002%
28	4.186	947	963	995	rBV	227372	700708	26.62%	3.153%
29	4.643	1088	1105	1136	rVV	424902	1012784	38.48%	4.558%
30	4.987	1205	1212	1215	rBV5	1755	2001	0.08%	0.009%
31	5.054	1230	1233	1238	rBV5	640	550	0.02%	0.002%
32	5.115	1248	1252	1255	rBV4	904	671	0.03%	0.003%
33	5.337	1297	1321	1345	rBV2	886352	2632131	100.00%	11.845%
34	5.800	1460	1465	1469	rVB4	842	798	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031429.D
 Acq On : 23 Apr 2019 11:43
 Operator : JC/SP
 Sample : K2477-06DL 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.884	1473	1491	1520	rBV	750874	1571483	59.70%	7.072%
36	6.122	1562	1565	1568	rBV4	1057	882	0.03%	0.004%
37	6.183	1569	1584	1615	rVV	1118440	2264838	86.05%	10.192%
38	6.328	1617	1629	1662	rVB	564981	1180969	44.87%	5.315%
39	6.623	1717	1721	1727	rVB5	686	646	0.02%	0.003%
40	6.675	1732	1737	1739	rBV4	926	624	0.02%	0.003%
41	6.704	1743	1746	1753	rVB5	1158	1044	0.04%	0.005%
42	7.106	1867	1871	1873	rBV2	808	603	0.02%	0.003%
43	7.128	1875	1878	1883	rVB2	1170	829	0.03%	0.004%
44	7.157	1883	1887	1890	rBV2	1009	753	0.03%	0.003%
45	7.183	1890	1895	1897	rBV2	856	773	0.03%	0.003%
46	7.225	1897	1908	1933	rBV	314138	588719	22.37%	2.649%
47	7.472	1982	1985	1988	rVB2	878	553	0.02%	0.002%
48	7.562	1996	2013	2063	rBV	1132428	2105998	80.01%	9.478%
49	7.849	2091	2102	2125	rBV	206358	383666	14.58%	1.727%
50	8.103	2178	2181	2183	rBV2	1074	599	0.02%	0.003%
51	8.154	2192	2197	2199	rBV2	1094	911	0.03%	0.004%
52	8.176	2201	2204	2208	rBV4	1178	1009	0.04%	0.005%
53	8.228	2210	2220	2231	rBV3	38813	68771	2.61%	0.309%
54	8.312	2235	2246	2278	rBV	810611	1530983	58.17%	6.890%
55	8.765	2384	2387	2392	rBV3	1103	823	0.03%	0.004%
56	8.797	2393	2397	2401	rVB2	865	652	0.02%	0.003%
57	8.861	2410	2417	2421	rBV4	1144	1352	0.05%	0.006%
58	8.890	2421	2426	2429	rBV3	1187	1011	0.04%	0.005%
59	8.932	2434	2439	2444	rBV6	860	846	0.03%	0.004%
60	8.961	2444	2448	2451	rVB4	1038	888	0.03%	0.004%
61	8.987	2452	2456	2458	rBV2	861	605	0.02%	0.003%
62	9.086	2474	2487	2518	rBV	1070997	1864403	70.83%	8.390%
63	9.321	2556	2560	2563	rVV3	816	684	0.03%	0.003%
64	9.369	2573	2575	2578	rBV3	988	537	0.02%	0.002%
65	9.492	2610	2613	2616	rBV2	1159	935	0.04%	0.004%
66	9.627	2652	2655	2659	rVB2	1188	843	0.03%	0.004%
67	9.659	2659	2665	2666	rBV3	855	633	0.02%	0.003%
68	9.736	2684	2689	2693	rBV5	1442	1494	0.06%	0.007%
69	9.791	2699	2706	2712	rBV6	876	1249	0.05%	0.006%
70	9.881	2731	2734	2741	rBV3	830	850	0.03%	0.004%
71	9.993	2766	2769	2770	rBV2	1014	640	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031429.D
 Acq On : 23 Apr 2019 11:43
 Operator : JC/SP
 Sample : K2477-06DL 25X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.035	2781	2782	2788	rVB	1185	692	0.03%	0.003%
73	10.073	2788	2794	2797	rBV2	1496	1635	0.06%	0.007%
74	10.311	2860	2868	2869	rBV3	627	720	0.03%	0.003%
75	10.427	2891	2904	2929	rBV	769965	1261013	47.91%	5.675%
76	10.726	2992	2997	3000	rBV2	907	731	0.03%	0.003%
77	10.746	3000	3003	3005	rBV3	690	550	0.02%	0.002%
78	10.781	3010	3014	3016	rBV4	858	655	0.02%	0.003%
79	10.926	3055	3059	3065	rBV2	645	922	0.04%	0.004%
80	11.257	3159	3162	3165	rBV3	886	751	0.03%	0.003%
81	11.273	3165	3167	3173	rVB3	1059	752	0.03%	0.003%
82	11.331	3178	3185	3186	rBV2	745	869	0.03%	0.004%
83	11.398	3200	3206	3207	rBV3	811	763	0.03%	0.003%
84	11.430	3213	3216	3219	rVB2	666	515	0.02%	0.002%
85	11.482	3219	3232	3263	rBV	925008	1532691	58.23%	6.898%
86	11.858	3336	3349	3374	rBV	936284	1598261	60.72%	7.193%
87	12.144	3435	3438	3440	rBV2	1120	794	0.03%	0.004%
88	12.308	3484	3489	3492	rBV4	771	870	0.03%	0.004%
89	12.427	3521	3526	3528	rBV2	1059	931	0.04%	0.004%
90	12.546	3558	3563	3567	rVB2	1464	1391	0.05%	0.006%
91	12.630	3586	3589	3592	rBV	1371	979	0.04%	0.004%
92	12.652	3592	3596	3598	rBV3	870	543	0.02%	0.002%
93	12.845	3652	3656	3658	rBV3	886	723	0.03%	0.003%
94	13.051	3717	3720	3726	rBV4	1286	1406	0.05%	0.006%
95	13.083	3726	3730	3733	rBV3	724	624	0.02%	0.003%
96	13.646	3902	3905	3910	rBV2	760	719	0.03%	0.003%
97	14.096	4043	4045	4050	rBV2	1305	1107	0.04%	0.005%
98	14.392	4131	4137	4142	rBV4	1433	2046	0.08%	0.009%
99	14.485	4162	4166	4169	rVB3	1847	1308	0.05%	0.006%
100	14.501	4169	4171	4174	rBV2	1219	744	0.03%	0.003%


Sum of corrected areas: 22220830

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031429.D
Acq On : 23 Apr 2019 11:43
Operator : JC/SP
Sample : K2477-06DL 25X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

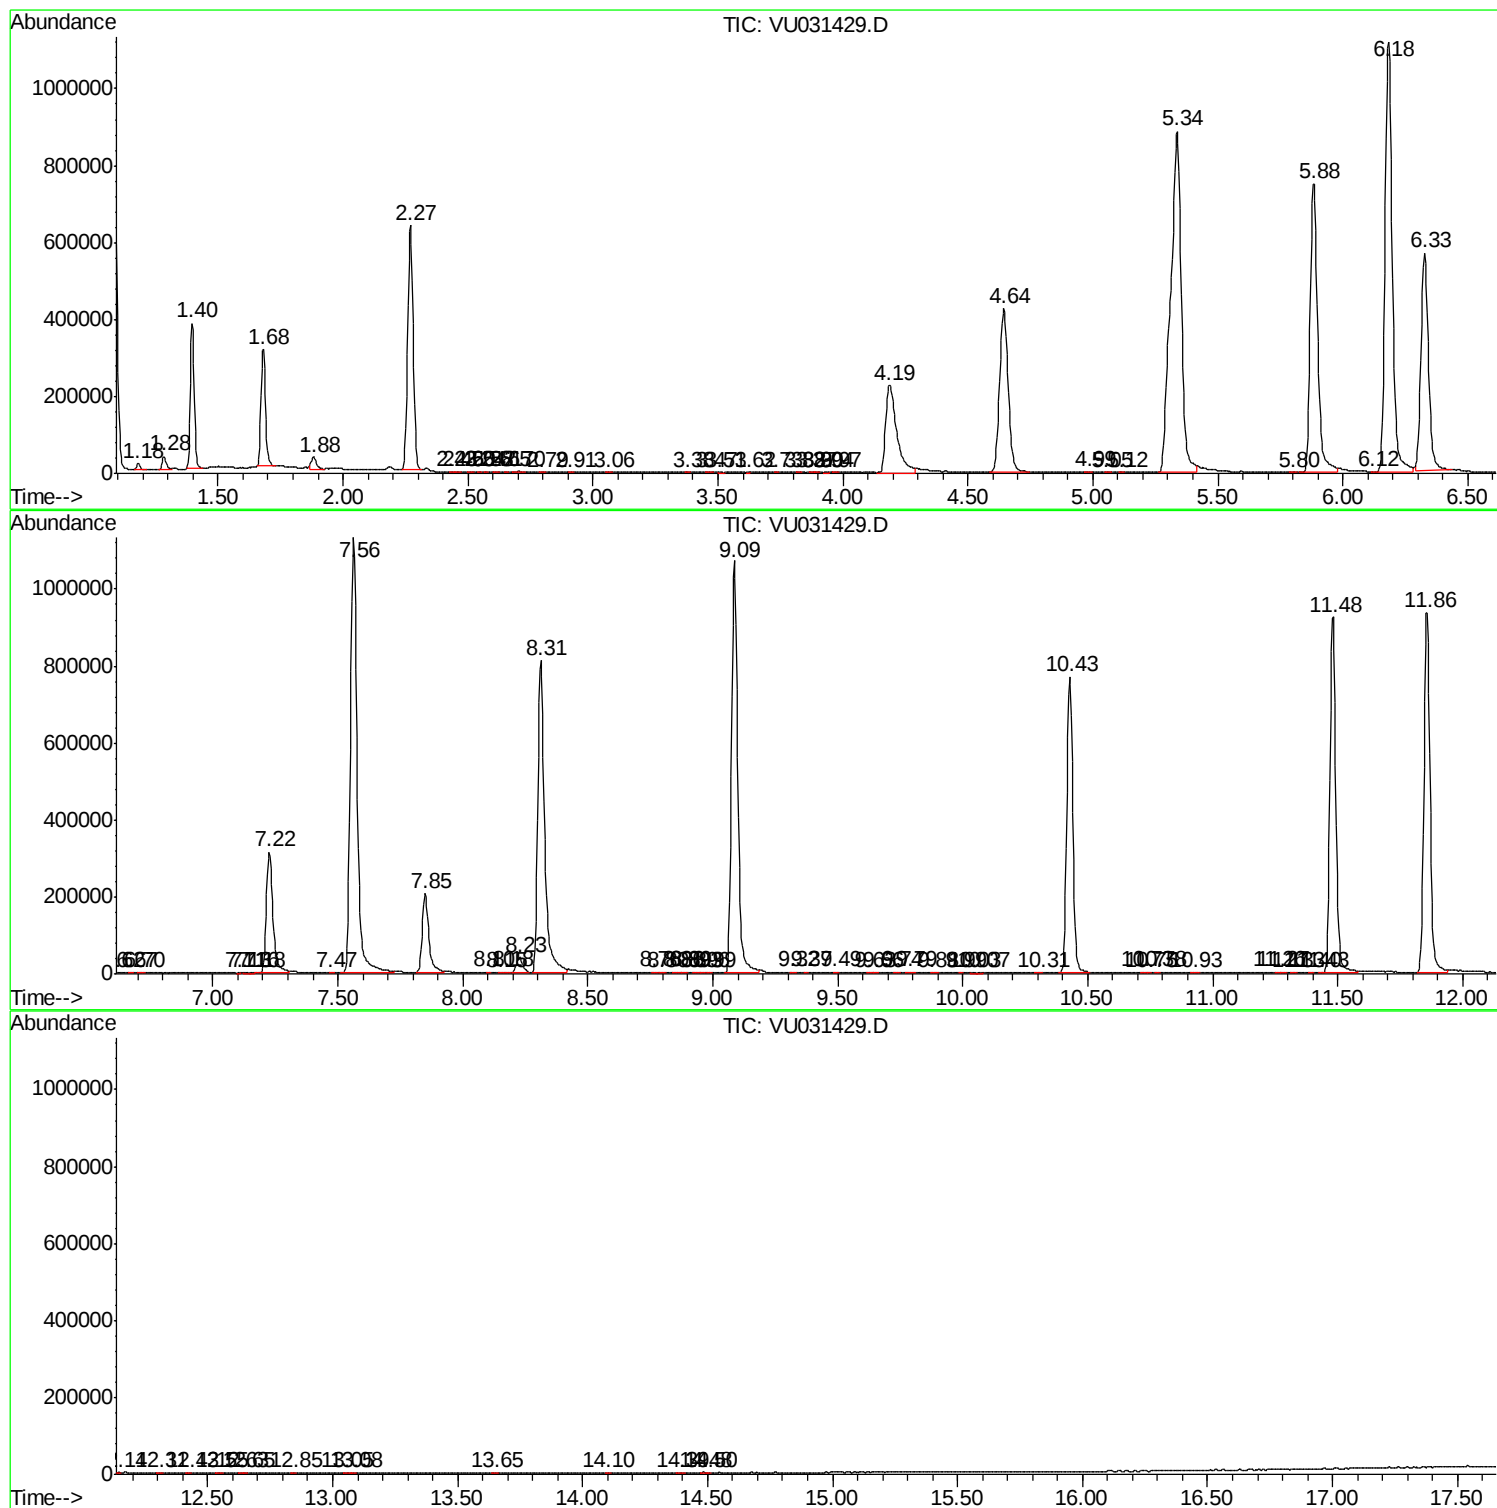

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031429.D
Acq On : 23 Apr 2019 11:43
Operator : JC/SP
Sample : K2477-06DL 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031429.D
Acq On : 23 Apr 2019 11:43
Operator : JC/SP
Sample : K2477-06DL 25X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X63DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc