

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031430.D
 Acq On : 23 Apr 2019 12:07
 Operator : JC/SP
 Sample : K2477-19DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XC6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB	18731	17789	0.69%	0.088%
2	1.396	88	95	109	rBV	358592	386329	14.96%	1.921%
3	1.682	176	184	199	rVB	280706	354206	13.72%	1.761%
4	1.884	242	247	258	rVB6	14545	21506	0.83%	0.107%
5	2.270	356	367	381	rVB	616640	935529	36.23%	4.652%
6	2.495	435	437	440	rVB3	1153	564	0.02%	0.003%
7	2.514	440	443	446	rBV3	913	631	0.02%	0.003%
8	2.531	446	448	451	rBV2	723	524	0.02%	0.003%
9	2.685	490	496	497	rBV4	1162	1182	0.05%	0.006%
10	2.878	552	556	558	rBV	915	712	0.03%	0.004%
11	2.916	564	568	569	rBV	1033	631	0.02%	0.003%
12	2.984	586	589	592	rBV4	960	762	0.03%	0.004%
13	3.003	593	595	600	rVV4	550	565	0.02%	0.003%
14	3.206	656	658	664	rVB2	740	522	0.02%	0.003%
15	3.251	668	672	677	rBV4	688	648	0.03%	0.003%
16	3.280	677	681	684	rBV2	800	707	0.03%	0.004%
17	3.315	689	692	699	rVV4	569	499	0.02%	0.002%
18	3.392	714	716	721	rVB2	985	622	0.02%	0.003%
19	3.502	743	750	753	rBV3	597	908	0.04%	0.005%
20	3.646	788	795	798	rBV5	899	1112	0.04%	0.006%
21	3.778	830	836	847	rVB3	1109	2251	0.09%	0.011%
22	3.836	847	854	857	rBV4	1068	1255	0.05%	0.006%
23	3.952	884	890	894	rBV4	806	861	0.03%	0.004%
24	4.010	905	908	912	rVV3	631	626	0.02%	0.003%
25	4.096	928	935	936	rBV2	517	588	0.02%	0.003%
26	4.190	951	964	1002	rBV2	200727	657006	25.44%	3.267%
27	4.376	1020	1022	1025	rVB2	2108	884	0.03%	0.004%
28	4.575	1080	1084	1087	rVB6	732	644	0.02%	0.003%
29	4.643	1088	1105	1127	rBV	416056	988089	38.27%	4.913%
30	4.839	1163	1166	1170	rBV4	1031	640	0.02%	0.003%
31	5.000	1201	1216	1220	rBV8	2160	4797	0.19%	0.024%
32	5.055	1232	1233	1238	rVB4	973	714	0.03%	0.004%
33	5.096	1244	1246	1251	rVB3	640	482	0.02%	0.002%
34	5.132	1253	1257	1259	rBV3	874	675	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031430.D
 Acq On : 23 Apr 2019 12:07
 Operator : JC/SP
 Sample : K2477-19DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XC6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.235	1287	1289	1292	rVB	1090	557	0.02%	0.003%
36	5.337	1297	1321	1352	rBV2	855368	2582129	100.00%	12.840%
37	5.727	1439	1442	1446	rBV4	946	644	0.02%	0.003%
38	5.813	1467	1469	1472	rVB2	1039	566	0.02%	0.003%
39	5.884	1477	1491	1522	rBV	733808	1548970	59.99%	7.702%
40	6.183	1570	1584	1615	rBV	771941	1571382	60.86%	7.814%
41	6.328	1616	1629	1654	rVV	542031	1113922	43.14%	5.539%
42	6.630	1721	1723	1727	rVB4	895	476	0.02%	0.002%
43	6.752	1758	1761	1769	rVB3	1074	1255	0.05%	0.006%
44	6.791	1769	1773	1775	rBV2	636	515	0.02%	0.003%
45	6.823	1780	1783	1787	rVB2	971	557	0.02%	0.003%
46	7.103	1863	1870	1873	rBV3	759	742	0.03%	0.004%
47	7.225	1896	1908	1932	rBV	262564	504455	19.54%	2.508%
48	7.399	1958	1962	1967	rVB5	1053	1121	0.04%	0.006%
49	7.562	2000	2013	2052	rBV	983790	1846058	71.49%	9.180%
50	7.849	2092	2102	2121	rBV	175433	321846	12.46%	1.600%
51	8.119	2180	2186	2189	rBV4	551	485	0.02%	0.002%
52	8.167	2199	2201	2207	rBV5	785	821	0.03%	0.004%
53	8.228	2210	2220	2235	rBV3	21128	36378	1.41%	0.181%
54	8.312	2235	2246	2283	rBV	682900	1312513	50.83%	6.526%
55	8.746	2376	2381	2384	rVB3	591	524	0.02%	0.003%
56	8.839	2407	2410	2414	rVV3	1149	906	0.04%	0.005%
57	8.858	2414	2416	2421	rVB	842	578	0.02%	0.003%
58	8.929	2436	2438	2443	rBV3	843	693	0.03%	0.003%
59	9.087	2474	2487	2516	rVV	989816	1714893	66.41%	8.527%
60	9.395	2579	2583	2587	rBV3	953	680	0.03%	0.003%
61	9.421	2587	2591	2594	rVV3	755	620	0.02%	0.003%
62	9.505	2614	2617	2623	rVB4	1067	873	0.03%	0.004%
63	9.578	2637	2640	2643	rVB3	920	535	0.02%	0.003%
64	9.704	2677	2679	2684	rVB3	989	839	0.03%	0.004%
65	9.762	2692	2697	2699	rBV3	703	646	0.03%	0.003%
66	9.781	2701	2703	2707	rVB4	848	616	0.02%	0.003%
67	9.845	2717	2723	2726	rVB2	692	776	0.03%	0.004%
68	9.877	2728	2733	2736	rBV3	596	506	0.02%	0.003%
69	9.990	2765	2768	2776	rBV4	502	692	0.03%	0.003%
70	10.025	2776	2779	2782	rBV2	1377	1094	0.04%	0.005%
71	10.080	2792	2796	2799	rBV3	616	478	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031430.D
 Acq On : 23 Apr 2019 12:07
 Operator : JC/SP
 Sample : K2477-19DL 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XC6DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.115	2804	2807	2809	rBV2	725	485	0.02%	0.002%
73	10.228	2839	2842	2846	rVB2	795	687	0.03%	0.003%
74	10.341	2873	2877	2880	rBV2	606	520	0.02%	0.003%
75	10.427	2890	2904	2925	rBV	687259	1129796	43.75%	5.618%
76	10.604	2951	2959	2965	rBV5	1325	2182	0.08%	0.011%
77	10.739	2998	3001	3007	rBV2	778	775	0.03%	0.004%
78	10.778	3007	3013	3015	rBV3	601	642	0.02%	0.003%
79	11.045	3093	3096	3100	rVB2	710	495	0.02%	0.002%
80	11.405	3200	3208	3211	rBV3	1261	1569	0.06%	0.008%
81	11.479	3220	3231	3261	rBV	906557	1504727	58.27%	7.482%
82	11.855	3336	3348	3372	rBV	882159	1494374	57.87%	7.431%
83	12.205	3453	3457	3459	rBV4	870	623	0.02%	0.003%
84	12.353	3500	3503	3507	rBV3	1255	1066	0.04%	0.005%
85	12.402	3514	3518	3521	rBV3	969	702	0.03%	0.003%
86	12.517	3549	3554	3562	rBV3	1109	1431	0.06%	0.007%
87	12.781	3634	3636	3642	rBV3	836	783	0.03%	0.004%
88	12.871	3659	3664	3667	rBV3	1002	1195	0.05%	0.006%
89	12.913	3674	3677	3681	rVB3	1254	1013	0.04%	0.005%
90	13.131	3742	3745	3752	rBV3	1101	846	0.03%	0.004%
91	13.192	3760	3764	3767	rBV2	601	504	0.02%	0.003%
92	13.273	3785	3789	3792	rBV2	1102	916	0.04%	0.005%
93	13.453	3842	3845	3846	rBV2	1234	688	0.03%	0.003%
94	13.546	3871	3874	3880	rBV2	977	806	0.03%	0.004%
95	13.967	4003	4005	4009	rBV3	1163	913	0.04%	0.005%
96	14.032	4020	4025	4029	rBV4	1275	1305	0.05%	0.006%
97	14.286	4102	4104	4107	rBV2	1023	620	0.02%	0.003%
98	14.430	4147	4149	4153	rBV2	764	616	0.02%	0.003%
99	14.807	4262	4266	4270	rBV4	1575	1852	0.07%	0.009%
100	14.877	4286	4288	4295	rVB4	1883	1610	0.06%	0.008%


Sum of corrected areas: 20110542

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031430.D
Acq On : 23 Apr 2019 12:07
Operator : JC/SP
Sample : K2477-19DL 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XC6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

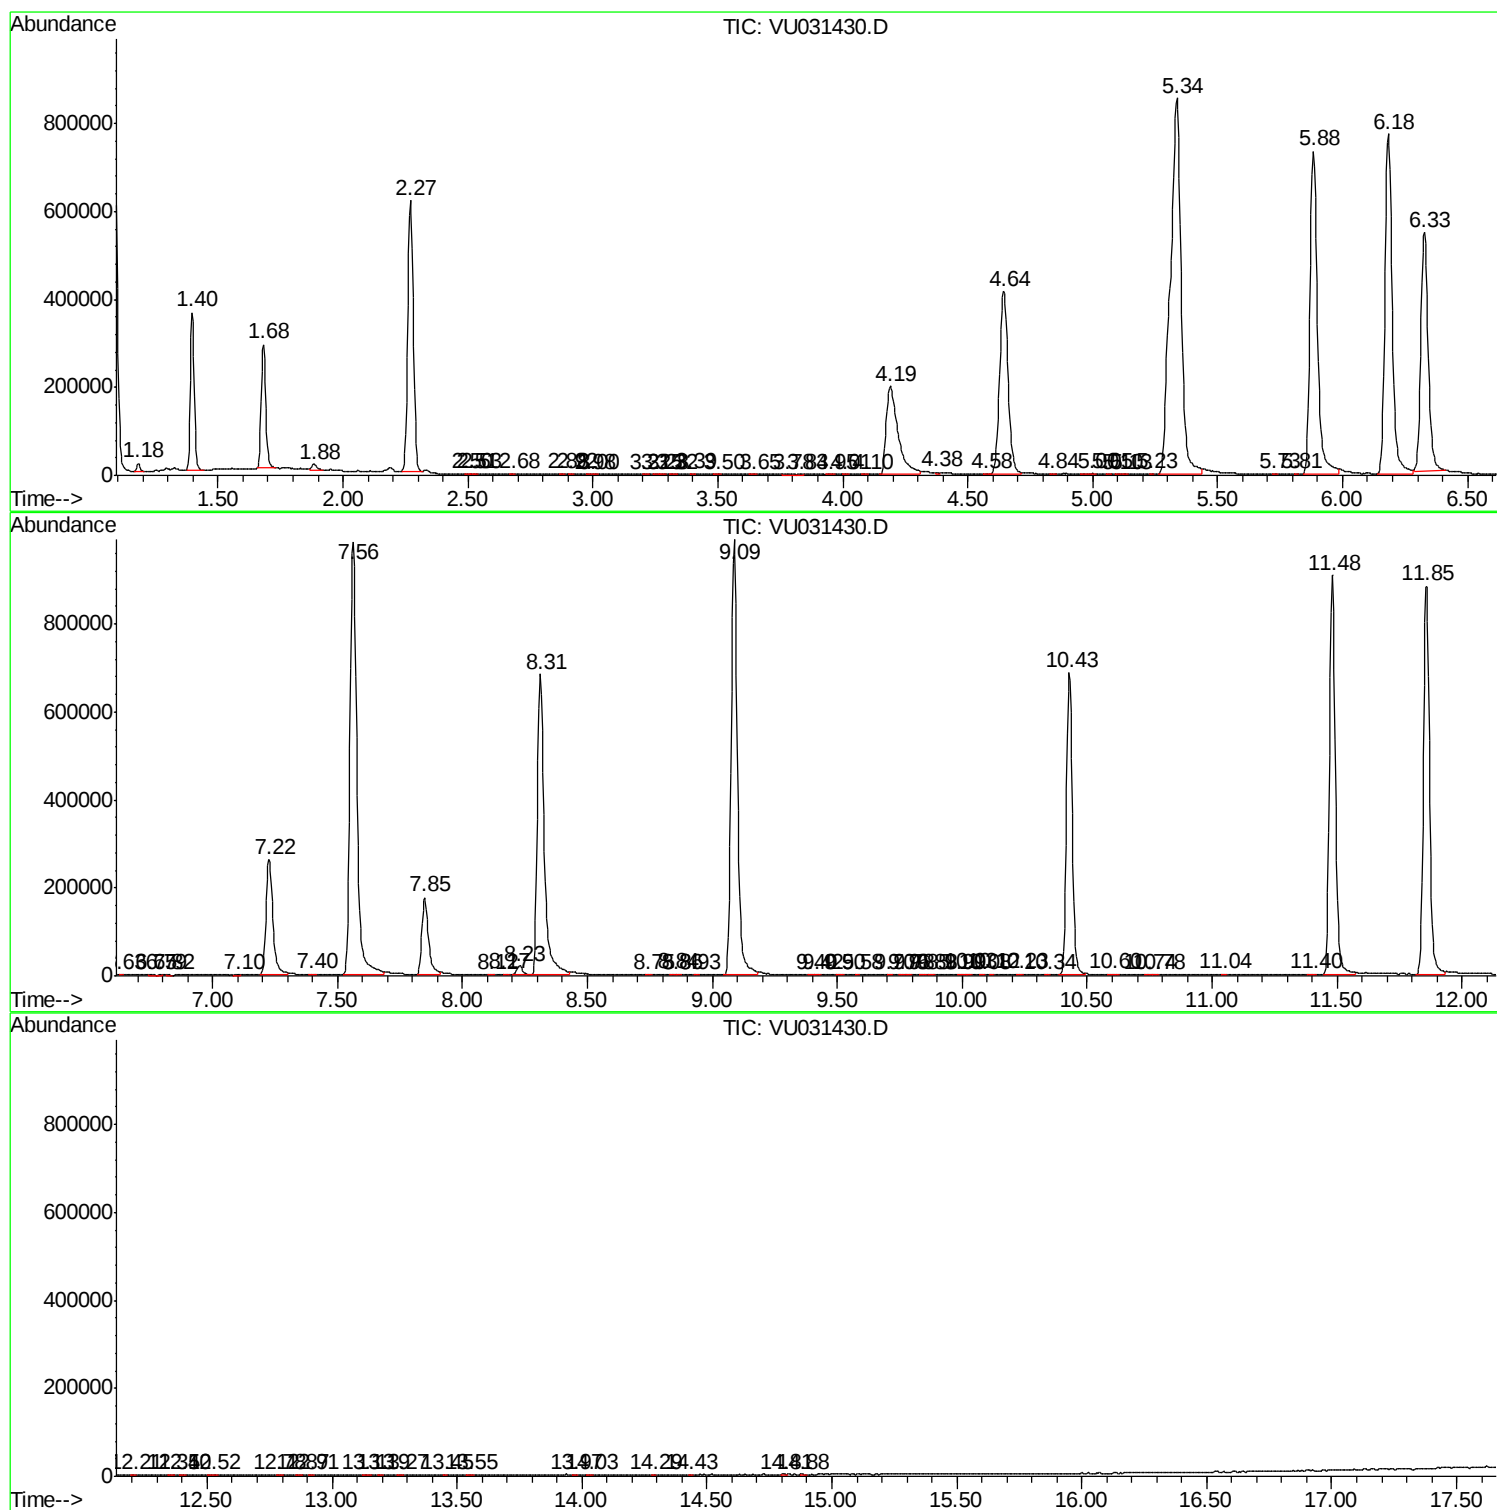

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031430.D
Acq On : 23 Apr 2019 12:07
Operator : JC/SP
Sample : K2477-19DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XC6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031430.D
Acq On : 23 Apr 2019 12:07
Operator : JC/SP
Sample : K2477-19DL 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XC6DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc