

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031431.D
 Acq On : 23 Apr 2019 12:30
 Operator : JC/SP
 Sample : K2478-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB2	17887	18641	0.72%	0.089%
2	1.396	88	95	114	rVB	368405	398249	15.38%	1.897%
3	1.682	176	184	198	rBV	285404	363456	14.04%	1.732%
4	2.270	356	367	380	rBV	627735	950644	36.72%	4.529%
5	2.424	412	415	418	rBV3	1166	752	0.03%	0.004%
6	2.460	424	426	429	rBV4	816	528	0.02%	0.003%
7	2.588	463	466	470	rBV3	804	724	0.03%	0.003%
8	2.637	478	481	487	rVB3	749	705	0.03%	0.003%
9	2.704	493	502	504	rBV8	2359	2980	0.12%	0.014%
10	2.759	515	519	528	rVB4	796	1140	0.04%	0.005%
11	2.833	537	542	545	rVV5	1333	1575	0.06%	0.008%
12	2.894	559	561	566	rVB3	993	601	0.02%	0.003%
13	2.916	566	568	572	rBV	707	632	0.02%	0.003%
14	3.051	605	610	614	rBV3	893	1025	0.04%	0.005%
15	3.074	614	617	622	rVB4	831	793	0.03%	0.004%
16	3.251	669	672	675	rVV2	696	562	0.02%	0.003%
17	3.267	675	677	682	rVV3	787	698	0.03%	0.003%
18	3.302	685	688	690	rVV2	866	571	0.02%	0.003%
19	3.624	784	788	791	rBV2	774	564	0.02%	0.003%
20	3.682	800	806	809	rVB2	565	535	0.02%	0.003%
21	3.765	827	832	836	rVB4	1067	1011	0.04%	0.005%
22	3.817	843	848	853	rBV3	1196	1462	0.06%	0.007%
23	3.862	859	862	866	rVB2	740	543	0.02%	0.003%
24	3.894	866	872	875	rVB2	595	580	0.02%	0.003%
25	3.936	879	885	889	rBV3	974	1178	0.05%	0.006%
26	3.977	894	898	901	rBV2	902	785	0.03%	0.004%
27	4.067	921	926	928	rBV2	626	512	0.02%	0.002%
28	4.103	932	937	938	rBV2	731	598	0.02%	0.003%
29	4.193	952	965	1014	rBV	203887	699519	27.02%	3.333%
30	4.643	1083	1105	1130	rBV	420900	995670	38.46%	4.743%
31	4.865	1171	1174	1176	rBV3	1138	867	0.03%	0.004%
32	4.990	1209	1213	1219	rBV7	1188	1802	0.07%	0.009%
33	5.055	1230	1233	1239	rVB4	1169	1044	0.04%	0.005%
34	5.083	1239	1242	1244	rBV2	1202	881	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031431.D
 Acq On : 23 Apr 2019 12:30
 Operator : JC/SP
 Sample : K2478-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.174	1265	1270	1272	rBV2	665	506	0.02%	0.002%
36	5.338	1295	1321	1360	rBV2	850355	2589156	100.00%	12.335%
37	5.723	1438	1441	1443	rBV3	1012	648	0.03%	0.003%
38	5.781	1457	1459	1467	rVB6	1425	1050	0.04%	0.005%
39	5.820	1467	1471	1474	rVB3	767	556	0.02%	0.003%
40	5.884	1474	1491	1522	rBV	744230	1540336	59.49%	7.338%
41	6.183	1569	1584	1615	rBV	851129	1724325	66.60%	8.215%
42	6.328	1616	1629	1652	rVV	537484	1083543	41.85%	5.162%
43	6.585	1705	1709	1712	rBV3	803	686	0.03%	0.003%
44	6.643	1725	1727	1730	rBV	1020	589	0.02%	0.003%
45	6.704	1743	1746	1755	rVB5	861	1135	0.04%	0.005%
46	7.077	1859	1862	1866	rVB2	1064	813	0.03%	0.004%
47	7.122	1870	1876	1878	rBV3	726	632	0.02%	0.003%
48	7.225	1896	1908	1933	rBV	295478	562097	21.71%	2.678%
49	7.562	1999	2013	2064	rBV	1056906	2000181	77.25%	9.529%
50	7.849	2090	2102	2124	rBV	188311	351015	13.56%	1.672%
51	8.016	2151	2154	2159	rVB5	1377	1073	0.04%	0.005%
52	8.087	2172	2176	2180	rBV3	786	741	0.03%	0.004%
53	8.180	2198	2205	2209	rBV5	1331	1788	0.07%	0.009%
54	8.228	2209	2220	2234	rBV3	39849	73033	2.82%	0.348%
55	8.312	2235	2246	2280	rBV	742130	1410687	54.48%	6.721%
56	8.736	2376	2378	2381	rVB2	1146	692	0.03%	0.003%
57	8.775	2387	2390	2392	rBV3	963	687	0.03%	0.003%
58	8.858	2412	2416	2421	rVB4	1070	1006	0.04%	0.005%
59	8.980	2450	2454	2462	rVB3	1466	1881	0.07%	0.009%
60	9.087	2471	2487	2524	rBV	1067386	1854185	71.61%	8.833%
61	9.392	2578	2582	2585	rVB4	1299	956	0.04%	0.005%
62	9.559	2632	2634	2638	rVB2	1040	609	0.02%	0.003%
63	9.595	2638	2645	2647	rBV3	1047	1126	0.04%	0.005%
64	9.829	2715	2718	2722	rVB3	755	544	0.02%	0.003%
65	9.858	2723	2727	2730	rBV2	793	612	0.02%	0.003%
66	10.074	2792	2794	2798	rVB	825	530	0.02%	0.003%
67	10.157	2815	2820	2823	rBV2	1174	1323	0.05%	0.006%
68	10.318	2866	2870	2872	rVB2	591	494	0.02%	0.002%
69	10.363	2881	2884	2891	rBV3	776	849	0.03%	0.004%
70	10.427	2891	2904	2924	rBV	752329	1241771	47.96%	5.916%
71	10.646	2970	2972	2980	rBV5	893	863	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031431.D
 Acq On : 23 Apr 2019 12:30
 Operator : JC/SP
 Sample : K2478-08DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XG1DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	11.045	3093	3096	3099	rVB2	1481	846	0.03%	0.004%
73	11.080	3104	3107	3112	rVV5	884	698	0.03%	0.003%
74	11.292	3168	3173	3176	rBV2	765	816	0.03%	0.004%
75	11.353	3188	3192	3195	rBV2	990	721	0.03%	0.003%
76	11.376	3195	3199	3203	rBV3	615	676	0.03%	0.003%
77	11.482	3219	3232	3251	rBV	925394	1506864	58.20%	7.179%
78	11.855	3336	3348	3368	rBV	934929	1556312	60.11%	7.414%
79	12.302	3481	3487	3490	rVB6	1186	1024	0.04%	0.005%
80	12.620	3582	3586	3590	rBV4	774	644	0.02%	0.003%
81	12.643	3590	3593	3596	rBV3	715	501	0.02%	0.002%
82	12.832	3646	3652	3656	rVB3	1202	1345	0.05%	0.006%
83	12.858	3656	3660	3663	rBV3	668	780	0.03%	0.004%
84	12.910	3674	3676	3679	rBV3	802	510	0.02%	0.002%
85	13.054	3718	3721	3723	rBV2	971	717	0.03%	0.003%
86	13.122	3739	3742	3743	rBV2	927	508	0.02%	0.002%
87	13.144	3747	3749	3752	rVV2	1171	668	0.03%	0.003%
88	13.318	3799	3803	3805	rBV2	884	564	0.02%	0.003%
89	13.463	3843	3848	3850	rBV2	1171	1077	0.04%	0.005%
90	14.180	4068	4071	4076	rVB2	1201	1029	0.04%	0.005%
91	14.295	4104	4107	4111	rBV2	929	745	0.03%	0.004%
92	14.623	4206	4209	4212	rBV3	990	647	0.02%	0.003%
93	14.649	4213	4217	4219	rBV	1366	1285	0.05%	0.006%
94	14.720	4236	4239	4241	rBV2	1357	857	0.03%	0.004%
95	14.868	4283	4285	4288	rBV2	1008	641	0.02%	0.003%
96	14.964	4313	4315	4319	rBV5	1038	799	0.03%	0.004%
97	14.983	4319	4321	4324	rVV2	1784	1008	0.04%	0.005%
98	15.118	4360	4363	4366	rVB3	2005	1237	0.05%	0.006%
99	15.212	4389	4392	4395	rBV4	1963	1338	0.05%	0.006%
100	15.565	4499	4502	4506	rBV2	1897	1177	0.05%	0.006%


Sum of corrected areas: 20990579

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031431.D
Acq On : 23 Apr 2019 12:30
Operator : JC/SP
Sample : K2478-08DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

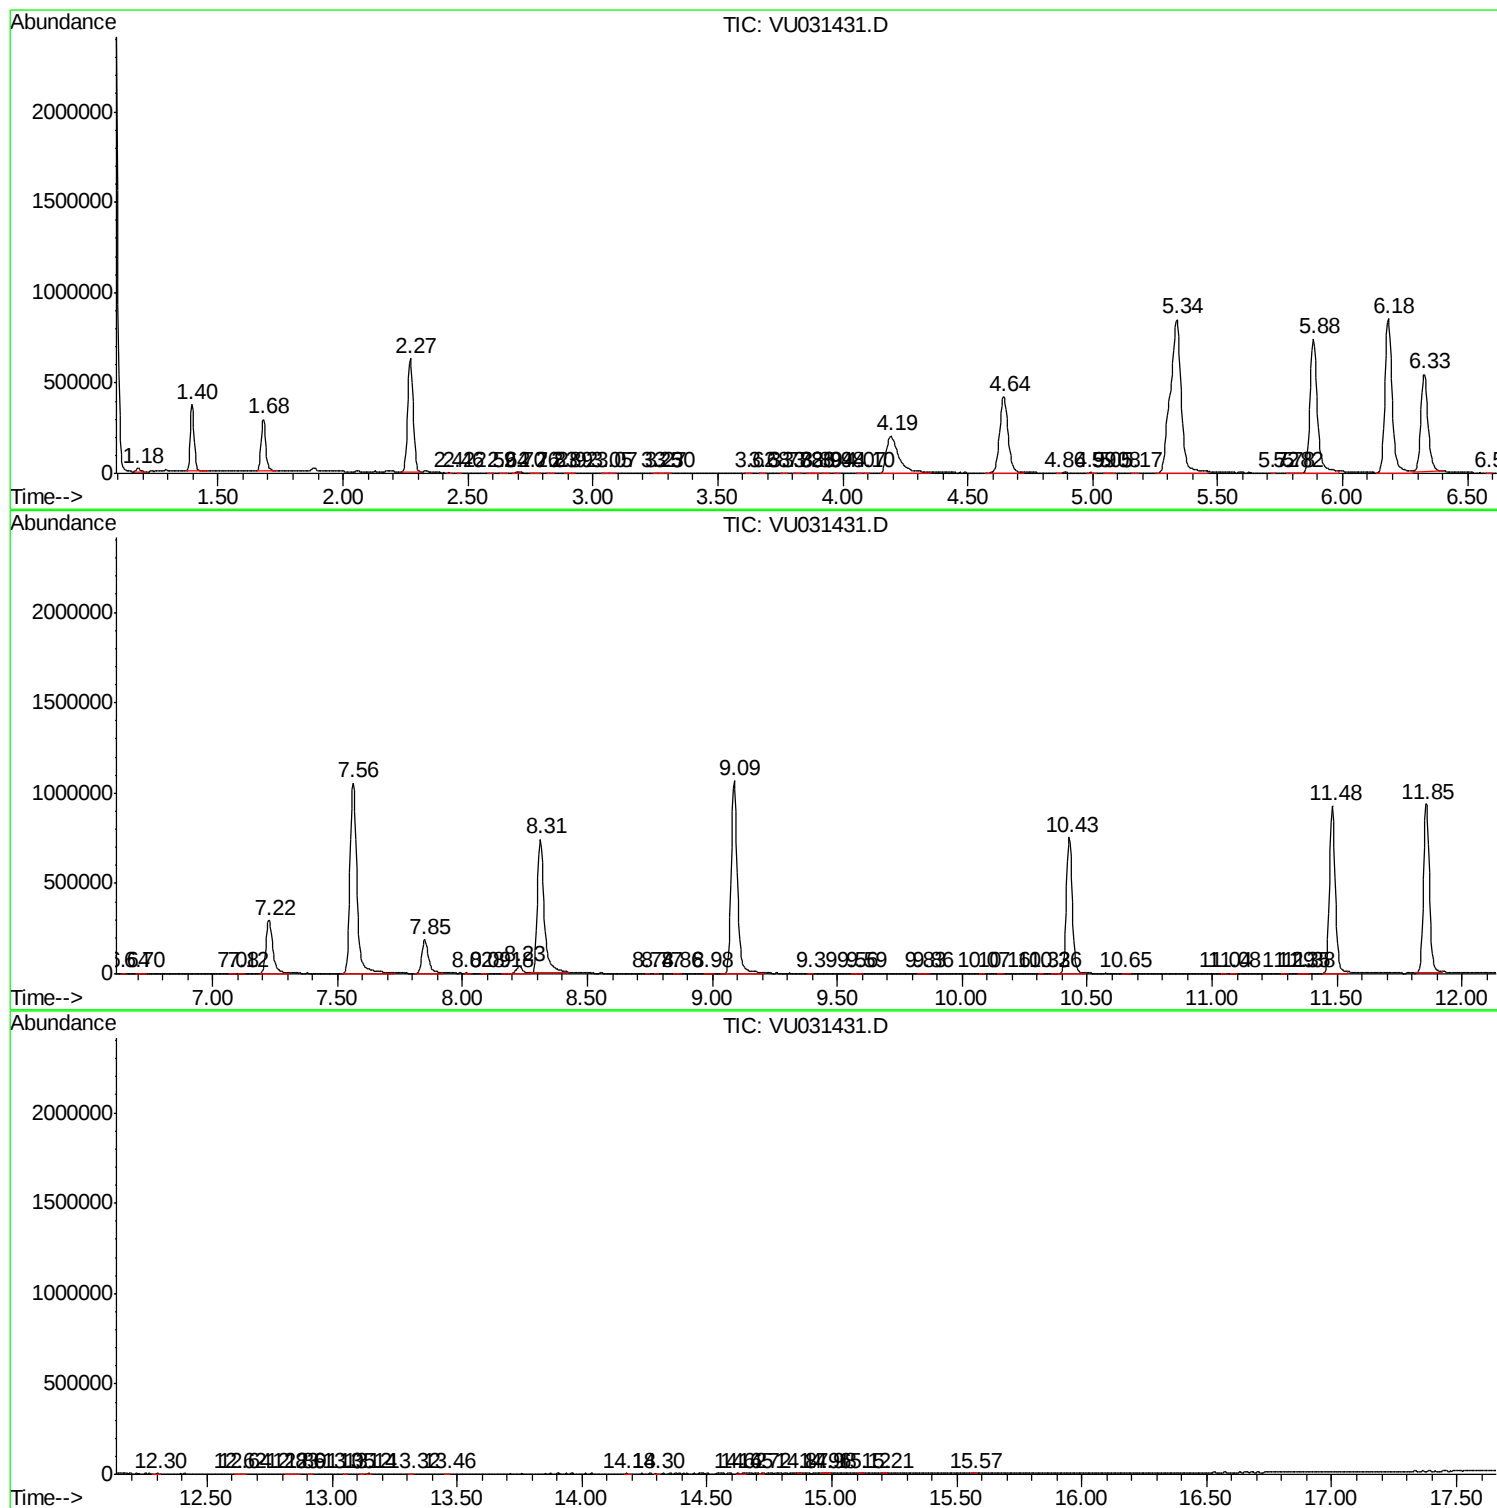

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031431.D
Acq On : 23 Apr 2019 12:30
Operator : JC/SP
Sample : K2478-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031431.D
Acq On : 23 Apr 2019 12:30
Operator : JC/SP
Sample : K2478-08DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XG1DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc