

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031433.D
 Acq On : 23 Apr 2019 13:16
 Operator : JC/SP
 Sample : K2428-13 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	37	rVB	18704	18134	0.52%	0.080%
2	1.283	55	60	67	rBV3	20578	22059	0.63%	0.097%
3	1.395	88	95	113	rVB	360179	398746	11.34%	1.756%
4	1.682	176	184	197	rBV	284235	359031	10.21%	1.581%
5	1.884	242	247	256	rVB	29313	37807	1.08%	0.166%
6	2.270	356	367	381	rVB	606946	928405	26.40%	4.088%
7	2.434	415	418	420	rVB4	1048	533	0.02%	0.002%
8	2.550	450	454	456	rBV3	1186	931	0.03%	0.004%
9	2.575	460	462	466	rVB4	1142	665	0.02%	0.003%
10	2.701	494	501	506	rVV6	2884	3786	0.11%	0.017%
11	2.807	530	534	537	rBV3	769	556	0.02%	0.002%
12	2.839	539	544	550	rVB4	1059	1495	0.04%	0.007%
13	3.157	641	643	648	rVB3	881	734	0.02%	0.003%
14	3.186	648	652	655	rBV3	586	543	0.02%	0.002%
15	3.225	660	664	667	rBV	815	589	0.02%	0.003%
16	3.460	732	737	743	rVB5	756	1005	0.03%	0.004%
17	3.579	772	774	777	rVB	836	520	0.01%	0.002%
18	3.646	792	795	799	rBV2	1014	727	0.02%	0.003%
19	3.810	842	846	849	rBV2	887	739	0.02%	0.003%
20	4.016	904	910	917	rVB4	776	962	0.03%	0.004%
21	4.128	940	945	947	rBV	752	613	0.02%	0.003%
22	4.190	951	964	1006	rBV2	211296	695225	19.77%	3.061%
23	4.463	1047	1049	1057	rVB6	901	593	0.02%	0.003%
24	4.643	1088	1105	1128	rBV	416208	987648	28.09%	4.349%
25	4.881	1176	1179	1188	rVB6	2437	2932	0.08%	0.013%
26	4.919	1188	1191	1193	rVB3	824	533	0.02%	0.002%
27	4.987	1203	1212	1217	rBV8	1756	2930	0.08%	0.013%
28	5.054	1227	1233	1235	rBV5	1022	821	0.02%	0.004%
29	5.116	1247	1252	1253	rBV3	740	653	0.02%	0.003%
30	5.167	1264	1268	1273	rVB4	810	748	0.02%	0.003%
31	5.337	1297	1321	1359	rBV2	816326	2475222	70.39%	10.899%
32	5.620	1407	1409	1414	rVB5	1298	755	0.02%	0.003%
33	5.746	1443	1448	1453	rBV7	1317	1652	0.05%	0.007%
34	5.768	1453	1455	1460	rVB4	1443	976	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031433.D
 Acq On : 23 Apr 2019 13:16
 Operator : JC/SP
 Sample : K2428-13 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.791	1460	1462	1466	rBV2	532	473	0.01%	0.002%
36	5.884	1477	1491	1530	rBV	750767	1586119	45.10%	6.984%
37	6.128	1565	1567	1569	rBV2	1058	569	0.02%	0.003%
38	6.183	1569	1584	1611	rBV	1756361	3516524	100.00%	15.484%
39	6.328	1617	1629	1664	rVB	551089	1159905	32.98%	5.107%
40	6.681	1736	1739	1740	rVV2	816	481	0.01%	0.002%
41	6.788	1766	1772	1773	rBV2	872	914	0.03%	0.004%
42	6.820	1778	1782	1785	rBV3	674	489	0.01%	0.002%
43	6.913	1807	1811	1815	rBV2	901	925	0.03%	0.004%
44	6.942	1815	1820	1824	rVB5	594	682	0.02%	0.003%
45	7.016	1838	1843	1845	rBV2	969	803	0.02%	0.004%
46	7.048	1850	1853	1855	rVV2	710	502	0.01%	0.002%
47	7.093	1863	1867	1874	rBV3	846	989	0.03%	0.004%
48	7.125	1874	1877	1883	rBV	731	794	0.02%	0.003%
49	7.225	1895	1908	1942	rBV	294508	569253	16.19%	2.507%
50	7.431	1968	1972	1974	rBV5	1075	921	0.03%	0.004%
51	7.562	1999	2013	2055	rBV	1089879	2020416	57.45%	8.897%
52	7.849	2091	2102	2130	rBV	202058	376932	10.72%	1.660%
53	8.173	2199	2203	2204	rBV	1035	605	0.02%	0.003%
54	8.225	2209	2219	2235	rBV2	65132	118385	3.37%	0.521%
55	8.312	2235	2246	2280	rBV	786494	1497702	42.59%	6.595%
56	8.640	2345	2348	2351	rVB4	867	558	0.02%	0.002%
57	8.662	2351	2355	2362	rVB4	1347	1470	0.04%	0.006%
58	8.922	2433	2436	2441	rVV4	770	706	0.02%	0.003%
59	9.006	2457	2462	2465	rBV2	952	948	0.03%	0.004%
60	9.086	2472	2487	2523	rBV	1041543	1825517	51.91%	8.038%
61	9.276	2544	2546	2552	rVB5	1345	1304	0.04%	0.006%
62	9.540	2625	2628	2630	rBV2	863	470	0.01%	0.002%
63	9.553	2630	2632	2637	rVB4	748	598	0.02%	0.003%
64	9.643	2654	2660	2662	rBV2	483	550	0.02%	0.002%
65	9.697	2673	2677	2681	rVB2	629	500	0.01%	0.002%
66	9.730	2681	2687	2692	rBV4	1107	1106	0.03%	0.005%
67	9.758	2692	2696	2699	rVB2	1064	917	0.03%	0.004%
68	9.791	2699	2706	2711	rBV3	1486	2018	0.06%	0.009%
69	9.813	2711	2713	2718	rVV2	760	584	0.02%	0.003%
70	9.955	2751	2757	2759	rBV3	762	582	0.02%	0.003%
71	10.054	2783	2788	2791	rBV3	1564	1457	0.04%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031433.D
 Acq On : 23 Apr 2019 13:16
 Operator : JC/SP
 Sample : K2428-13 40X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X13

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.167	2819	2823	2824	rBV2	731	530	0.02%	0.002%
73	10.427	2890	2904	2923	rBV	701900	1144088	32.53%	5.038%
74	10.781	3011	3014	3017	rVV2	737	498	0.01%	0.002%
75	10.865	3037	3040	3045	rBV2	710	485	0.01%	0.002%
76	11.012	3083	3086	3087	rBV2	956	514	0.01%	0.002%
77	11.051	3094	3098	3101	rBV2	705	684	0.02%	0.003%
78	11.086	3106	3109	3113	rVV3	973	788	0.02%	0.003%
79	11.119	3116	3119	3121	rVV2	1021	625	0.02%	0.003%
80	11.366	3192	3196	3199	rBV2	754	566	0.02%	0.002%
81	11.414	3208	3211	3219	rBV4	863	950	0.03%	0.004%
82	11.479	3219	3231	3262	rBV	867502	1442459	41.02%	6.352%
83	11.858	3336	3349	3375	rBV	867252	1461593	41.56%	6.436%
84	12.276	3476	3479	3482	rBV3	824	638	0.02%	0.003%
85	12.324	3489	3494	3496	rBV3	977	699	0.02%	0.003%
86	12.344	3496	3500	3503	rBV3	730	724	0.02%	0.003%
87	12.379	3509	3511	3516	rBV4	790	607	0.02%	0.003%
88	12.543	3559	3562	3564	rBV3	806	487	0.01%	0.002%
89	12.559	3565	3567	3572	rVB2	1043	817	0.02%	0.004%
90	12.607	3579	3582	3585	rBV4	914	874	0.02%	0.004%
91	12.649	3592	3595	3597	rBV2	882	486	0.01%	0.002%
92	12.697	3606	3610	3611	rBV	867	622	0.02%	0.003%
93	12.749	3622	3626	3628	rBV2	929	730	0.02%	0.003%
94	13.051	3717	3720	3723	rBV2	990	619	0.02%	0.003%
95	13.192	3760	3764	3768	rBV4	619	546	0.02%	0.002%
96	13.752	3933	3938	3940	rBV2	1387	1131	0.03%	0.005%
97	13.787	3946	3949	3952	rVB2	924	580	0.02%	0.003%
98	13.813	3952	3957	3959	rBV2	1166	999	0.03%	0.004%
99	14.684	4225	4228	4231	rBV	1275	1044	0.03%	0.005%
100	14.961	4309	4314	4316	rBV3	1560	1675	0.05%	0.007%


Sum of corrected areas: 22709994

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031433.D
Acq On : 23 Apr 2019 13:16
Operator : JC/SP
Sample : K2428-13 40X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

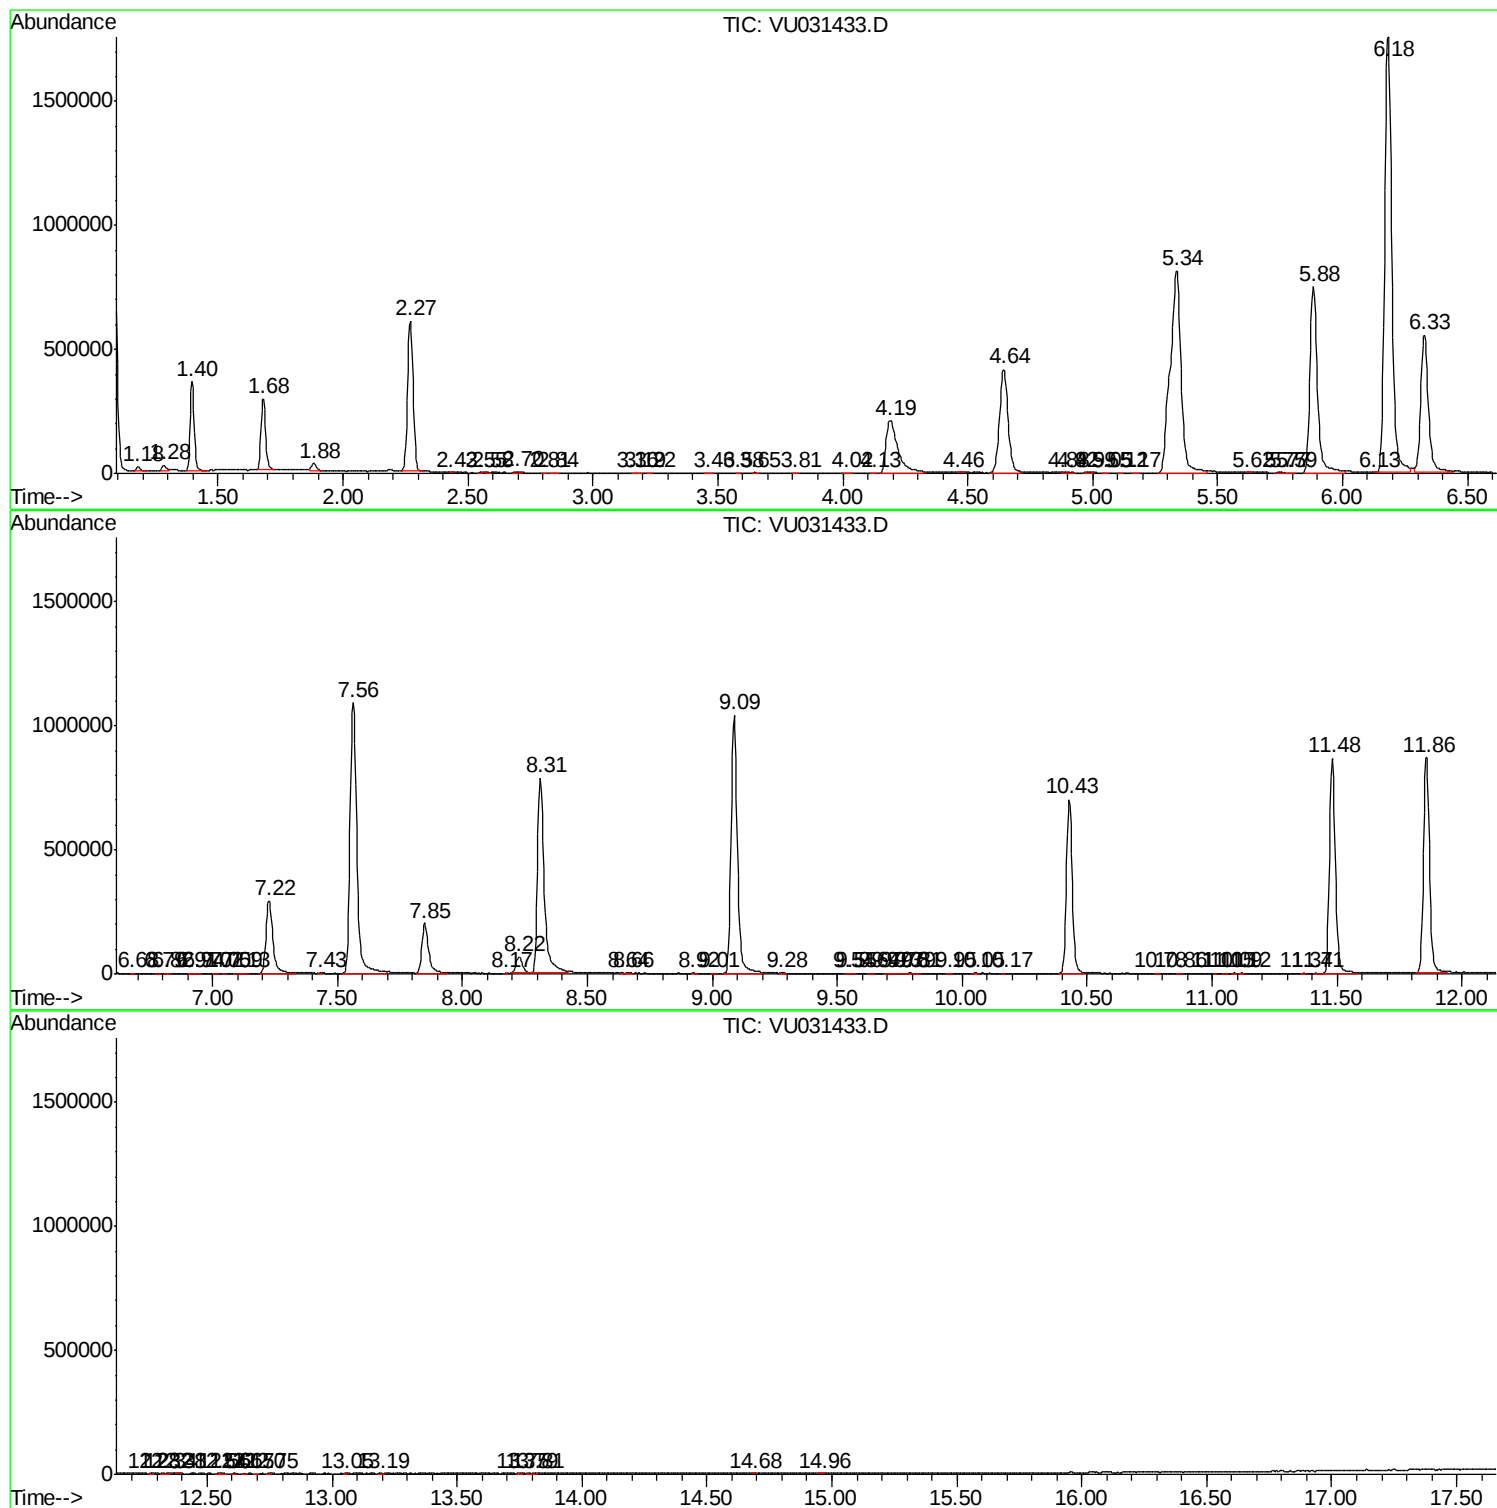

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031433.D
Acq On : 23 Apr 2019 13:16
Operator : JC/SP
Sample : K2428-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031433.D
Acq On : 23 Apr 2019 13:16
Operator : JC/SP
Sample : K2428-13 40X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X13

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc