

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031435.D
 Acq On : 23 Apr 2019 14:03
 Operator : JC/SP
 Sample : K2477-01DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rBV2	16971	16695	0.39%	0.068%
2	1.395	88	95	110	rVB	385803	421616	9.82%	1.725%
3	1.682	176	184	195	rBV	293982	373312	8.70%	1.527%
4	1.881	241	246	256	rVB2	35217	48739	1.14%	0.199%
5	2.270	356	367	381	rVV	635427	982033	22.88%	4.017%
6	2.328	381	385	399	rVB4	8243	13277	0.31%	0.054%
7	2.450	420	423	427	rBV4	1211	1123	0.03%	0.005%
8	2.701	495	501	504	rBV5	1660	1869	0.04%	0.008%
9	2.865	549	552	557	rBV4	736	877	0.02%	0.004%
10	2.971	582	585	588	rBV3	913	715	0.02%	0.003%
11	3.161	641	644	650	rBV3	740	905	0.02%	0.004%
12	3.186	650	652	658	rVB3	781	779	0.02%	0.003%
13	3.215	658	661	667	rBV4	622	729	0.02%	0.003%
14	3.289	681	684	687	rVB3	791	557	0.01%	0.002%
15	3.456	733	736	741	rBV3	791	607	0.01%	0.002%
16	3.646	793	795	798	rBV2	865	632	0.01%	0.003%
17	3.701	809	812	819	rBV3	1058	1123	0.03%	0.005%
18	3.804	842	844	854	rVB3	829	1120	0.03%	0.005%
19	3.993	901	903	907	rVB3	688	505	0.01%	0.002%
20	4.190	947	964	993	rBV	214726	699288	16.29%	2.861%
21	4.643	1087	1105	1134	rVV2	424754	1020307	23.77%	4.174%
22	4.823	1158	1161	1166	rVB4	866	627	0.01%	0.003%
23	4.993	1204	1214	1217	rBV3	2355	3381	0.08%	0.014%
24	5.141	1254	1260	1267	rBV5	792	1147	0.03%	0.005%
25	5.180	1270	1272	1278	rVB4	635	551	0.01%	0.002%
26	5.209	1278	1281	1286	rVB4	1145	857	0.02%	0.004%
27	5.337	1296	1321	1364	rBV2	883868	2692723	62.73%	11.015%
28	5.665	1420	1423	1429	rVB6	1945	1833	0.04%	0.007%
29	5.717	1437	1439	1444	rVB2	1319	912	0.02%	0.004%
30	5.755	1448	1451	1453	rBV2	913	588	0.01%	0.002%
31	5.807	1465	1467	1472	rBV3	950	643	0.01%	0.003%
32	5.884	1477	1491	1530	rBV	752672	1587541	36.98%	6.494%
33	6.183	1568	1584	1616	rBV	2143697	4292586	100.00%	17.560%
34	6.328	1617	1629	1650	rVB	567935	1163602	27.11%	4.760%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031435.D
 Acq On : 23 Apr 2019 14:03
 Operator : JC/SP
 Sample : K2477-01DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	6.521	1687	1689	1693	rVB5	2074	1368	0.03%	0.006%
36	6.588	1707	1710	1713	rBV4	1358	862	0.02%	0.004%
37	6.701	1743	1745	1752	rVB3	1390	985	0.02%	0.004%
38	6.733	1752	1755	1758	rVB2	883	634	0.01%	0.003%
39	6.752	1758	1761	1764	rBV3	1018	796	0.02%	0.003%
40	6.852	1787	1792	1795	rBV3	1252	1275	0.03%	0.005%
41	6.910	1807	1810	1816	rVB6	733	798	0.02%	0.003%
42	6.955	1819	1824	1825	rBV3	1087	816	0.02%	0.003%
43	6.977	1828	1831	1836	rBV3	764	737	0.02%	0.003%
44	7.128	1870	1878	1881	rBV2	838	1034	0.02%	0.004%
45	7.167	1886	1890	1895	rVB3	965	1016	0.02%	0.004%
46	7.225	1895	1908	1939	rBV	311509	601250	14.01%	2.460%
47	7.562	1999	2013	2059	rVV	1119480	2089945	48.69%	8.550%
48	7.849	2091	2102	2128	rBV	205722	382333	8.91%	1.564%
49	8.083	2172	2175	2179	rBV3	1107	825	0.02%	0.003%
50	8.167	2198	2201	2207	rVB4	854	857	0.02%	0.004%
51	8.225	2207	2219	2235	rBV2	99173	179918	4.19%	0.736%
52	8.312	2235	2246	2287	rVV	801323	1534771	35.75%	6.278%
53	8.913	2431	2433	2439	rVB2	746	599	0.01%	0.002%
54	9.086	2474	2487	2517	rBV	1077072	1877711	43.74%	7.681%
55	9.469	2603	2606	2611	rVB4	785	636	0.01%	0.003%
56	9.495	2611	2614	2619	rBV2	542	483	0.01%	0.002%
57	9.623	2652	2654	2658	rBV2	885	699	0.02%	0.003%
58	9.652	2662	2663	2668	rVB2	1115	701	0.02%	0.003%
59	9.701	2675	2678	2681	rBV4	813	573	0.01%	0.002%
60	9.768	2696	2699	2701	rBV	722	572	0.01%	0.002%
61	9.916	2736	2745	2750	rVB5	946	1514	0.04%	0.006%
62	9.938	2750	2752	2758	rBV3	883	810	0.02%	0.003%
63	9.967	2758	2761	2766	rBV3	866	749	0.02%	0.003%
64	10.057	2786	2789	2791	rBV2	681	480	0.01%	0.002%
65	10.180	2824	2827	2830	rBV3	1079	668	0.02%	0.003%
66	10.209	2830	2836	2837	rBV2	951	713	0.02%	0.003%
67	10.266	2851	2854	2857	rBV2	771	515	0.01%	0.002%
68	10.283	2857	2859	2862	rVB	1160	658	0.02%	0.003%
69	10.299	2862	2864	2867	rBV	814	619	0.01%	0.003%
70	10.427	2892	2904	2929	rVV	770901	1259501	29.34%	5.152%
71	10.614	2959	2962	2965	rBV3	895	525	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031435.D
 Acq On : 23 Apr 2019 14:03
 Operator : JC/SP
 Sample : K2477-01DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X35DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.633	2965	2968	2971	rBV4	707	546	0.01%	0.002%
73	10.710	2986	2992	2993	rBV2	1216	992	0.02%	0.004%
74	10.848	3033	3035	3040	rVB2	1176	952	0.02%	0.004%
75	10.874	3040	3043	3046	rVB2	808	598	0.01%	0.002%
76	10.919	3046	3057	3060	rBV2	1080	1668	0.04%	0.007%
77	11.006	3082	3084	3092	rVB4	945	815	0.02%	0.003%
78	11.051	3095	3098	3101	rBV3	1073	830	0.02%	0.003%
79	11.144	3124	3127	3130	rVB2	763	478	0.01%	0.002%
80	11.344	3186	3189	3192	rVB2	1015	655	0.02%	0.003%
81	11.366	3192	3196	3203	rBV4	867	1213	0.03%	0.005%
82	11.479	3219	3231	3254	rBV	919682	1515620	35.31%	6.200%
83	11.688	3294	3296	3299	rBV3	1383	770	0.02%	0.003%
84	11.855	3336	3348	3382	rBV	961804	1620582	37.75%	6.629%
85	12.080	3415	3418	3422	rBV5	1670	1585	0.04%	0.006%
86	12.225	3459	3463	3466	rBV4	1237	1002	0.02%	0.004%
87	12.334	3495	3497	3500	rBV3	900	627	0.01%	0.003%
88	12.395	3514	3516	3517	rBV	1198	517	0.01%	0.002%
89	12.700	3609	3611	3614	rBV2	1014	646	0.02%	0.003%
90	13.048	3715	3719	3722	rBV2	1167	1012	0.02%	0.004%
91	13.183	3759	3761	3768	rVB4	1176	1088	0.03%	0.004%
92	13.221	3768	3773	3776	rBV3	1255	1305	0.03%	0.005%
93	13.369	3815	3819	3822	rBV2	1446	1547	0.04%	0.006%
94	13.990	4009	4012	4016	rBV3	701	601	0.01%	0.002%
95	14.151	4061	4062	4069	rVB4	858	603	0.01%	0.002%
96	14.675	4221	4225	4228	rBV3	1185	982	0.02%	0.004%
97	14.720	4235	4239	4241	rBV3	1132	822	0.02%	0.003%
98	14.758	4247	4251	4255	rBV4	1440	1601	0.04%	0.007%
99	15.337	4429	4431	4435	rVB3	1990	1005	0.02%	0.004%
100	15.511	4480	4485	4488	rBV6	1511	1821	0.04%	0.007%


Sum of corrected areas: 24445228

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031435.D
Acq On : 23 Apr 2019 14:03
Operator : JC/SP
Sample : K2477-01DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X35DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

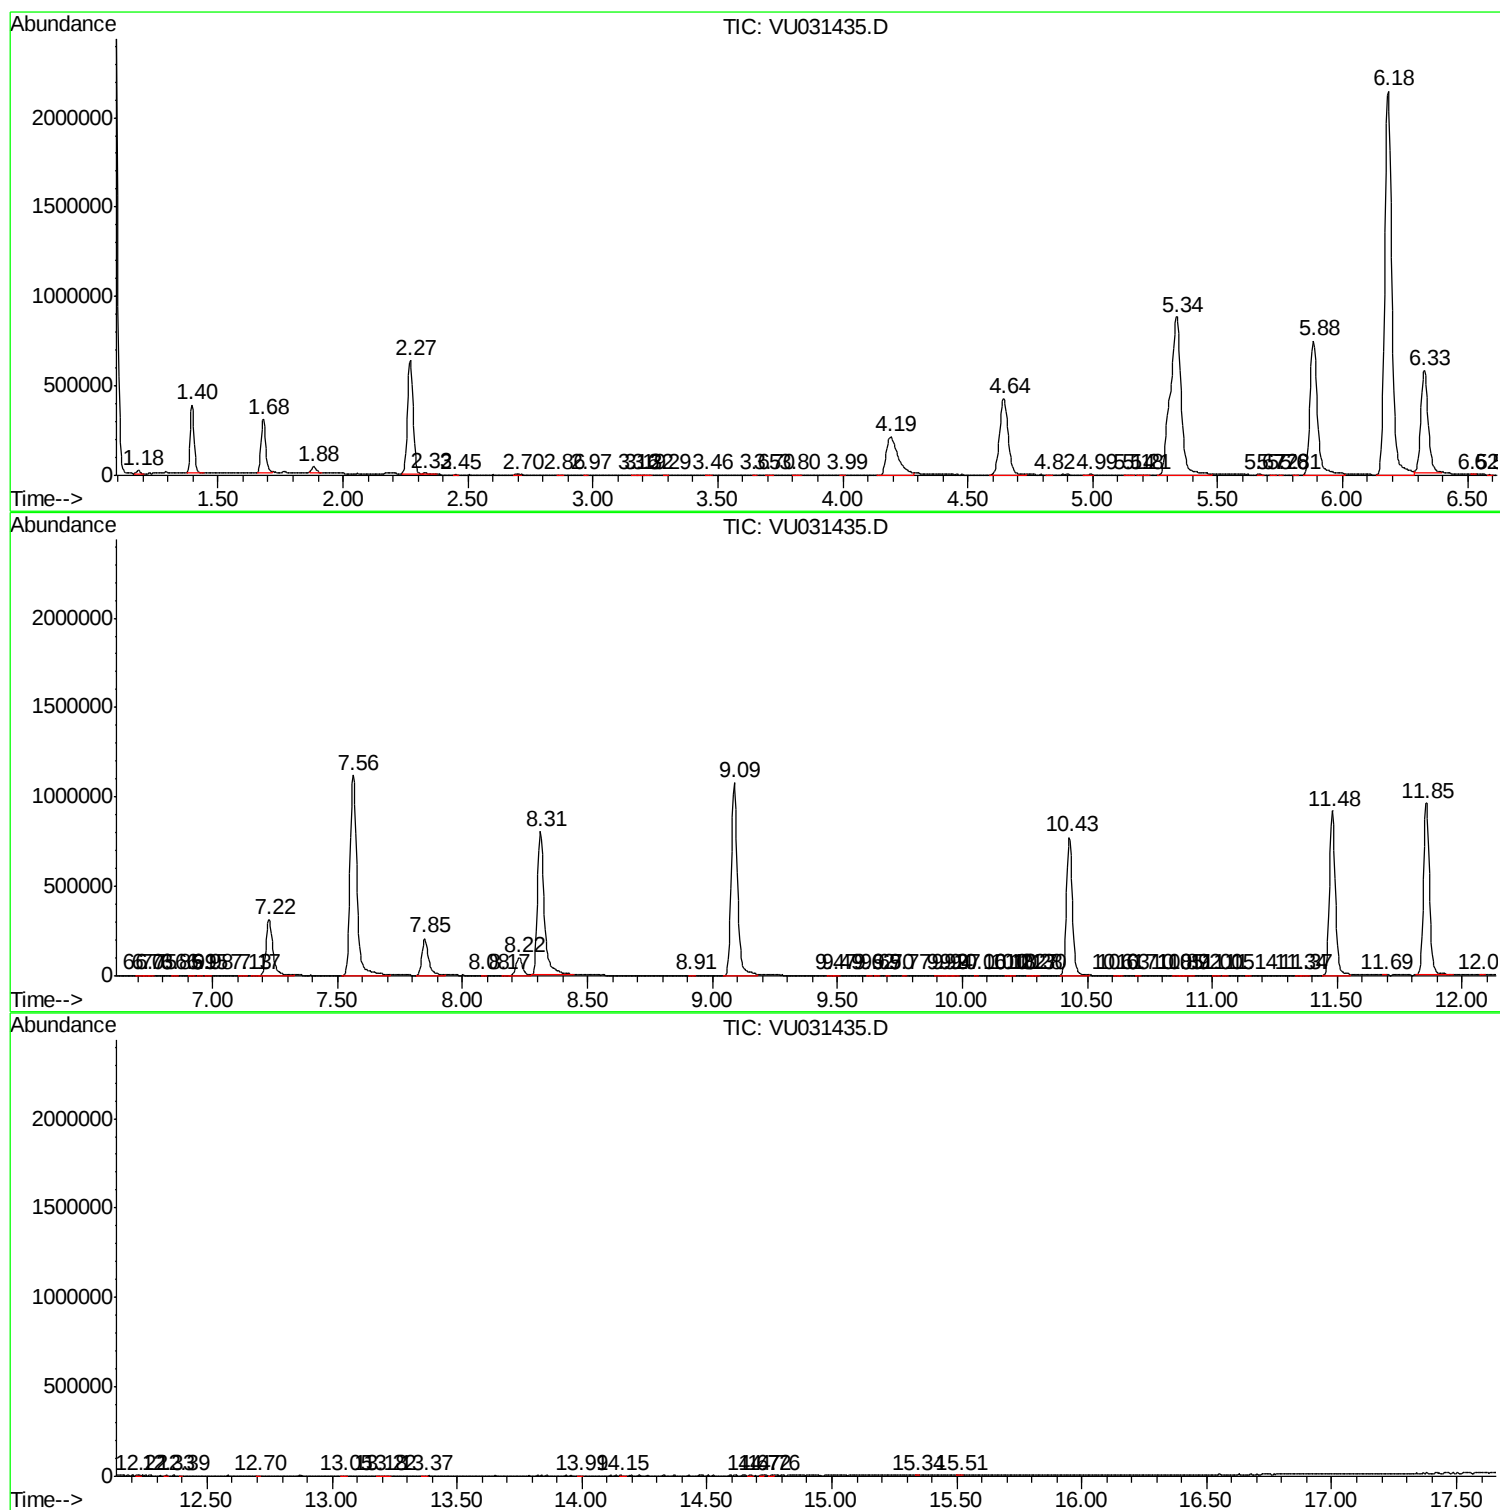

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031435.D
Acq On : 23 Apr 2019 14:03
Operator : JC/SP
Sample : K2477-01DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X35DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031435.D
Acq On : 23 Apr 2019 14:03
Operator : JC/SP
Sample : K2477-01DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X35DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc