

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031453.D
 Acq On : 23 Apr 2019 21:49
 Operator : JC/SP
 Sample : K2536-04DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rVB2	26843	26421	1.06%	0.125%
2	1.286	56	61	67	rVB2	16403	17776	0.71%	0.084%
3	1.396	87	95	107	rBV	322443	351865	14.08%	1.668%
4	1.678	175	183	198	rBV	278194	348558	13.94%	1.653%
5	1.881	241	246	259	rVB	24320	33838	1.35%	0.160%
6	2.267	355	366	379	rVB	571787	862645	34.51%	4.090%
7	2.408	408	410	413	rVB2	1132	571	0.02%	0.003%
8	2.473	424	430	433	rBV4	2482	2688	0.11%	0.013%
9	2.518	439	444	446	rBV4	1664	1595	0.06%	0.008%
10	2.698	493	500	503	rBV7	1980	2784	0.11%	0.013%
11	2.833	531	542	552	rBV4	3348	7385	0.30%	0.035%
12	2.871	552	554	558	rVB3	1165	799	0.03%	0.004%
13	2.894	558	561	563	rBV2	1017	600	0.02%	0.003%
14	2.907	563	565	572	rVB4	593	578	0.02%	0.003%
15	2.945	572	577	578	rBV2	707	652	0.03%	0.003%
16	3.051	607	610	615	rBV2	891	761	0.03%	0.004%
17	3.080	615	619	624	rBV4	672	825	0.03%	0.004%
18	3.177	645	649	652	rVB2	839	700	0.03%	0.003%
19	3.321	691	694	698	rBV2	826	664	0.03%	0.003%
20	3.421	722	725	733	rVB3	856	1071	0.04%	0.005%
21	3.460	733	737	741	rBV	788	669	0.03%	0.003%
22	3.672	801	803	806	rBV	977	620	0.02%	0.003%
23	3.691	806	809	813	rVB2	673	574	0.02%	0.003%
24	3.778	831	836	841	rVB3	565	626	0.03%	0.003%
25	3.817	841	848	852	rBV3	658	892	0.04%	0.004%
26	4.000	899	905	907	rBV3	655	812	0.03%	0.004%
27	4.125	941	944	948	rVB2	802	573	0.02%	0.003%
28	4.186	948	963	1007	rBV	237943	754386	30.18%	3.577%
29	4.402	1021	1030	1047	rVB4	10419	27472	1.10%	0.130%
30	4.643	1087	1105	1132	rBV	412329	972651	38.91%	4.612%
31	4.984	1209	1211	1214	rBV2	1433	707	0.03%	0.003%
32	5.038	1224	1228	1230	rBV3	884	636	0.03%	0.003%
33	5.051	1230	1232	1236	rVB3	1079	693	0.03%	0.003%
34	5.083	1236	1242	1246	rBV5	1273	1308	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031453.D
 Acq On : 23 Apr 2019 21:49
 Operator : JC/SP
 Sample : K2536-04DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.128	1253	1256	1259	rVV2	836	605	0.02%	0.003%
36	5.206	1277	1280	1285	rBV4	892	909	0.04%	0.004%
37	5.334	1297	1320	1358	rBV3	833616	2499773	100.00%	11.853%
38	5.601	1399	1403	1405	rBV4	861	711	0.03%	0.003%
39	5.678	1423	1427	1431	rVB3	1829	1443	0.06%	0.007%
40	5.820	1468	1471	1475	rVB3	792	619	0.02%	0.003%
41	5.881	1477	1490	1529	rBV	796997	1655446	66.22%	7.849%
42	6.183	1569	1584	1615	rBV	891090	1802693	72.11%	8.547%
43	6.328	1616	1629	1660	rVB	535000	1101583	44.07%	5.223%
44	6.498	1681	1682	1686	rVB4	2283	1170	0.05%	0.006%
45	6.524	1686	1690	1697	rBV6	1647	1711	0.07%	0.008%
46	6.707	1742	1747	1751	rVB4	828	713	0.03%	0.003%
47	6.871	1795	1798	1803	rBV3	681	605	0.02%	0.003%
48	6.926	1813	1815	1821	rVB4	1342	1017	0.04%	0.005%
49	7.025	1844	1846	1851	rVB3	942	713	0.03%	0.003%
50	7.054	1851	1855	1858	rBV2	1060	823	0.03%	0.004%
51	7.225	1896	1908	1930	rBV2	279117	527503	21.10%	2.501%
52	7.562	2000	2013	2050	rBV	979133	1802055	72.09%	8.544%
53	7.849	2089	2102	2126	rBV	183900	333195	13.33%	1.580%
54	7.980	2141	2143	2150	rVB7	1121	1015	0.04%	0.005%
55	8.045	2161	2163	2168	rVB5	1219	867	0.03%	0.004%
56	8.070	2168	2171	2174	rBV4	1046	909	0.04%	0.004%
57	8.167	2198	2201	2202	rBV2	1540	804	0.03%	0.004%
58	8.225	2210	2219	2235	rBV3	36348	64484	2.58%	0.306%
59	8.312	2235	2246	2276	rBV	828736	1538321	61.54%	7.294%
60	8.701	2363	2367	2369	rBV2	1206	944	0.04%	0.004%
61	8.800	2391	2398	2400	rBV3	851	914	0.04%	0.004%
62	8.894	2425	2427	2431	rVB2	1043	675	0.03%	0.003%
63	8.939	2438	2441	2447	rVB4	605	605	0.02%	0.003%
64	9.013	2460	2464	2467	rBV4	1001	679	0.03%	0.003%
65	9.086	2473	2487	2511	rBV	1055206	1814402	72.58%	8.603%
66	9.331	2561	2563	2568	rVB2	1468	1041	0.04%	0.005%
67	9.595	2643	2645	2652	rVB4	886	729	0.03%	0.003%
68	9.784	2699	2704	2705	rBV2	1385	1066	0.04%	0.005%
69	9.926	2742	2748	2750	rBV2	618	667	0.03%	0.003%
70	10.045	2778	2785	2790	rVB3	961	936	0.04%	0.004%
71	10.074	2790	2794	2798	rVB3	1009	828	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031453.D
 Acq On : 23 Apr 2019 21:49
 Operator : JC/SP
 Sample : K2536-04DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X24DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	10.106	2798	2804	2808	rBV4	1160	1237	0.05%	0.006%
73	10.228	2836	2842	2847	rVV6	1400	1765	0.07%	0.008%
74	10.427	2891	2904	2925	rBV	756466	1218366	48.74%	5.777%
75	10.601	2951	2958	2966	rVV6	2557	3876	0.16%	0.018%
76	10.746	2999	3003	3008	rVB4	758	864	0.03%	0.004%
77	10.800	3017	3020	3023	rBV3	1025	807	0.03%	0.004%
78	10.967	3069	3072	3075	rVB2	1468	809	0.03%	0.004%
79	11.029	3087	3091	3094	rBV3	764	562	0.02%	0.003%
80	11.080	3104	3107	3108	rBV2	985	588	0.02%	0.003%
81	11.170	3132	3135	3139	rVB2	864	616	0.02%	0.003%
82	11.199	3139	3144	3147	rBV3	1062	1087	0.04%	0.005%
83	11.270	3163	3166	3173	rVB3	887	988	0.04%	0.005%
84	11.482	3219	3232	3255	rBV	1024721	1659945	66.40%	7.871%
85	11.855	3336	3348	3374	rBV	946149	1575053	63.01%	7.468%
86	12.160	3440	3443	3446	rBV4	1722	1331	0.05%	0.006%
87	12.662	3597	3599	3601	rVV3	1302	688	0.03%	0.003%
88	12.694	3605	3609	3612	rBV3	1002	813	0.03%	0.004%
89	12.977	3693	3697	3699	rVB3	995	636	0.03%	0.003%
90	13.305	3796	3799	3802	rBV3	1412	1085	0.04%	0.005%
91	13.453	3842	3845	3848	rBV2	1444	1202	0.05%	0.006%
92	13.524	3865	3867	3871	rVB2	1287	664	0.03%	0.003%
93	13.543	3871	3873	3880	rVV3	989	862	0.03%	0.004%
94	13.765	3933	3942	3943	rBV3	3856	4561	0.18%	0.022%
95	14.356	4123	4126	4130	rBV2	1459	1127	0.05%	0.005%
96	14.588	4196	4198	4202	rVB3	1208	865	0.03%	0.004%
97	14.610	4202	4205	4208	rBV2	1303	1124	0.04%	0.005%
98	14.916	4288	4300	4302	rBV8	6864	12201	0.49%	0.058%
99	15.083	4347	4352	4365	rVB9	4133	7233	0.29%	0.034%
100	15.318	4422	4425	4426	rBV3	1235	850	0.03%	0.004%


Sum of corrected areas: 21090373

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031453.D
Acq On : 23 Apr 2019 21:49
Operator : JC/SP
Sample : K2536-04DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X24DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

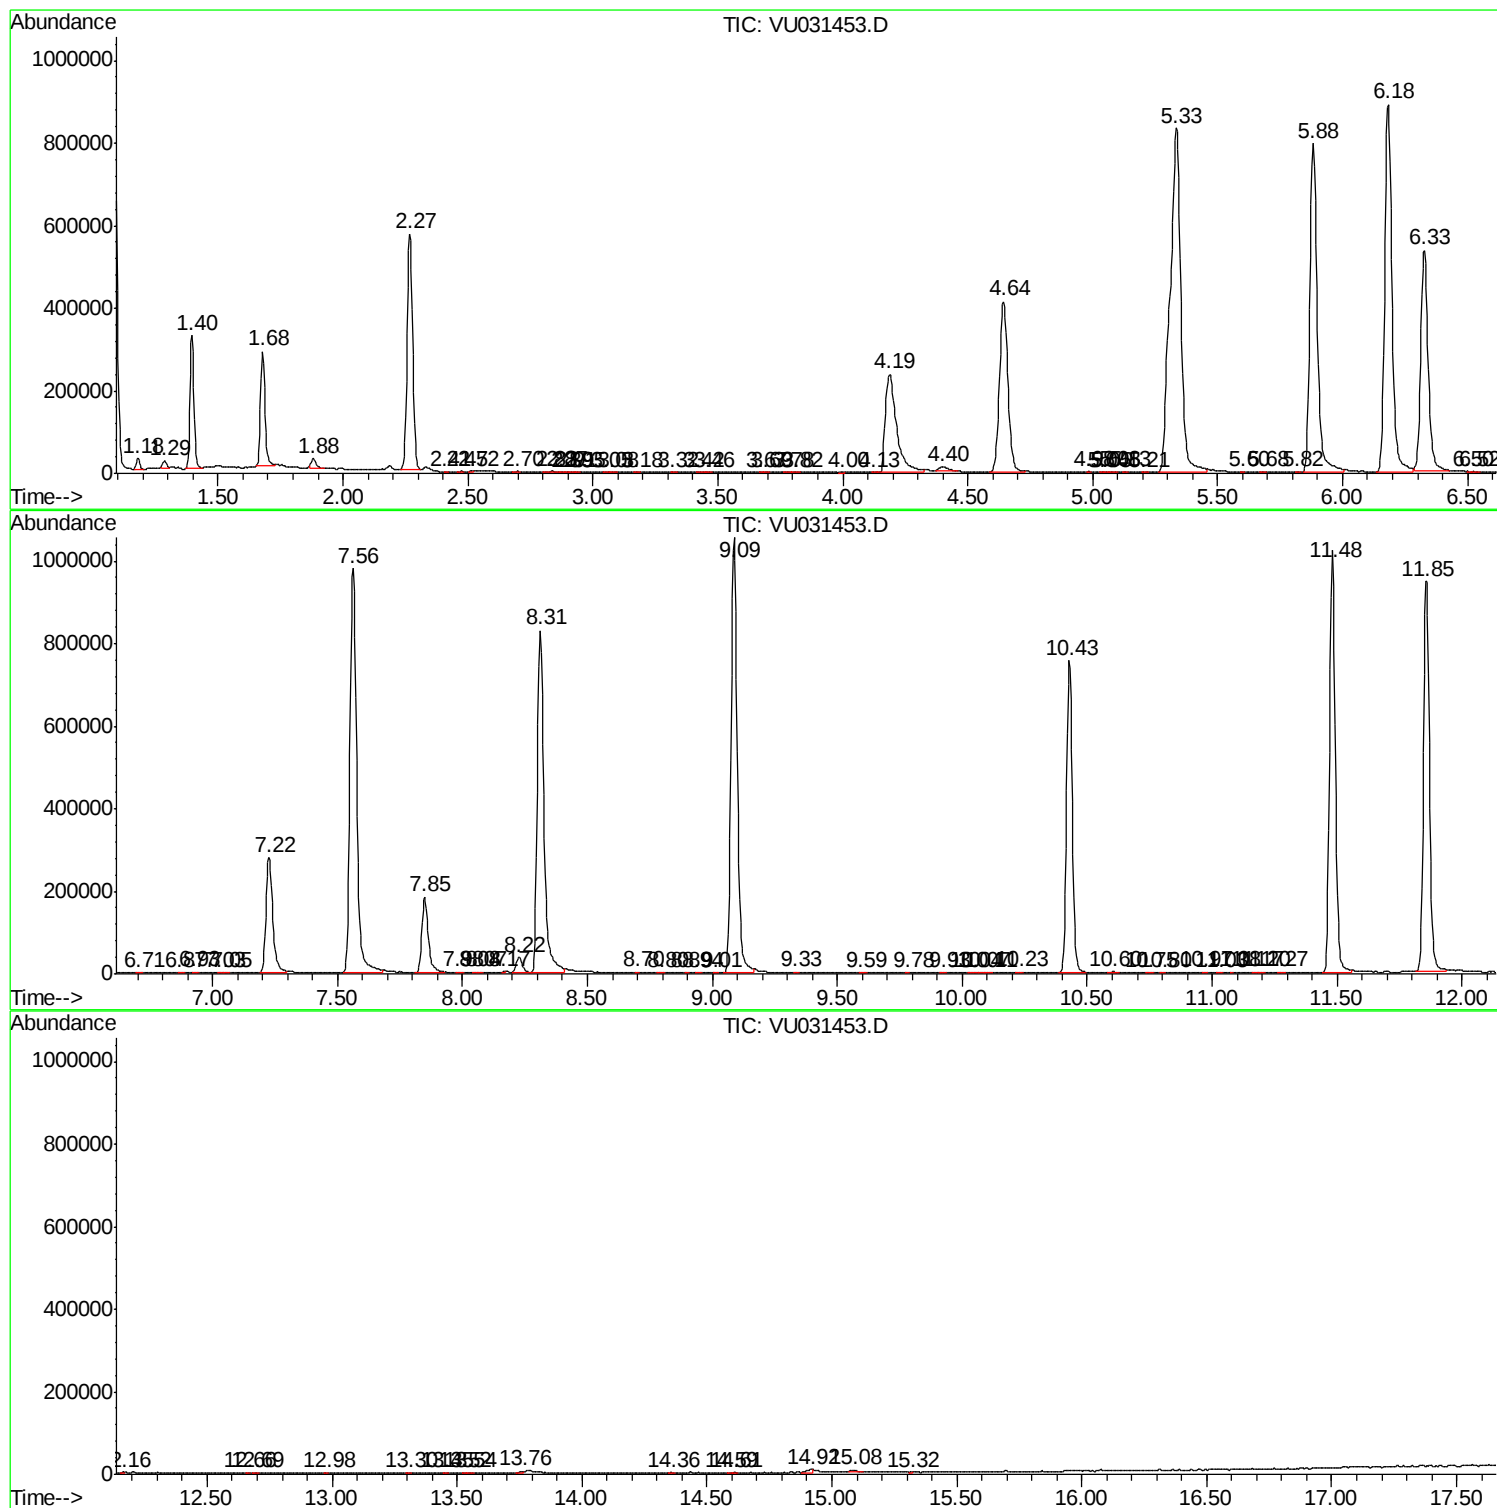

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031453.D
Acq On : 23 Apr 2019 21:49
Operator : JC/SP
Sample : K2536-04DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X24DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031453.D
Acq On : 23 Apr 2019 21:49
Operator : JC/SP
Sample : K2536-04DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X24DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc