

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031454.D
 Acq On : 23 Apr 2019 22:12
 Operator : JC/SP
 Sample : K2536-02 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB	22249	22158	0.92%	0.103%
2	1.283	55	60	66	rBV2	35950	34845	1.44%	0.162%
3	1.395	88	95	109	rVB	303467	332680	13.79%	1.551%
4	1.678	175	183	194	rBV	264865	323651	13.42%	1.509%
5	1.881	241	246	257	rVB	29659	37028	1.53%	0.173%
6	2.267	355	366	380	rVB	549878	830778	34.44%	3.873%
7	2.466	424	428	429	rBV3	1545	908	0.04%	0.004%
8	2.479	430	432	436	rVV3	1172	1191	0.05%	0.006%
9	2.823	533	539	540	rBV3	1794	1607	0.07%	0.007%
10	2.919	567	569	574	rVB3	855	487	0.02%	0.002%
11	3.077	616	618	621	rBV2	995	706	0.03%	0.003%
12	3.135	632	636	639	rVB2	915	731	0.03%	0.003%
13	3.199	653	656	659	rBV2	980	598	0.02%	0.003%
14	3.215	659	661	668	rVB5	656	617	0.03%	0.003%
15	3.427	725	727	733	rVB2	640	468	0.02%	0.002%
16	3.598	776	780	781	rBV2	701	463	0.02%	0.002%
17	3.614	781	785	786	rBV2	641	463	0.02%	0.002%
18	3.791	836	840	844	rBV3	1258	1078	0.04%	0.005%
19	3.842	850	856	859	rVB3	670	614	0.03%	0.003%
20	3.861	859	862	864	rBV	644	469	0.02%	0.002%
21	3.906	872	876	879	rBV3	831	677	0.03%	0.003%
22	3.997	901	904	909	rVB4	915	763	0.03%	0.004%
23	4.035	913	916	920	rBV	814	456	0.02%	0.002%
24	4.090	931	933	937	rVB2	829	597	0.02%	0.003%
25	4.122	937	943	946	rBV3	965	1162	0.05%	0.005%
26	4.186	951	963	1004	rBV	224027	701191	29.07%	3.269%
27	4.643	1088	1105	1131	rBV	385197	919076	38.10%	4.285%
28	4.823	1158	1161	1166	rBV3	782	705	0.03%	0.003%
29	4.881	1176	1179	1180	rBV3	1231	701	0.03%	0.003%
30	4.990	1209	1213	1216	rBV4	1439	880	0.04%	0.004%
31	5.125	1250	1255	1256	rBV2	1270	1065	0.04%	0.005%
32	5.180	1268	1272	1274	rVB3	757	589	0.02%	0.003%
33	5.196	1274	1277	1284	rBV2	840	1128	0.05%	0.005%
34	5.231	1284	1288	1292	rVB5	950	902	0.04%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031454.D
 Acq On : 23 Apr 2019 22:12
 Operator : JC/SP
 Sample : K2536-02 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

35	5.334	1297	1320	1360	rBV2	748899	2262679	93.80%	10.549%
36	5.591	1397	1400	1404	rVB5	992	727	0.03%	0.003%
37	5.784	1456	1460	1464	rVB5	890	560	0.02%	0.003%
38	5.884	1474	1491	1519	rBV	759048	1574938	65.29%	7.343%
39	6.183	1567	1584	1613	rBV	1193015	2412334	100.00%	11.247%
40	6.328	1617	1629	1650	rVB	488181	1000890	41.49%	4.666%
41	6.623	1718	1721	1724	rVB3	677	471	0.02%	0.002%
42	6.639	1724	1726	1730	rVB2	903	499	0.02%	0.002%
43	6.662	1730	1733	1739	rVB3	908	826	0.03%	0.004%
44	6.746	1756	1759	1762	rBV3	775	458	0.02%	0.002%
45	6.868	1795	1797	1800	rBV2	867	532	0.02%	0.002%
46	6.894	1800	1805	1807	rBV2	1008	819	0.03%	0.004%
47	6.971	1824	1829	1830	rBV	768	583	0.02%	0.003%
48	7.003	1835	1839	1842	rBV2	738	611	0.03%	0.003%
49	7.022	1842	1845	1849	rVB	823	569	0.02%	0.003%
50	7.225	1897	1908	1936	rBV	293954	559746	23.20%	2.610%
51	7.427	1968	1971	1973	rBV3	859	597	0.02%	0.003%
52	7.495	1987	1992	1996	rVB3	853	862	0.04%	0.004%
53	7.562	1996	2013	2050	rBV	1025795	1916210	79.43%	8.934%
54	7.848	2091	2102	2127	rBV2	194348	364110	15.09%	1.698%
55	8.000	2147	2149	2153	rVB2	1373	907	0.04%	0.004%
56	8.028	2155	2158	2166	rVV6	901	1128	0.05%	0.005%
57	8.080	2171	2174	2178	rVB3	1116	896	0.04%	0.004%
58	8.138	2190	2192	2194	rBV2	784	460	0.02%	0.002%
59	8.176	2197	2204	2209	rVV4	3234	4133	0.17%	0.019%
60	8.225	2210	2219	2232	rVB3	41091	69913	2.90%	0.326%
61	8.311	2235	2246	2280	rBV	865178	1602398	66.43%	7.471%
62	8.643	2347	2349	2353	rBV3	666	537	0.02%	0.003%
63	8.694	2363	2365	2371	rVB3	782	748	0.03%	0.003%
64	8.858	2412	2416	2419	rBV4	790	797	0.03%	0.004%
65	8.980	2449	2454	2457	rBV3	1107	1025	0.04%	0.005%
66	9.086	2474	2487	2515	rBV	1126681	1946869	80.70%	9.077%
67	9.302	2550	2554	2562	rBV5	1461	1539	0.06%	0.007%
68	9.437	2593	2596	2598	rBV3	761	517	0.02%	0.002%
69	9.520	2619	2622	2626	rVB3	796	619	0.03%	0.003%
70	9.546	2626	2630	2633	rBV3	887	840	0.03%	0.004%
71	9.604	2644	2648	2655	rVB3	986	1105	0.05%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042319\
 Data File : VU031454.D
 Acq On : 23 Apr 2019 22:12
 Operator : JC/SP
 Sample : K2536-02 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
 Title : VOC Analysis

72	9.649	2657	2662	2664	rBV4	966	847	0.04%	0.004%
73	9.784	2701	2704	2707	rBV2	1228	805	0.03%	0.004%
74	9.813	2710	2713	2716	rVB3	650	454	0.02%	0.002%
75	9.877	2730	2733	2736	rBV2	1063	816	0.03%	0.004%
76	10.051	2785	2787	2792	rBV2	1183	976	0.04%	0.005%
77	10.225	2839	2841	2842	rBV2	1074	474	0.02%	0.002%
78	10.360	2881	2883	2889	rVB2	684	457	0.02%	0.002%
79	10.427	2892	2904	2928	rBV	790968	1258922	52.19%	5.869%
80	10.578	2949	2951	2953	rBV2	954	472	0.02%	0.002%
81	10.607	2954	2960	2966	rVB6	2247	2749	0.11%	0.013%
82	10.691	2981	2986	2990	rBV4	1637	1426	0.06%	0.007%
83	10.739	2999	3001	3005	rVV2	714	465	0.02%	0.002%
84	11.054	3095	3099	3102	rVV3	776	659	0.03%	0.003%
85	11.080	3102	3107	3114	rVB6	1118	1395	0.06%	0.007%
86	11.231	3150	3154	3157	rBV2	1053	974	0.04%	0.005%
87	11.253	3158	3161	3163	rBV	1221	882	0.04%	0.004%
88	11.327	3182	3184	3190	rVB2	901	659	0.03%	0.003%
89	11.437	3215	3218	3220	rBV2	914	519	0.02%	0.002%
90	11.482	3220	3232	3255	rBV	1014069	1652428	68.50%	7.704%
91	11.858	3337	3349	3373	rBV	942752	1551977	64.34%	7.236%
92	12.356	3501	3504	3507	rBV	1159	908	0.04%	0.004%
93	12.395	3513	3516	3518	rBV2	1129	765	0.03%	0.004%
94	12.466	3536	3538	3540	rBV3	886	519	0.02%	0.002%
95	12.662	3595	3599	3600	rBV2	1278	880	0.04%	0.004%
96	13.266	3785	3787	3789	rBV3	985	531	0.02%	0.002%
97	13.739	3931	3934	3937	rBV3	1392	1112	0.05%	0.005%
98	13.787	3941	3949	3952	rBV7	4624	7354	0.30%	0.034%
99	14.858	4279	4282	4286	rBV	1919	1545	0.06%	0.007%
100	15.025	4329	4334	4337	rBV4	2471	2265	0.09%	0.011%


Sum of corrected areas: 21449119

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042319\
Data File : VU031454.D
Acq On : 23 Apr 2019 22:12
Operator : JC/SP
Sample : K2536-02 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

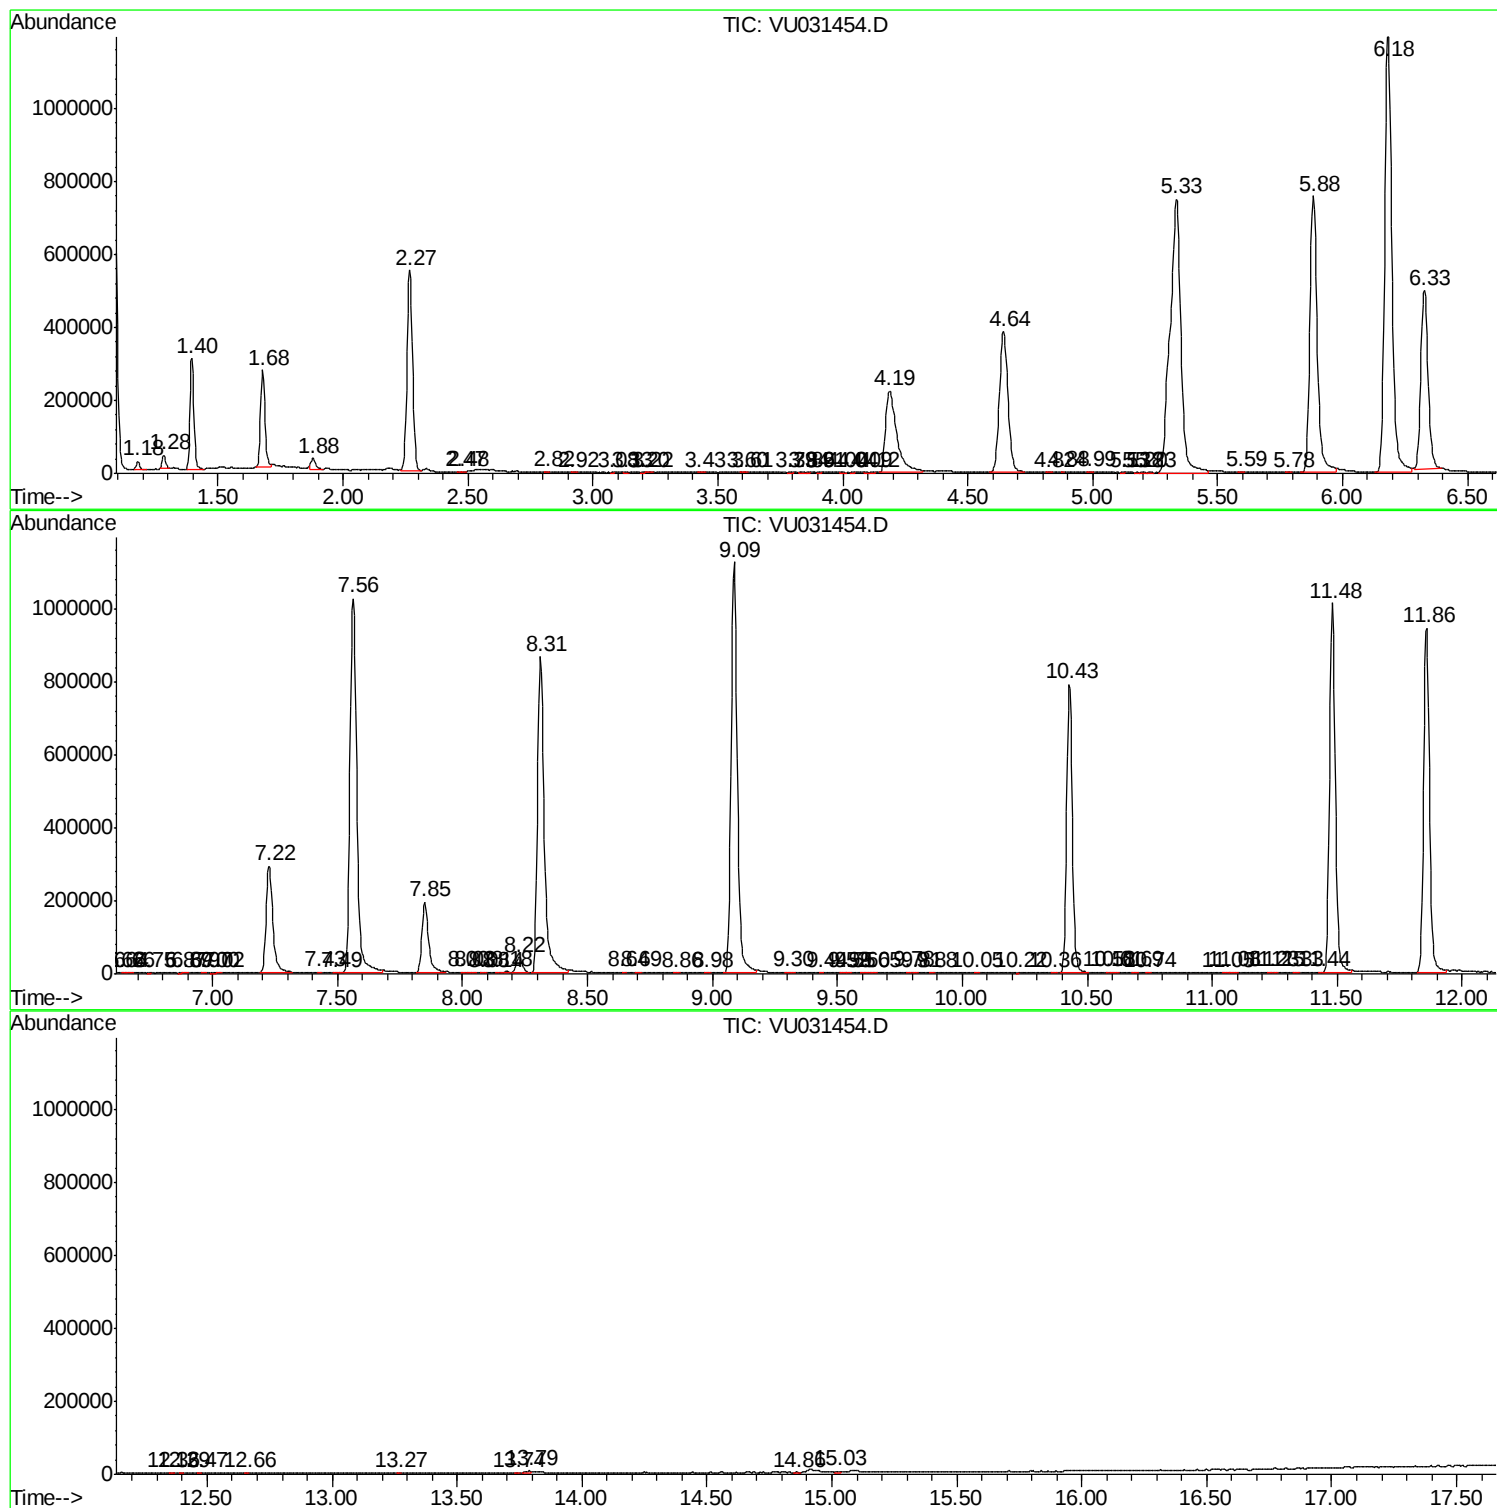

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031454.D
Acq On : 23 Apr 2019 22:12
Operator : JC/SP
Sample : K2536-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042319\
Data File : VU031454.D
Acq On : 23 Apr 2019 22:12
Operator : JC/SP
Sample : K2536-02 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X22

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc