


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042319\
Data File : VU031397.D
Acq On : 22 Apr 2019 16:35
Operator : JC/SP
Sample : BFB31
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB31

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Title : VOC Analysis
Last Update : Wed Apr 24 08:41:52 2019

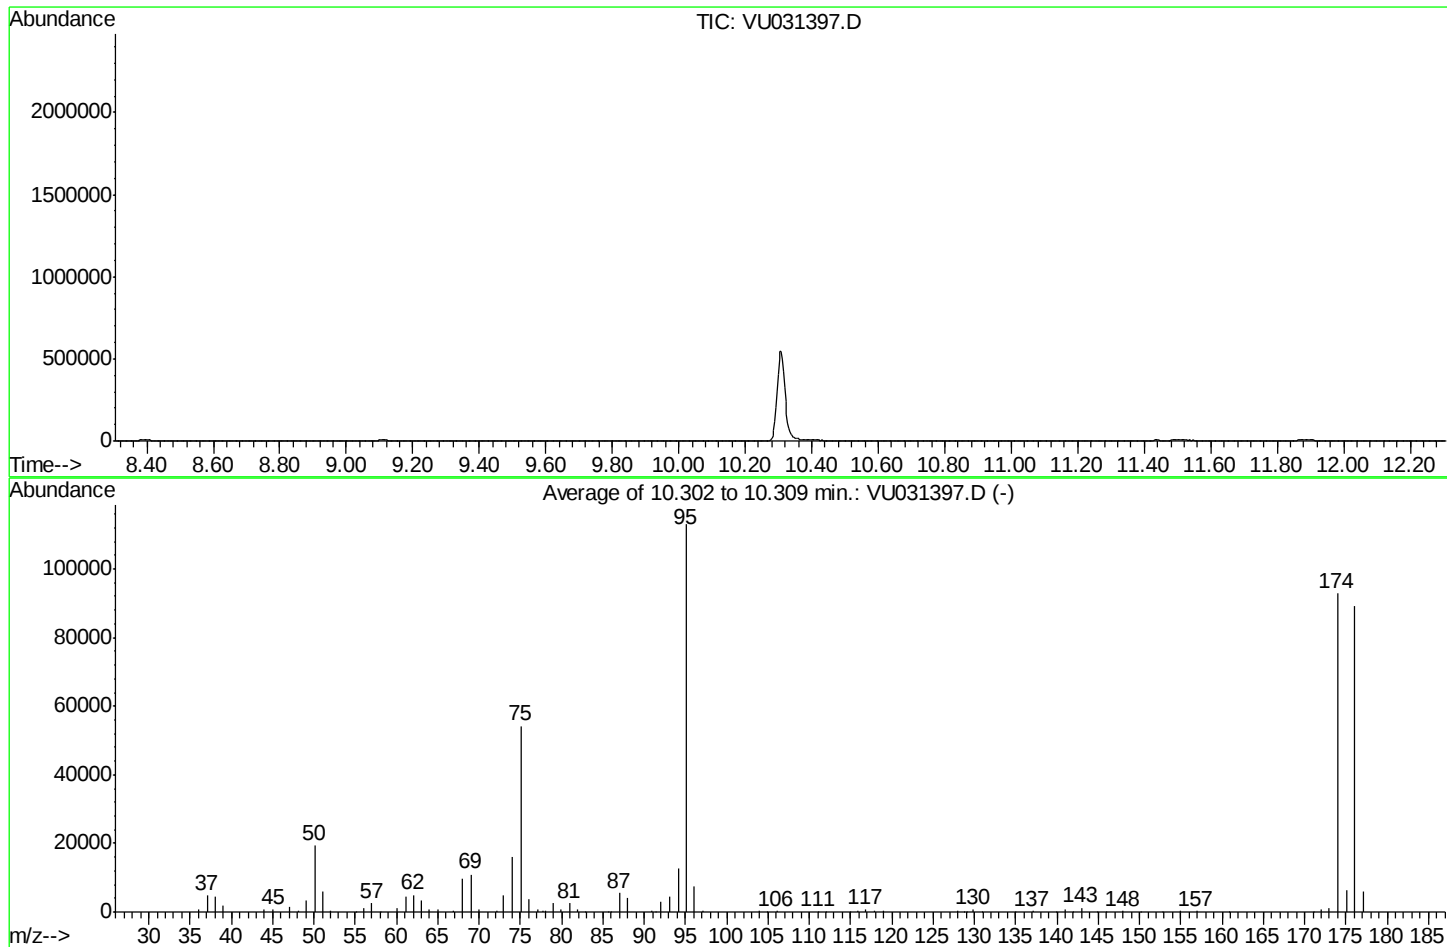

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	19298	PASS
75	95	30	80	48.0	54298	PASS
95	95	100	100	100.0	113013	PASS
96	95	5	9	6.5	7300	PASS
173	174	0.00	2	1.2	1120	PASS
174	95	50	120	82.1	92818	PASS
175	174	5	9	6.9	6425	PASS
176	174	95	101	96.0	89117	PASS
177	176	5	9	6.8	6023	PASS

Scan 2854 (10.267 min): VU031397.D
BFB31

m/z	Abundance
36.20	165.0
40.00	1551.0
44.00	1329.0
207.20	266.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	978.0
37.10	4149.0
38.00	4049.0
39.00	1601.0
39.90	1004.0
44.00	1921.0
45.10	610.0
47.00	1654.0
48.10	515.0
49.10	3321.0
50.10	18624.0
51.10	5798.0
52.00	375.0
55.00	127.0
56.10	1221.0
57.00	2400.0
60.00	877.0
61.10	4433.0
62.10	4439.0
63.00	3366.0
64.00	604.0
65.00	643.0
66.90	258.0
68.00	9690.0
69.00	10612.0
70.00	865.0
72.30	457.0
73.00	4349.0
74.10	15538.0
75.00	50616.0
76.10	3594.0
77.10	641.0
77.70	485.0
78.90	2296.0
80.00	696.0
81.00	2629.0
81.90	675.0
86.00	161.0
87.00	5358.0
88.00	4271.0
90.90	240.0
92.00	2723.0
93.10	4188.0
94.10	11829.0
95.10	105800.0
96.00	7009.0
97.20	318.0
104.00	368.0
104.90	167.0
106.10	365.0
111.10	111.0
112.00	179.0
115.90	496.0
116.90	585.0
117.90	299.0
119.00	433.0
128.00	443.0
128.70	163.0
129.10	102.0
129.90	656.0
130.90	142.0
134.90	179.0
137.10	142.0
141.00	907.0
141.90	205.0
143.00	1157.0
144.90	225.0
145.90	127.0
148.00	177.0
152.80	102.0
155.00	219.0
156.90	175.0
171.00	163.0
172.00	663.0
172.90	878.0
174.00	85576.0
175.00	6153.0
176.00	83280.0
177.10	5976.0
207.10	186.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
35.90	975.0
37.10	4912.0
38.00	4582.0
39.00	1778.0
39.90	1020.0
44.00	1995.0
45.00	749.0
47.00	1642.0
48.00	456.0
49.10	3587.0
50.10	19736.0
51.10	6040.0
52.00	298.0
55.00	147.0
56.10	1216.0
57.00	2556.0
58.10	102.0
60.00	1065.0
61.10	4749.0
62.10	5086.0
63.10	3439.0
64.00	704.0
65.00	593.0
66.90	248.0
68.00	10152.0
69.10	11230.0
70.00	812.0
72.10	454.0
73.00	4960.0
74.00	16440.0
75.10	56024.0
76.00	3978.0
77.10	819.0
77.70	418.0
78.10	372.0
79.00	2565.0
79.90	793.0
81.00	2552.0
82.00	705.0
86.00	178.0
87.00	5916.0
88.00	4410.0
90.80	290.0
91.30	225.0
92.00	2928.0
93.10	4622.0
94.10	13211.0
95.10	116832.0
96.00	7604.0
97.20	348.0
104.00	332.0
104.90	201.0
106.10	417.0
111.10	115.0
112.00	155.0
115.90	501.0
116.90	748.0
118.00	377.0
118.90	553.0
128.00	383.0
128.70	100.0
129.90	580.0
131.00	123.0
134.90	218.0
137.10	255.0
141.00	869.0
141.90	215.0
143.00	1291.0
144.90	205.0
145.90	148.0
148.00	260.0
150.10	108.0
152.80	146.0
155.00	201.0
156.90	213.0
171.00	143.0
171.90	725.0
173.00	1169.0
174.00	96080.0
175.10	6501.0
176.00	92112.0
177.00	6262.0
207.00	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31

m/z	Abundance
36.00	866.0
37.10	5074.0
38.00	4597.0
39.00	1813.0
40.00	1093.0
44.00	1915.0
45.00	803.0
47.00	1519.0
48.00	406.0
49.10	3739.0
50.10	19536.0
51.10	5646.0
52.00	173.0
55.10	131.0
56.00	1282.0
57.00	2691.0
58.10	114.0
60.00	1201.0
61.10	4728.0
62.00	5090.0
63.00	3302.0
64.00	738.0
65.00	480.0
66.80	196.0
68.00	9567.0
69.10	10672.0
70.00	640.0
72.00	623.0
73.00	4867.0
74.00	15990.0
75.10	56256.0
76.00	4180.0
77.10	900.0
77.80	369.0
78.10	389.0
79.00	2515.0
79.90	795.0
80.90	2453.0
82.00	617.0
82.80	106.0
85.70	219.0
87.00	5355.0
88.00	4037.0
90.80	300.0
91.30	235.0
92.00	2842.0
93.10	4633.0
94.10	13328.0
95.10	116408.0
96.00	7288.0
97.10	328.0
103.90	303.0
104.90	176.0
106.00	345.0
111.10	132.0
114.90	109.0
116.00	426.0
116.80	764.0
118.00	433.0
118.90	692.0
128.00	301.0
129.90	521.0
134.90	189.0
137.10	286.0
139.90	129.0
141.10	761.0
141.90	172.0
143.00	1301.0
144.90	169.0
145.90	225.0
148.00	313.0
150.10	116.0
152.80	171.0
154.90	185.0
156.90	231.0
160.80	117.0
171.90	776.0
173.00	1314.0
174.00	96800.0
175.10	6622.0
176.00	91960.0
177.00	5832.0
207.00	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB31