


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042319\
Data File : VU031422.D
Acq On : 23 Apr 2019 08:51
Operator : JC/SP
Sample : BFB32
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB32

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042319WMA.M
Title : VOC Analysis
Last Update : Wed Apr 24 08:41:52 2019

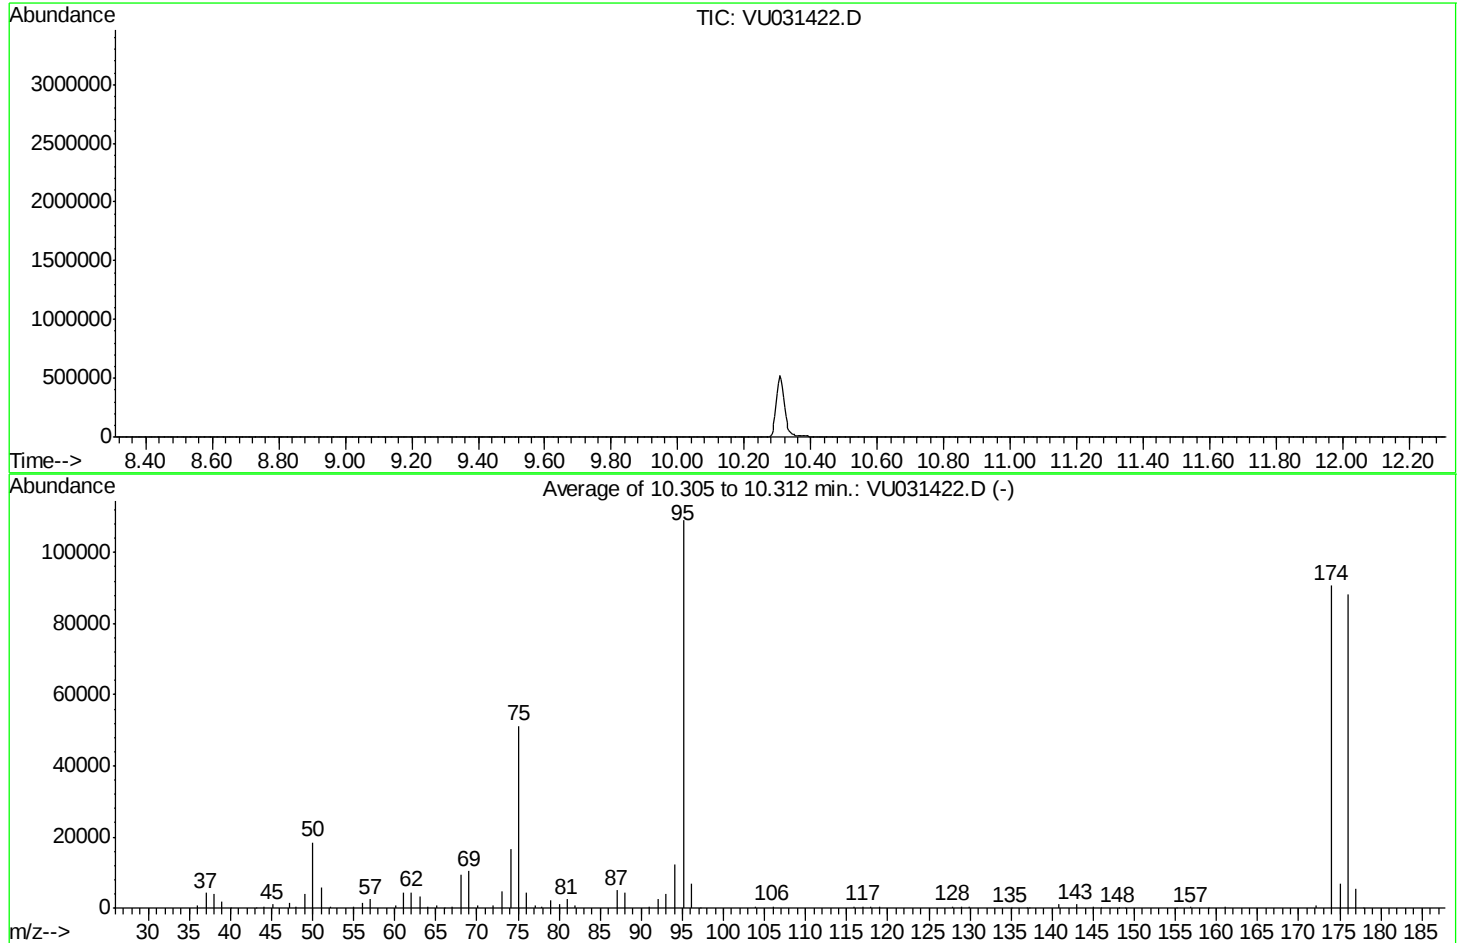

AutoFind: Scans 2866, 2867, 2868; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	18512	PASS
75	95	30	80	47.0	51221	PASS
95	95	100	100	100.0	109080	PASS
96	95	5	9	6.4	6932	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	83.1	90613	PASS
175	174	5	9	7.5	6810	PASS
176	174	95	101	97.5	88360	PASS
177	176	5	9	6.3	5549	PASS

Scan 2854 (10.267 min): VU031422.D
BFB32

m/z	Abundance
40.00	1413.0
44.00	1012.0
207.10	203.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.10	949.0
37.00	4091.0
38.00	4133.0
39.00	1765.0
40.00	1510.0
44.00	1298.0
45.10	966.0
47.20	1298.0
47.90	504.0
49.10	4220.0
50.10	18752.0
51.10	5928.0
52.10	292.0
54.90	456.0
56.10	1364.0
57.10	2389.0
60.00	835.0
61.00	4293.0
62.10	4445.0
63.10	3410.0
64.10	475.0
65.00	603.0
66.00	167.0
66.90	325.0
68.10	9492.0
69.00	10384.0
70.10	838.0
72.00	616.0
73.00	4808.0
74.10	17064.0
75.10	51784.0
76.10	4862.0
77.00	806.0
77.90	557.0
78.90	2539.0
80.00	1082.0
80.90	2467.0
82.00	658.0
87.00	4926.0
88.00	4323.0
90.80	449.0
92.00	2634.0
93.10	4074.0
94.10	12376.0
95.10	109456.0
96.10	7078.0
97.20	182.0
103.90	434.0
106.00	520.0
116.00	218.0
117.00	454.0
118.00	405.0
119.00	463.0
127.90	335.0
129.00	223.0
129.90	370.0
135.00	130.0
136.90	164.0
140.90	799.0
143.00	981.0
144.90	218.0
145.90	184.0
148.00	131.0
155.10	132.0
156.80	212.0
159.10	139.0
161.00	185.0
172.00	721.0
174.00	90224.0
175.00	6475.0
176.00	87872.0
177.00	5424.0
177.90	119.0
207.10	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
36.00	928.0
37.10	4360.0
38.00	4233.0
39.00	1757.0
40.00	1427.0
44.00	1196.0
45.10	945.0
47.20	1470.0
48.00	463.0
49.10	4025.0
50.00	18816.0
51.10	5951.0
52.20	367.0
54.90	473.0
56.00	1499.0
57.10	2387.0
60.10	841.0
61.10	4507.0
62.10	4567.0
63.10	3582.0
64.10	518.0
65.00	617.0
66.00	154.0
67.00	263.0
68.00	9493.0
69.00	10543.0
70.10	835.0
72.00	584.0
73.00	4762.0
74.10	16968.0
75.10	52576.0
76.00	4551.0
77.10	726.0
77.90	556.0
79.00	2387.0
80.00	1117.0
80.90	2435.0
81.90	598.0
87.00	5130.0
88.00	4285.0
90.90	473.0
92.00	2466.0
93.10	3912.0
94.10	12492.0
95.10	112752.0
96.10	7181.0
97.10	114.0
103.90	364.0
106.00	589.0
115.90	322.0
116.90	451.0
118.00	491.0
119.00	433.0
127.90	456.0
129.00	225.0
130.00	361.0
135.00	126.0
137.10	133.0
140.80	909.0
143.00	1114.0
144.90	203.0
146.00	177.0
148.00	131.0
148.90	139.0
155.20	153.0
156.90	207.0
159.10	127.0
161.00	223.0
172.10	849.0
174.00	93336.0
175.00	7048.0
176.00	91144.0
177.00	5755.0
177.80	134.0
207.20	206.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32

m/z	Abundance
35.90	741.0
37.10	4327.0
38.00	3790.0
39.00	1470.0
40.00	1311.0
43.10	137.0
44.00	1214.0
45.10	864.0
47.10	1207.0
48.00	454.0
49.10	3640.0
50.00	17968.0
51.10	5570.0
52.20	369.0
55.00	363.0
56.00	1395.0
57.00	2338.0
60.10	757.0
61.10	4225.0
62.00	4199.0
63.10	3259.0
64.00	430.0
65.10	650.0
67.00	221.0
68.00	8914.0
69.00	10045.0
70.10	840.0
72.00	520.0
73.00	4483.0
74.10	15249.0
75.10	49304.0
76.00	3825.0
77.00	555.0
77.90	506.0
79.00	2085.0
80.00	905.0
81.00	2423.0
81.90	595.0
87.00	4936.0
88.00	3918.0
91.00	447.0
92.00	2253.0
93.00	3550.0
94.10	11709.0
95.10	105032.0
96.10	6539.0
103.90	280.0
106.00	538.0
116.00	445.0
117.10	463.0
117.90	463.0
119.10	348.0
127.90	469.0
128.80	192.0
130.00	331.0
135.00	166.0
137.20	187.0
140.90	1030.0
142.90	1123.0
145.00	184.0
146.00	152.0
148.10	117.0
148.90	190.0
155.20	187.0
157.00	179.0
161.00	186.0
172.10	1020.0
174.00	88280.0
175.10	6909.0
176.00	86064.0
177.00	5468.0
177.90	137.0
207.20	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB32