

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
 Data File : PP035245.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 24 Apr 2021 00:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Apr 26 01:02:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Apr 21 17:37:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.840	4.244	1680201	1090498	20.620	21.176
2) SA Decachlor...	10.745	9.528	1660277	666877	26.273	28.067
Target Compounds						
32) L7 AR-1260-2	8.121f	0.000	16014	0	4.704	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP042321\
Data File : PP035245.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 24 Apr 2021 00:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Apr 26 01:02:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP042121.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Apr 21 17:37:28 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

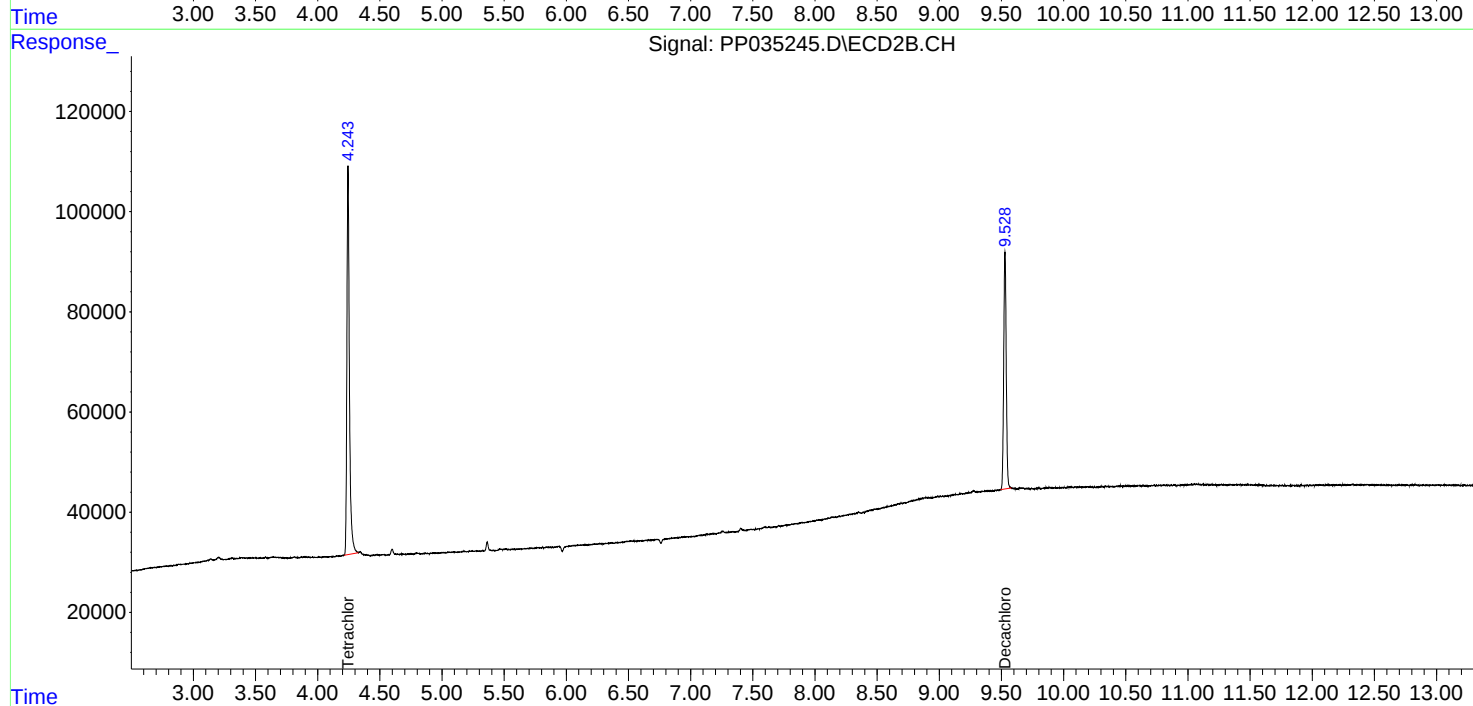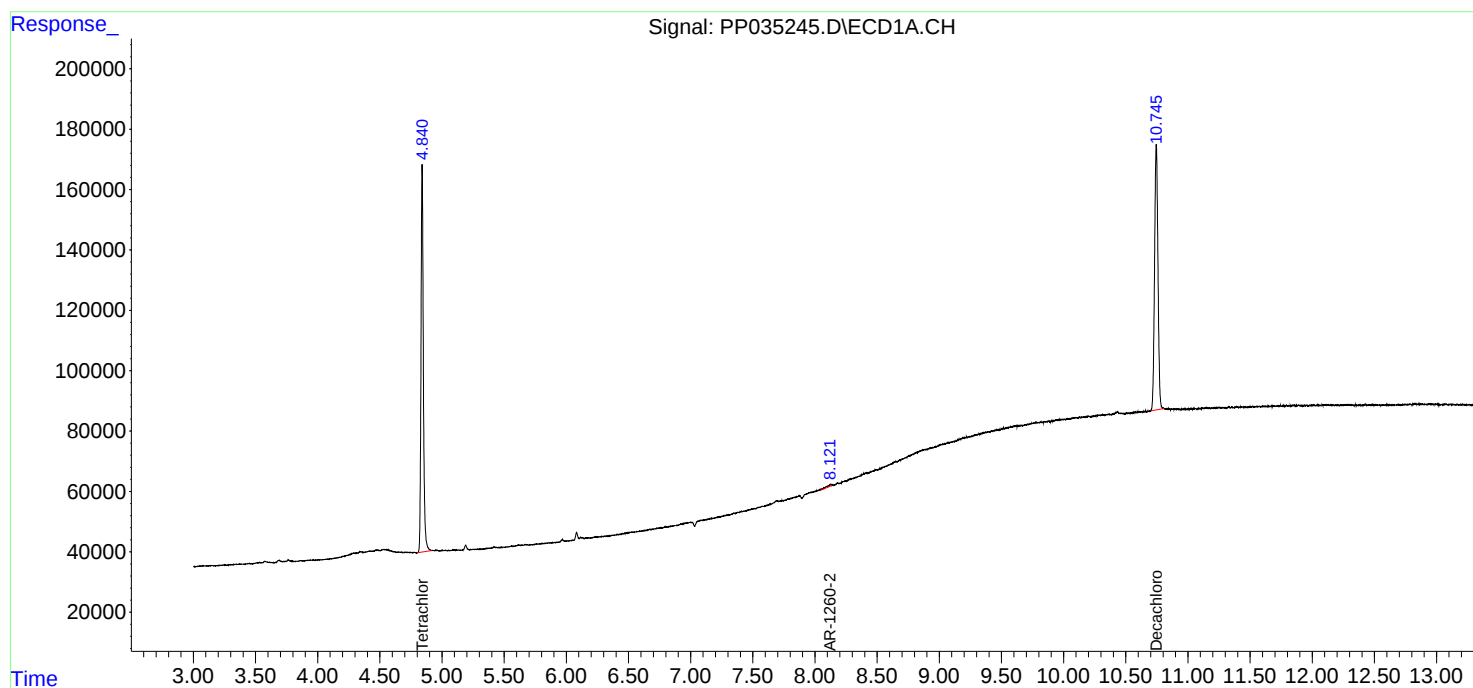


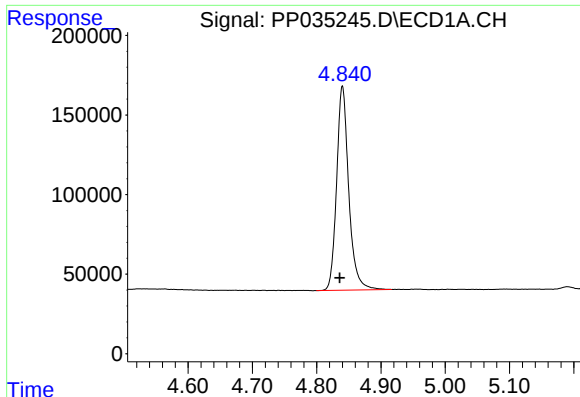

#1 Tetrachloro-m-xylene


R.T.: 4.840 min
Delta R.T.: 0.004 min
Response: 1680201
Conc: 20.62 ng/ml

Instrument :
MSVOA_U
ClientSampleId :

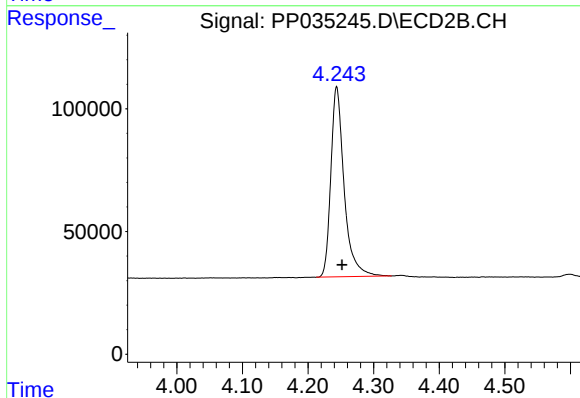


#1 Tetrachloro-m-xylene

R.T.: 4.244 min
Delta R.T.: -0.008 min
Response: 1090498
Conc: 21.18 ng/ml

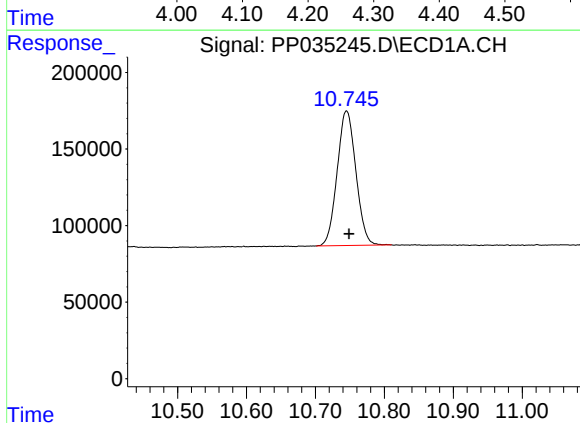


#2 Decachlorobiphenyl

R.T.: 10.745 min
Delta R.T.: -0.003 min
Response: 1660277
Conc: 26.27 ng/ml

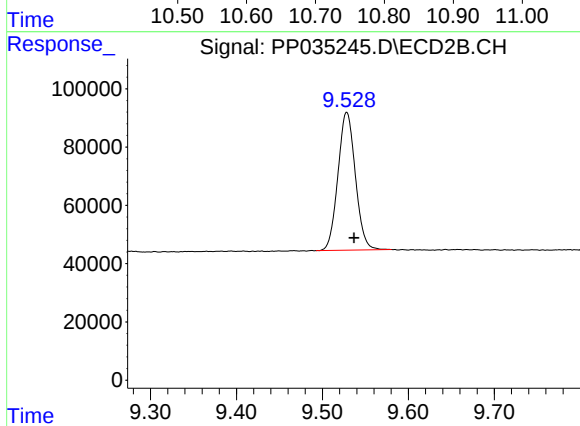

#2 Decachlorobiphenyl


R.T.: 9.528 min
Delta R.T.: -0.009 min
Response: 666877
Conc: 28.07 ng/ml

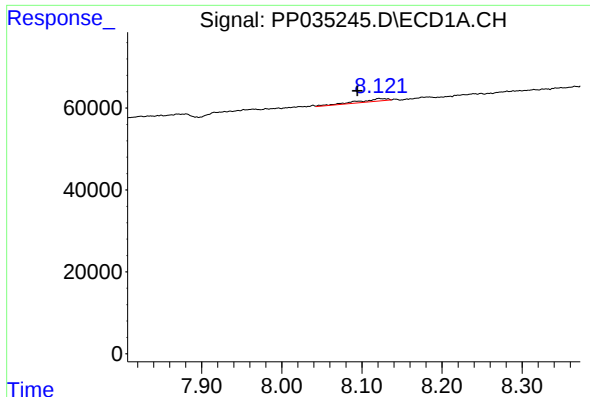

#32 AR-1260-2

R.T.: 8.121 min
Delta R.T.: 0.027 min
Response: 16014
Conc: 4.70 ng/ml

Instrument :
MSVOA_U
ClientSampleId :

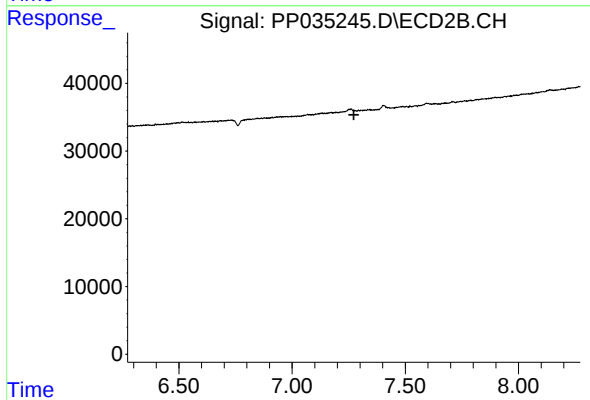

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.273 min
Response: 0
Conc: N.D.