


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU042321\  
Data File : VU043297.D  
Acq On : 23 Apr 2021 17:34  
Operator : SY/MD  
Sample : M2127-04  
Misc : 25.0mL/MSVOA\_U/WATER  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
E0AA1

Manual Integrations  
APPROVED

Quant Time: Apr 24 06:33:58 2021  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR041521WMA.M  
Quant Title : TRACE VOA SFAM1.0  
QLast Update : Sat Apr 24 06:31:00 2021  
Response via : Initial Calibration

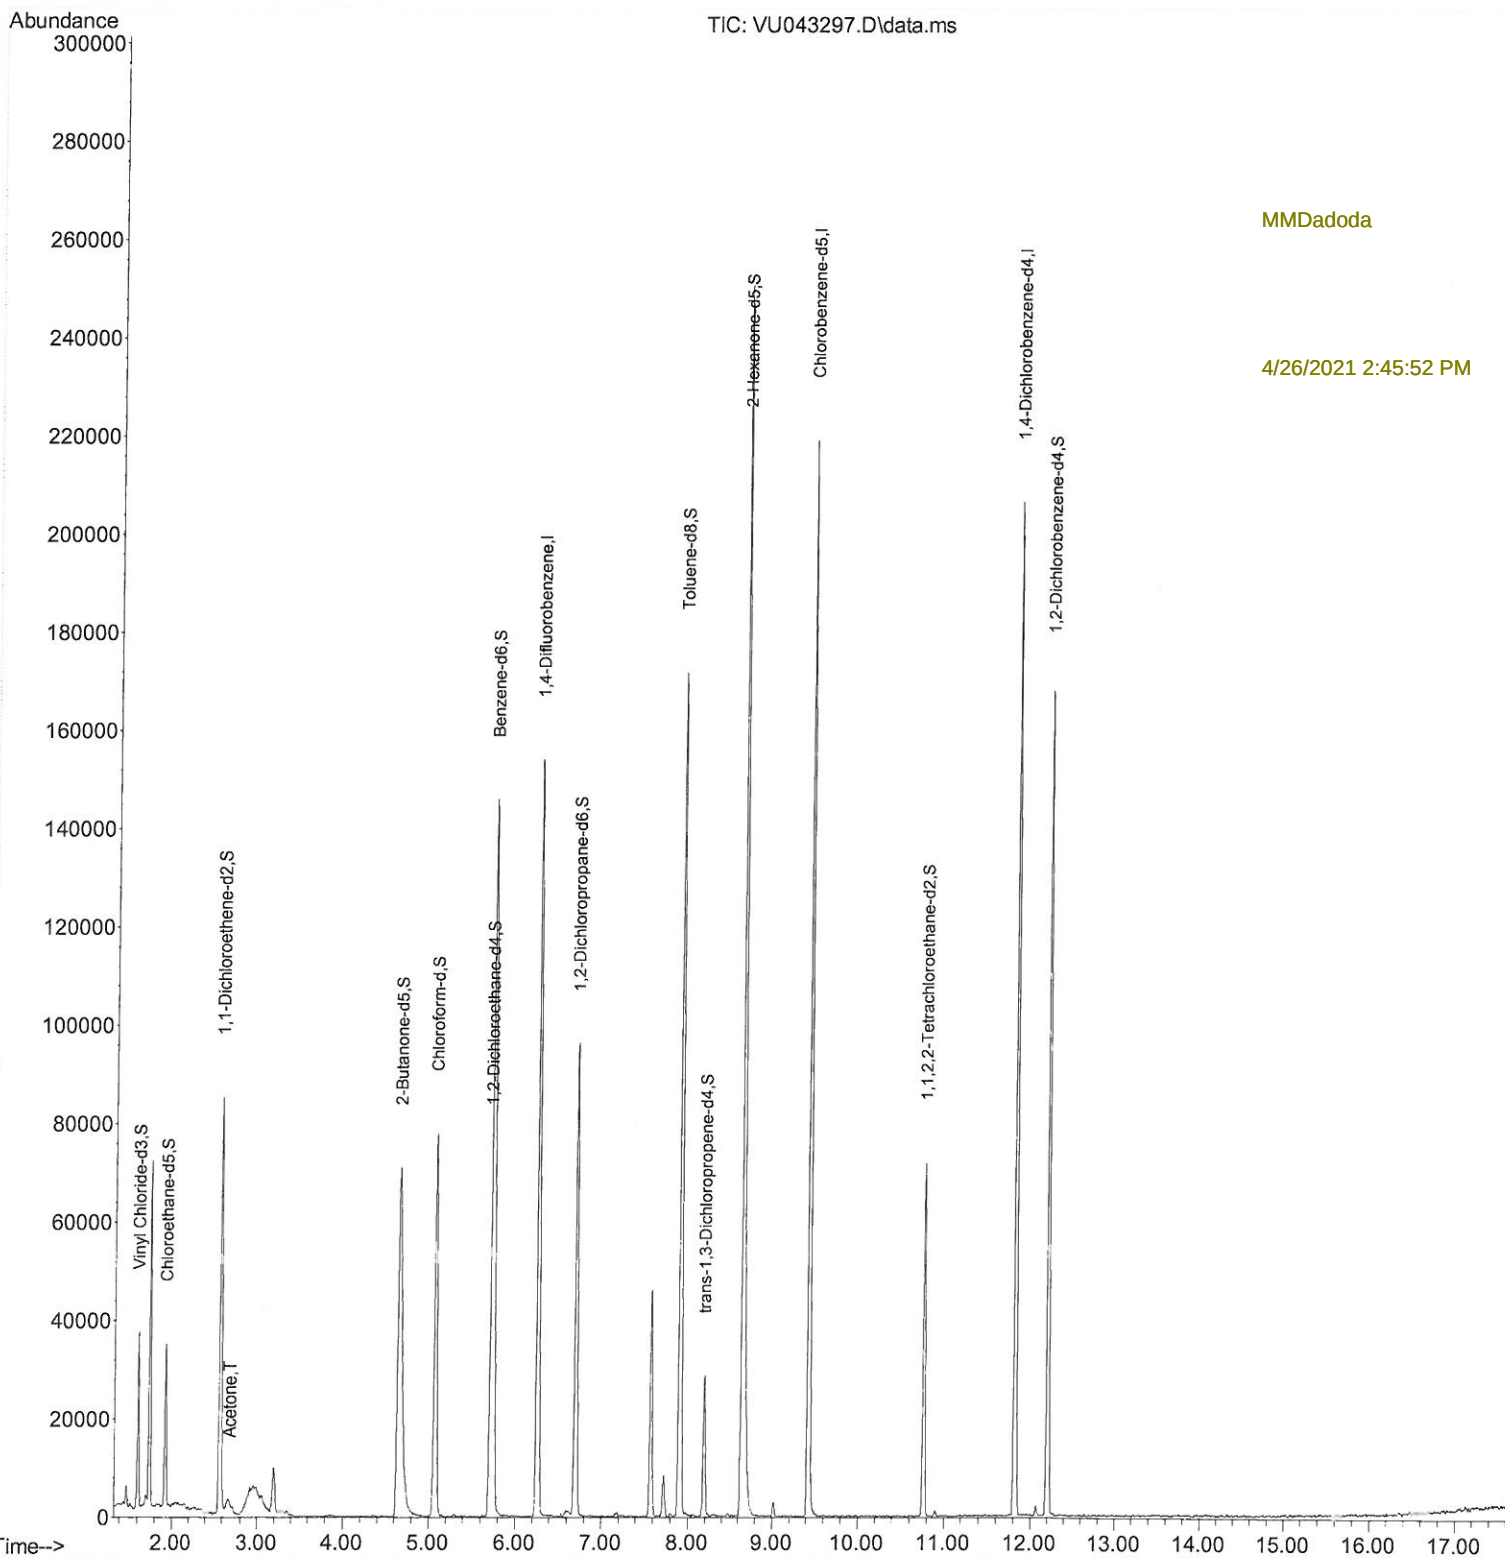

MMDadoda




4/26/2021 2:45:52 PM

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU042321\  
 Data File : VU043297.D  
 Acq On : 23 Apr 2021 17:34  
 Operator : SY/MD  
 Sample : M2127-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 E0AA1

Manual Integrations  
 APPROVED

Quant Time: Apr 24 06:33:58 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR041521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Apr 24 06:31:00 2021  
 Response via : Initial Calibration

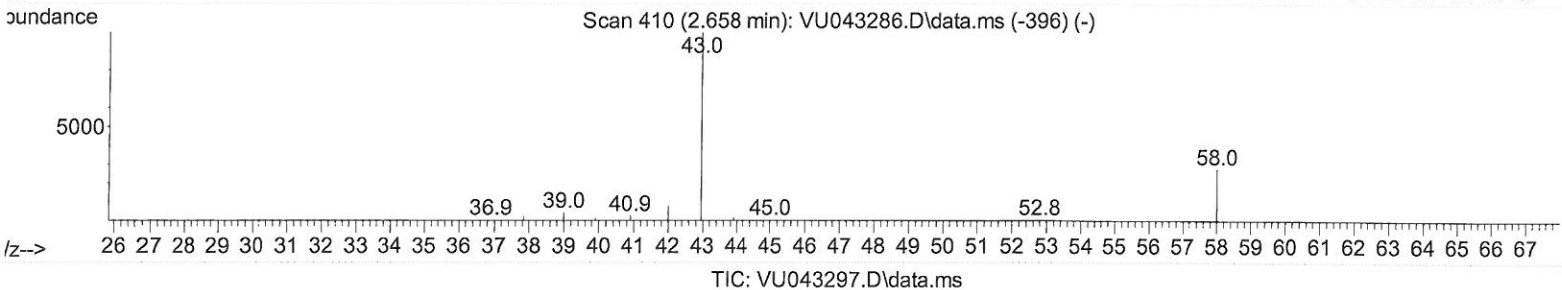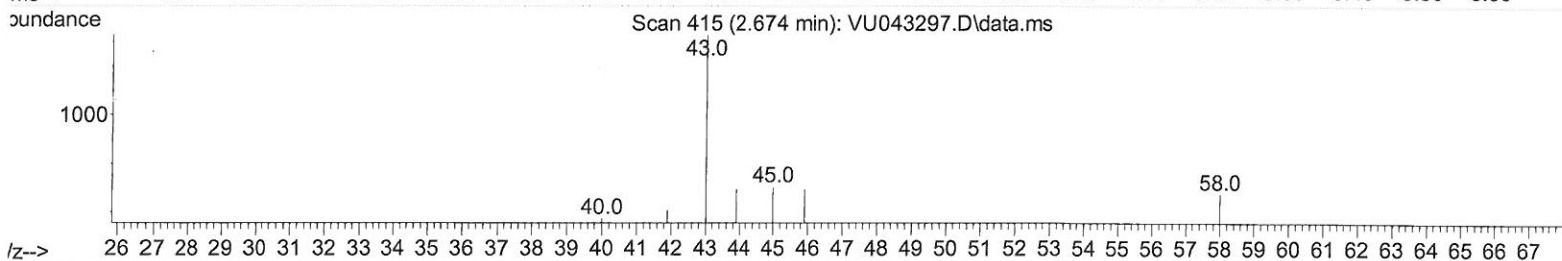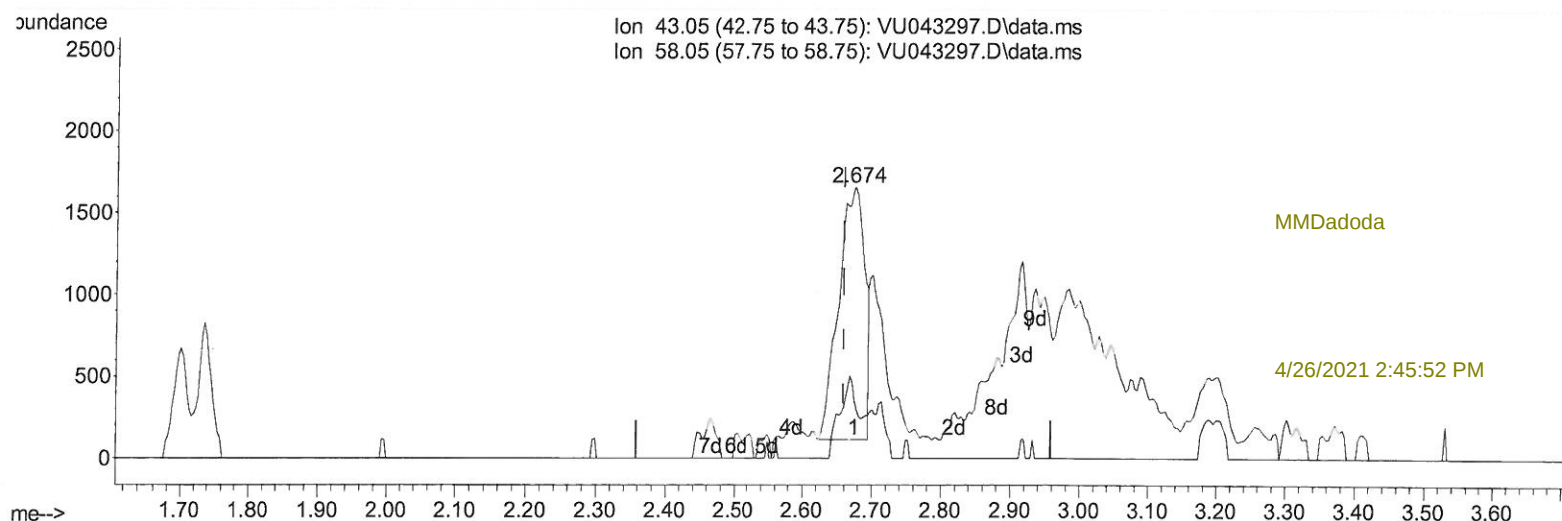

(13) Acetone (T)

2.674min (+ 0.016) 2.16 ug/L

response 3993




| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 12.50  | 20.99  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU042321\  
 Data File : VU043297.D  
 Acq On : 23 Apr 2021 17:34  
 Operator : SY/MD  
 Sample : M2127-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampleId :  
 E0AA1

Manual Integrations  
 APPROVED

Quant Time: Apr 24 06:33:58 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR041521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 QLast Update : Sat Apr 24 06:31:00 2021  
 Response via : Initial Calibration

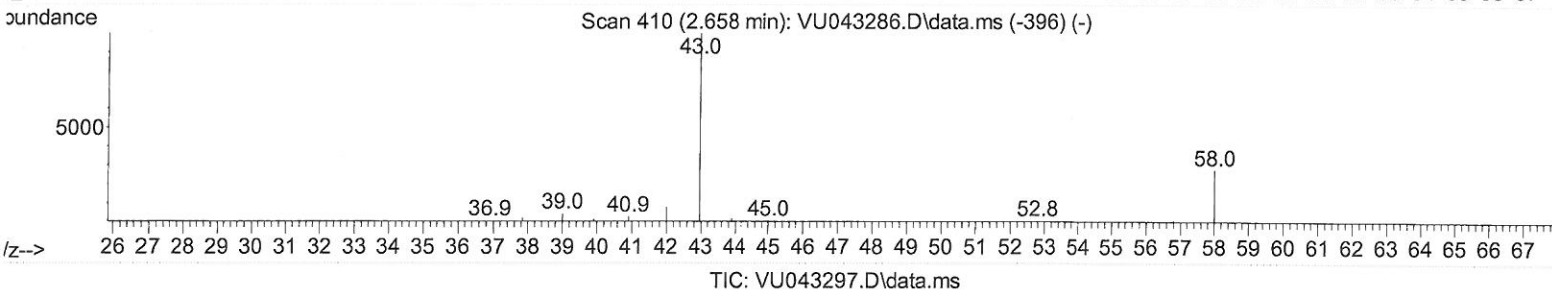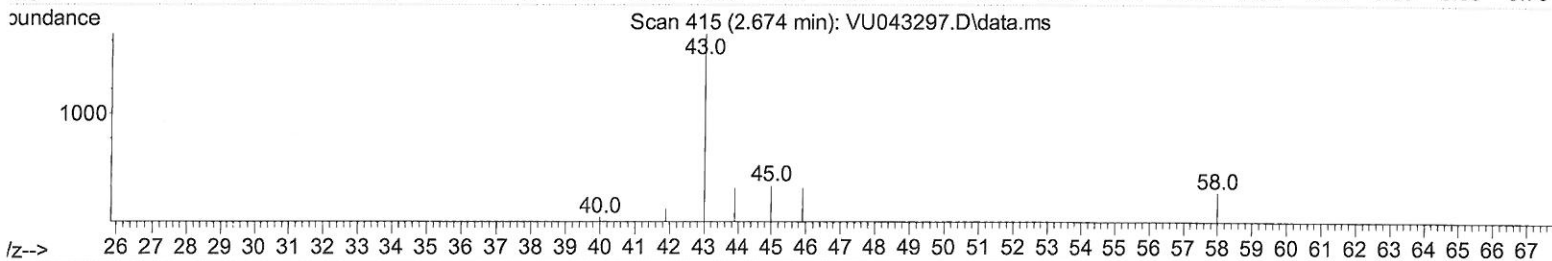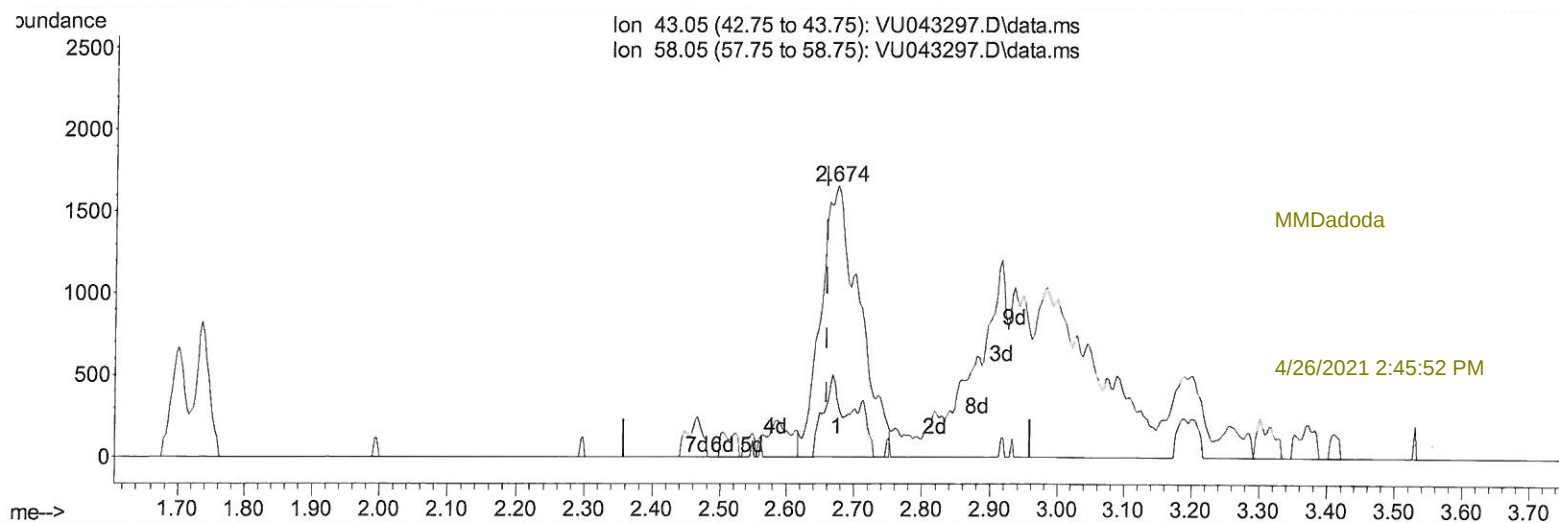

(13) Acetone (T)

2.674min (+ 0.016) 3.53 ug/L m

response 6535

| Ion   | Exp%   | Act%   |
|-------|--------|--------|
| 43.05 | 100.00 | 100.00 |
| 58.05 | 12.50  | 12.82  |
| 0.00  | 0.00   | 0.00   |
| 0.00  | 0.00   | 0.00   |

*MD*  
*4/27/21*

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU042321\  
 Data File : VU043297.D  
 Acq On : 23 Apr 2021 17:34  
 Operator : SY/MD  
 Sample : M2127-04  
 Misc : 25.0mL/MSVOA\_U/WATER  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 MSVOA\_U  
 ClientSampled :  
 E0AA1

Manual Integrations  
 APPROVED

Quant Time: Apr 24 06:33:58 2021  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\SFAMUTR041521WMA.M  
 Quant Title : TRACE VOA SFAM1.0  
 Last Update : Sat Apr 24 06:31:00 2021  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc | Units | Dev(Min) |
|----------------------------|--------|------|----------|------|-------|----------|
| Internal Standards         |        |      |          |      |       |          |
| 1) 1,4-Difluorobenzene     | 6.256  | 114  | 112897   | 5.00 | ug/L  | # 0.00   |
| 28) Chlorobenzene-d5       | 9.423  | 117  | 112055   | 5.00 | ug/L  | 0.00     |
| 58) 1,4-Dichlorobenzene-d4 | 11.819 | 152  | 51184    | 5.00 | ug/L  | 0.00     |

| Compound                      | R.T.   | QIon           | Response | Conc  | Units   | Dev(Min) |
|-------------------------------|--------|----------------|----------|-------|---------|----------|
| System Monitoring Compounds   |        |                |          |       |         |          |
| 4) Vinyl Chloride-d3          | 1.604  | 65             | 24124    | 4.20  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 40 - 130 | Recovery | =     | 84.00%  |          |
| 7) Chloroethane-d5            | 1.922  | 69             | 21436    | 3.96  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 130 | Recovery | =     | 79.20%  |          |
| 11) 1,1-Dichloroethene-d2     | 2.575  | 65             | 15645    | 4.71  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 125 | Recovery | =     | 94.20%  |          |
| 20) 2-Butanone-d5             | 4.652  | 46             | 132044   | 52.44 | ug/L    | 0.00     |
| Spiked Amount                 | 50.000 | Range 40 - 130 | Recovery | =     | 104.88% |          |
| 24) Chloroform-d              | 5.073  | 84             | 67216    | 4.60  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =     | 92.00%  |          |
| 26) 1,2-Dichloroethane-d4     | 5.710  | 65             | 43314    | 4.39  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =     | 87.80%  |          |
| 32) Benzene-d6                | 5.735  | 84             | 121134   | 4.64  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 125 | Recovery | =     | 92.80%  |          |
| 36) 1,2-Dichloropropane-d6    | 6.697  | 67             | 40770    | 4.71  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 60 - 140 | Recovery | =     | 94.20%  |          |
| 41) Toluene-d8                | 7.906  | 98             | 104149   | 3.84  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 70 - 130 | Recovery | =     | 76.80%  |          |
| 43) trans-1,3-Dichloroprop... | 8.185  | 79             | 15273    | 4.00  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 55 - 130 | Recovery | =     | 80.00%  |          |
| 46) 2-Hexanone-d5             | 8.642  | 63             | 77914    | 40.89 | ug/L    | 0.00     |
| Spiked Amount                 | 50.000 | Range 45 - 130 | Recovery | =     | 81.78%  |          |
| 56) 1,1,2,2-Tetrachloroeth... | 10.764 | 84             | 32771    | 4.31  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 65 - 120 | Recovery | =     | 86.20%  |          |
| 66) 1,2-Dichlorobenzene-d4    | 12.201 | 152            | 41857    | 4.77  | ug/L    | 0.00     |
| Spiked Amount                 | 5.000  | Range 80 - 120 | Recovery | =     | 95.40%  |          |

MMDadoda

4/26/2021 2:45:52 PM

| Target Compounds | R.T.  | QIon | Response | Conc | Units | Qvalue |
|------------------|-------|------|----------|------|-------|--------|
| 13) Acetone      | 2.674 | 43   | 6535m    | 3.53 | ug/L  |        |

7 MD  
 4/27/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed