

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
 Data File : VU043297.D
 Acq On : 23 Apr 2021 17:34
 Operator : SY/MD
 Sample : M2127-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AA1

Manual Integrations
 APPROVED

MMDadoda
 4/26/2021 2:45:52 PM

Quant Time: Apr 24 06:33:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 24 06:31:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	112897	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	112055	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	51184	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	24124	4.20	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.00%
7) Chloroethane-d5	1.922	69	21436	3.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	79.20%
11) 1,1-Dichloroethene-d2	2.575	65	15645	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	94.20%
20) 2-Butanone-d5	4.652	46	132044	52.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.88%
24) Chloroform-d	5.073	84	67216	4.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.00%
26) 1,2-Dichloroethane-d4	5.710	65	43314	4.39	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.80%
32) Benzene-d6	5.735	84	121134	4.64	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.80%
36) 1,2-Dichloropropane-d6	6.697	67	40770	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.906	98	104149	3.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	76.80%
43) trans-1,3-Dichloroprop...	8.185	79	15273	4.00	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.00%
46) 2-Hexanone-d5	8.642	63	77914	40.89	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.78%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	32771	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
66) 1,2-Dichlorobenzene-d4	12.201	152	41857	4.77	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	95.40%
Target Compounds						Qvalue
13) Acetone	2.674	43	6535m	3.53	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043297.D
Acq On : 23 Apr 2021 17:34
Operator : SY/MD
Sample : M2127-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
E0AA1

Manual Integrations
APPROVED


MMDadoda
4/26/2021 2:45:52 PM

Quant Time: Apr 24 06:33:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 24 06:31:00 2021
Response via : Initial Calibration


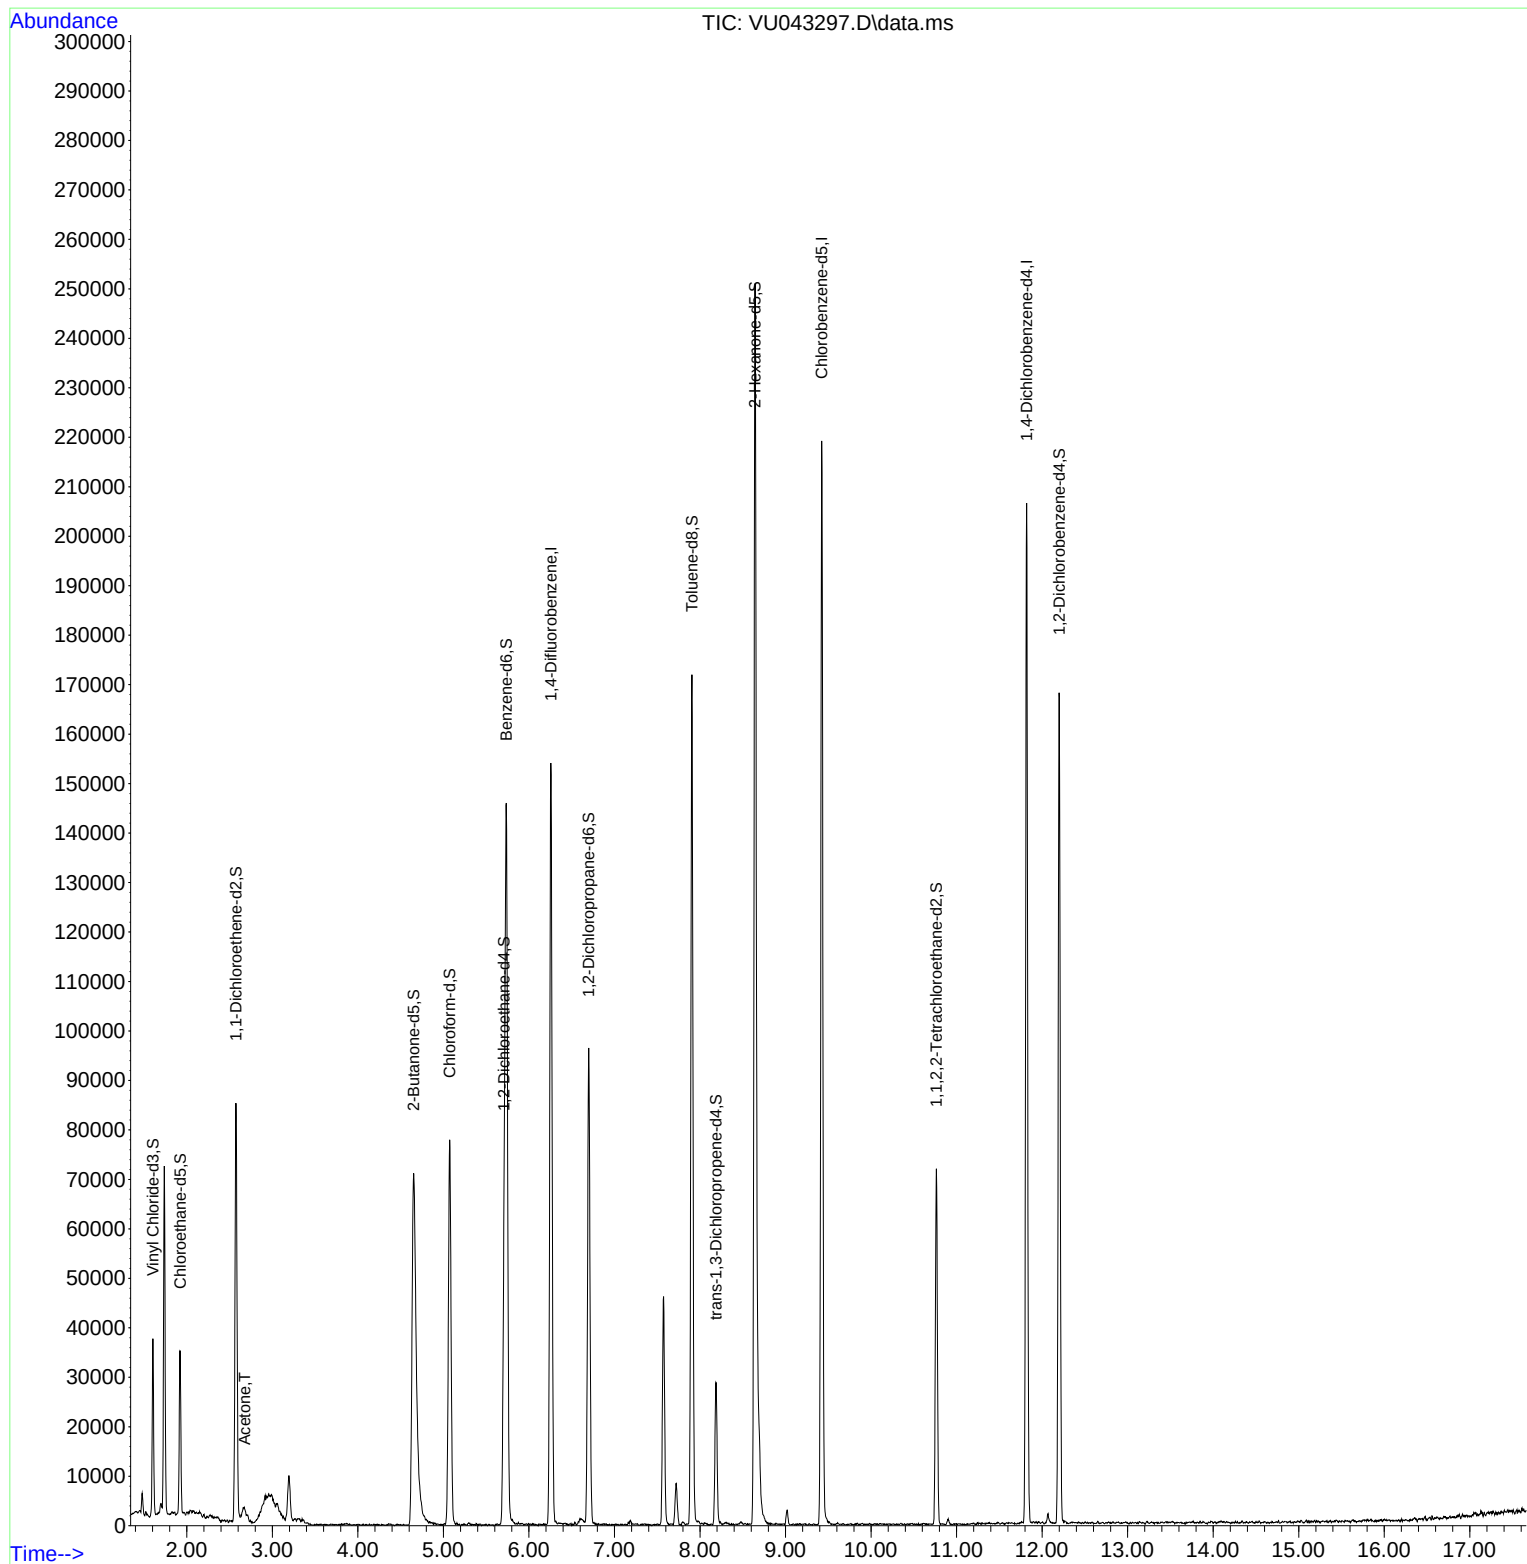


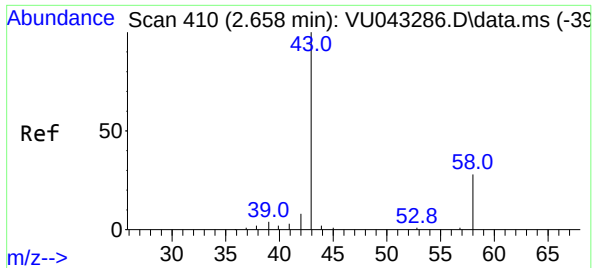

#13
Acetone
Concen: 3.53 ug/L m
RT: 2.674 min Scan# 415
Delta R.T. 0.016 min
Lab File: VU043297.D
Acq: 23 Apr 2021 17:34

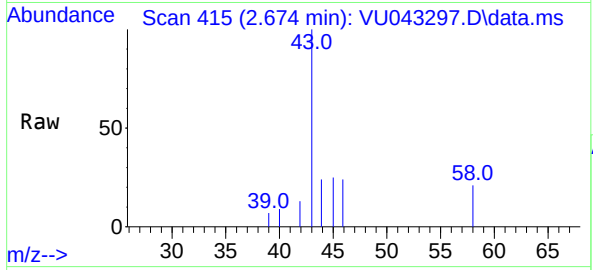

Tgt Ion: 43 Resp: 6535
Ion Ratio Lower Upper
43 100
58 12.8 0.0 25.0

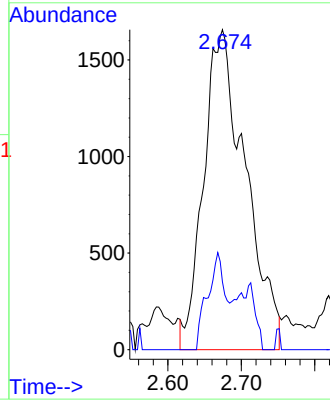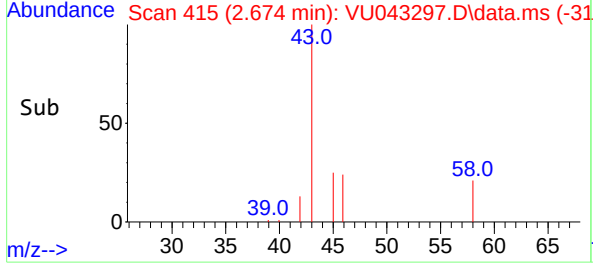

Instrument :
MSVOA_U
ClientSampleId :
E0AA1

Manual Integrations
APPROVED

MMDadoda
4/26/2021 2:45:52 PM