

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
 Data File : VU043300.D
 Acq On : 23 Apr 2021 18:46
 Operator : SY/MD
 Sample : M2127-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AB1

Quant Time: Apr 24 06:34:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 24 06:31:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.259	114	101628	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	101371	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	46189	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	23644	4.58	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.60%
7) Chloroethane-d5	1.919	69	21622	4.44	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	88.80%
11) 1,1-Dichloroethene-d2	2.575	65	16374	5.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	109.40%
20) 2-Butanone-d5	4.652	46	134719	59.44	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	118.88%
24) Chloroform-d	5.073	84	66982	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
26) 1,2-Dichloroethane-d4	5.710	65	42552	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.80%
32) Benzene-d6	5.735	84	119327	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.20%
36) 1,2-Dichloropropane-d6	6.700	67	40252	5.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.80%
41) Toluene-d8	7.906	98	101094	4.12	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.40%
43) trans-1,3-Dichloroprop...	8.185	79	15419	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.645	63	79421	46.07	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.14%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	33423	4.85	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.00%
66) 1,2-Dichlorobenzene-d4	12.201	152	40693	5.14	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	102.80%
Target Compounds					Qvalue	
13) Acetone	2.668	43	4160	2.50	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043300.D
Acq On : 23 Apr 2021 18:46
Operator : SY/MD
Sample : M2127-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AB1

Quant Time: Apr 24 06:34:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 24 06:31:00 2021
Response via : Initial Calibration

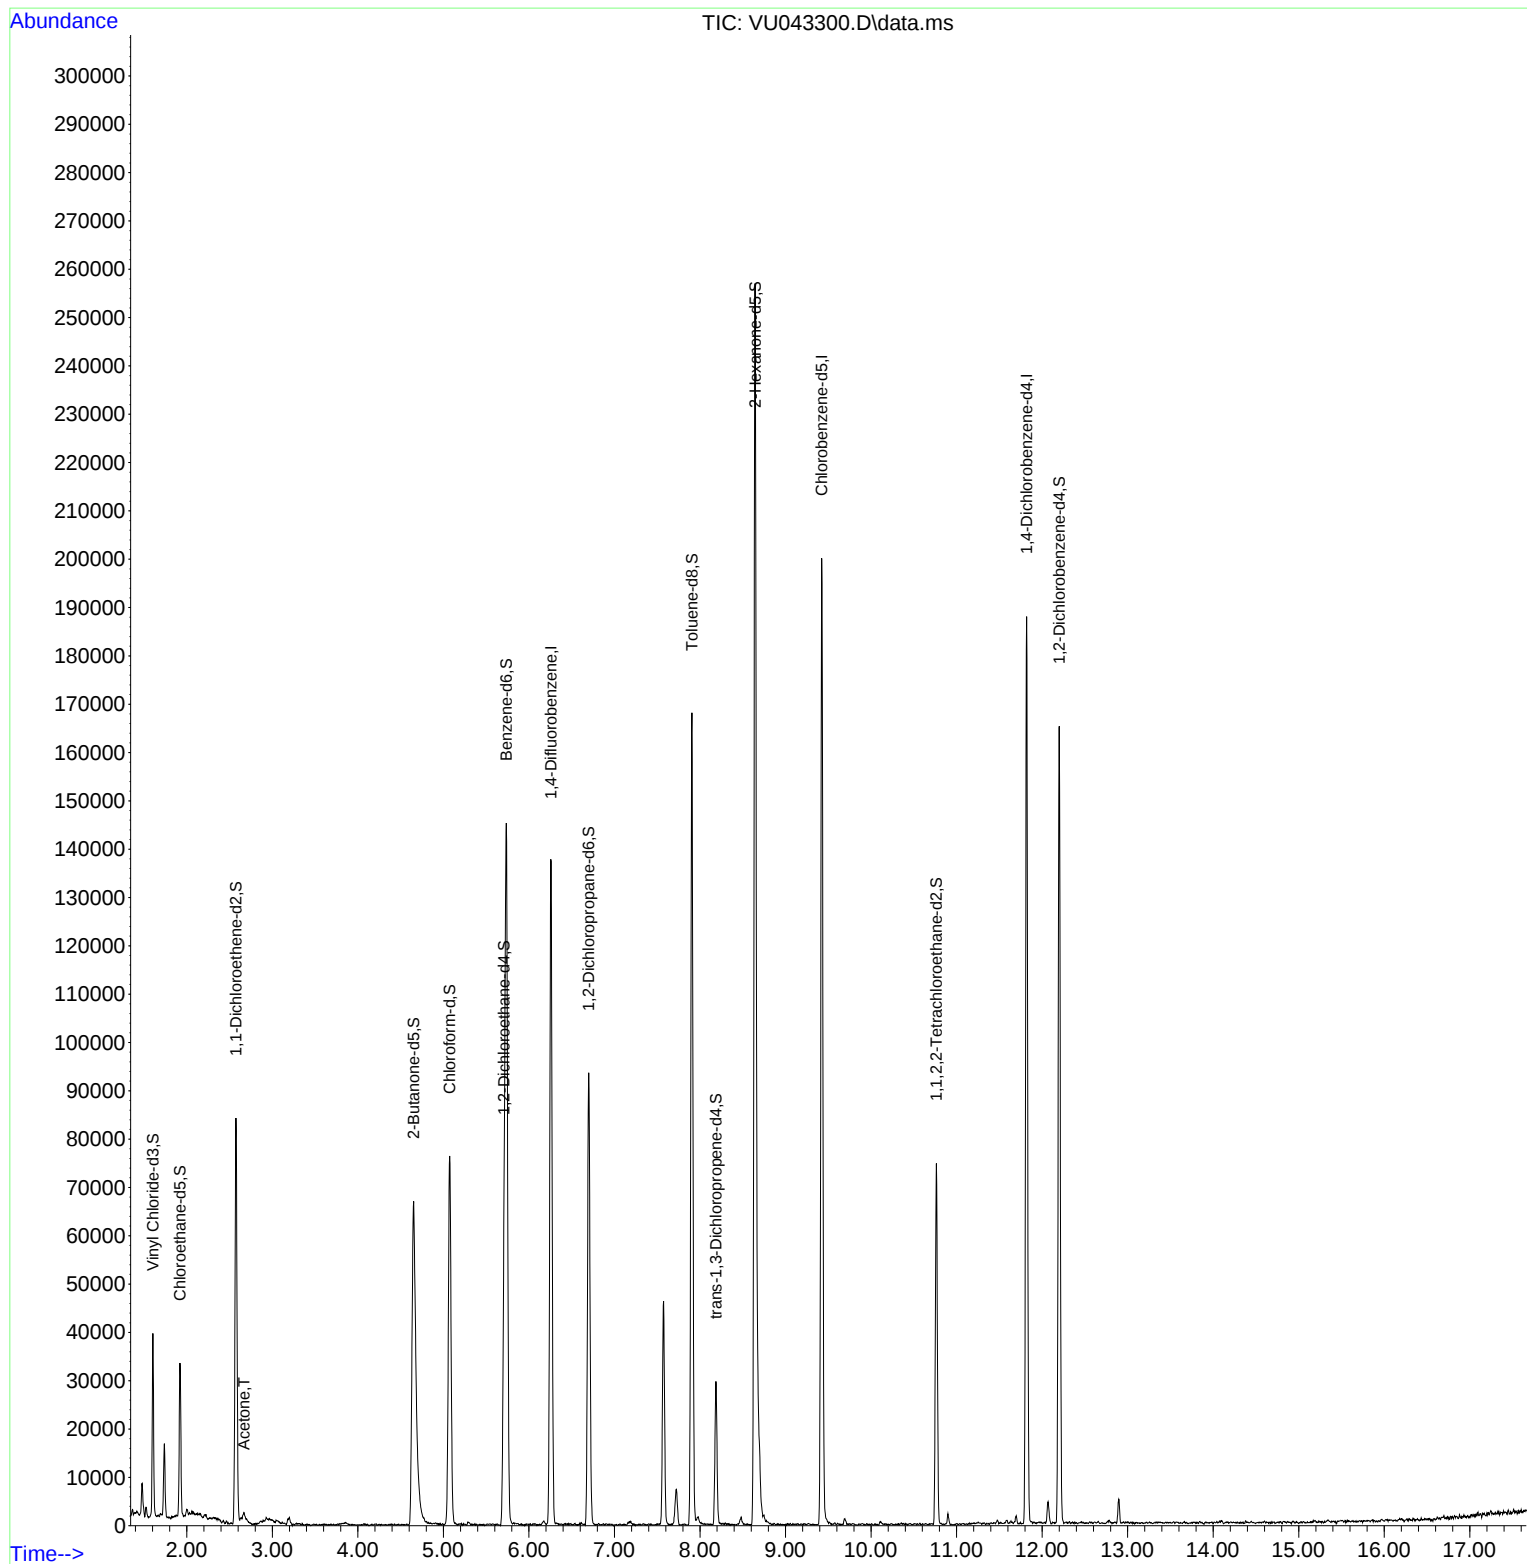

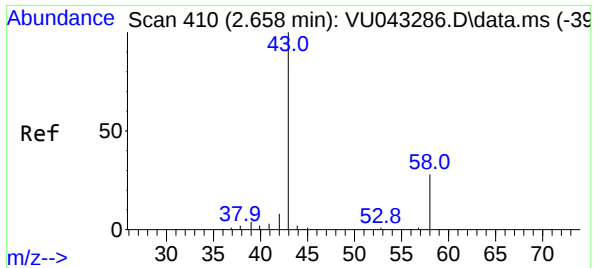

#13
 Acetone
 Concen: 2.50 ug/L
 RT: 2.668 min Scan# 413
 Delta R.T. 0.010 min
 Lab File: VU043300.D
 Acq: 23 Apr 2021 18:46

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AB1

Tgt Ion:	43	Resp:	4160
Ion	Ratio	Lower	Upper
43	100		
58	8.4	0.0	25.0

