

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
 Data File : VU043307.D
 Acq On : 23 Apr 2021 21:56
 Operator : SY/MD
 Sample : VU0423WBL02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Quant Time: Apr 24 07:56:22 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat Apr 24 07:55:52 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.256	114	101811	5.00	ug/L	# 0.00
28) Chlorobenzene-d5	9.423	117	104222	5.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.819	152	45741	5.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	27567	5.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.60%
7) Chloroethane-d5	1.919	69	24605	5.05	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.00%
11) 1,1-Dichloroethene-d2	2.575	65	18125	6.05	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	121.00%
20) 2-Butanone-d5	4.665	46	141517	62.32	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.64%
24) Chloroform-d	5.073	84	72699	5.52	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	110.40%
26) 1,2-Dichloroethane-d4	5.713	65	47438	5.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.60%
32) Benzene-d6	5.735	84	129627	5.34	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	106.80%
36) 1,2-Dichloropropane-d6	6.700	67	43392	5.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.80%
41) Toluene-d8	7.906	98	110129	4.37	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.40%
43) trans-1,3-Dichloroprop...	8.185	79	16556	4.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.20%
46) 2-Hexanone-d5	8.645	63	86612	48.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.74%
56) 1,1,2,2-Tetrachloroeth...	10.764	84	37820	5.34	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	106.80%
66) 1,2-Dichlorobenzene-d4	12.201	152	44654	5.70	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.00%
Target Compounds						
48) 2-Hexanone	8.693	43	6571	1.27	ug/L	# 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043307.D
Acq On : 23 Apr 2021 21:56
Operator : SY/MD
Sample : VU0423WBL02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK138

Quant Time: Apr 24 07:56:22 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat Apr 24 07:55:52 2021
Response via : Initial Calibration

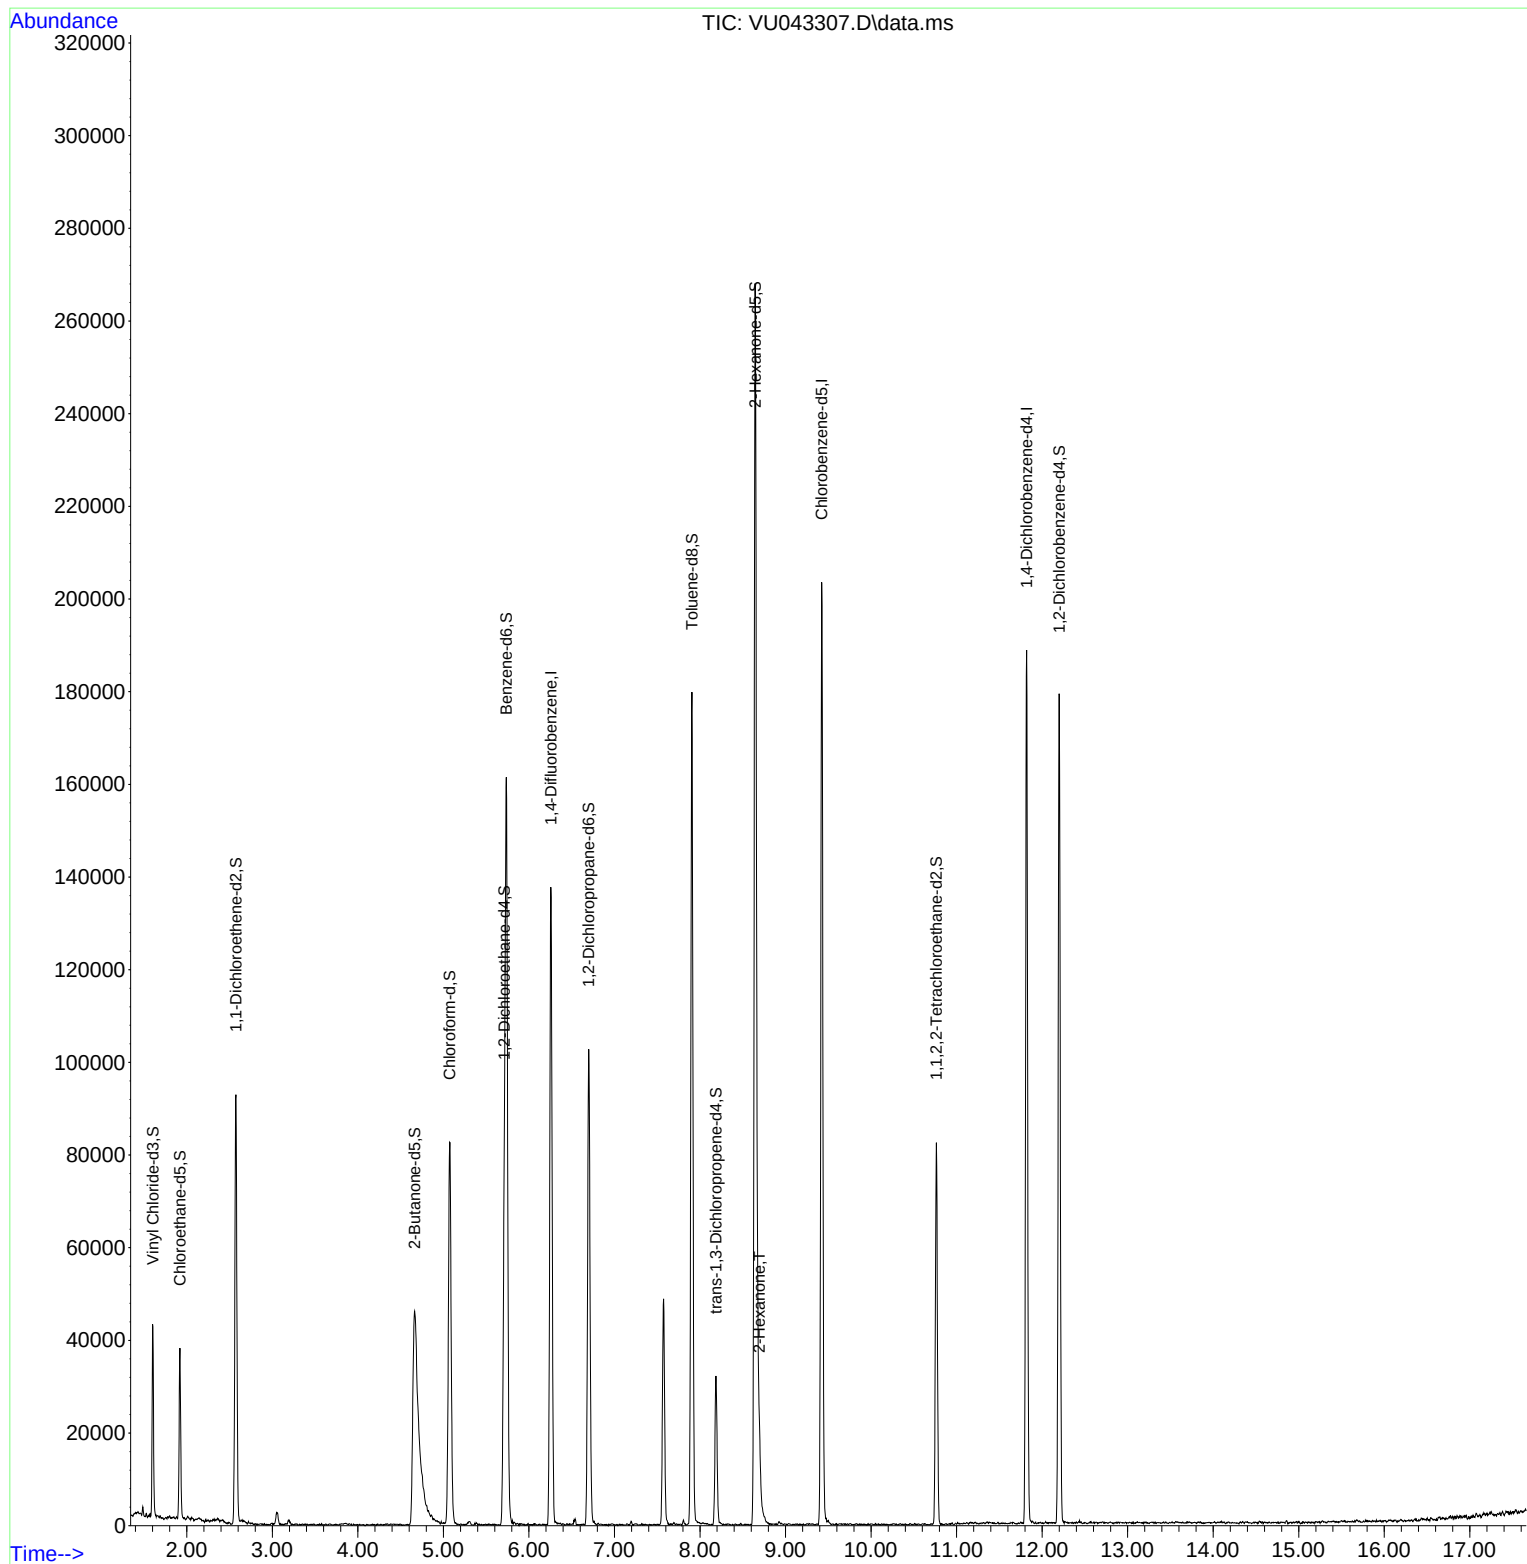

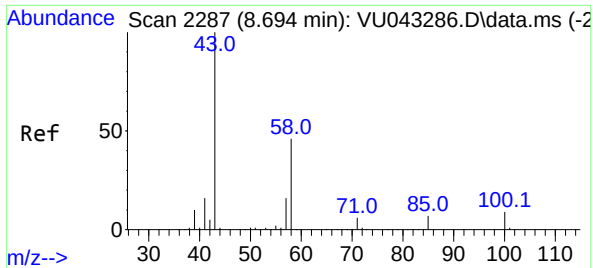

#48
 2-Hexanone
 Concen: 1.27 ug/L
 RT: 8.693 min Scan# 2287
 Delta R.T. -0.000 min
 Lab File: VU043307.D
 Acq: 23 Apr 2021 21:56

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK138

Tgt Ion: 43 Resp: 6571

Ion	Ratio	Lower	Upper
43	100		
58	54.2	50.0	75.0
57	23.0	17.4	26.0
100	5.6	11.8	17.8

