

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
 Data File : VU043300.D
 Acq On : 23 Apr 2021 18:46
 Operator : SY/MD
 Sample : M2127-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AB1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU043300.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.478	37	43	52	rVB4	6971	9228	1.80%	0.269%
2	1.604	75	82	95	rVB	37854	40928	8.00%	1.191%
3	1.739	116	124	134	rVB	15305	18910	3.70%	0.550%
4	1.919	172	180	193	rVB	31812	42625	8.33%	1.241%
5	2.575	372	384	398	rBV	84039	136874	26.76%	3.984%
6	4.652	1013	1030	1066	rBV	66972	218663	42.75%	6.365%
7	5.073	1140	1161	1179	rBV3	76415	167807	32.81%	4.885%
8	5.735	1346	1367	1390	rBV3	145422	385447	75.36%	11.220%
9	6.256	1512	1529	1546	rBV	137709	257487	50.34%	7.495%
10	6.700	1654	1667	1686	rBV2	93586	182822	35.74%	5.322%
11	7.575	1927	1939	1957	rVB3	46296	79563	15.56%	2.316%
12	7.722	1970	1985	1996	rVB4	7388	14498	2.83%	0.422%
13	7.906	2028	2042	2056	rBV	168080	286231	55.96%	8.332%
14	8.185	2118	2129	2142	rBV2	29645	49075	9.59%	1.429%
15	8.645	2258	2272	2300	rBV	256876	511468	100.00%	14.889%
16	9.423	2502	2514	2535	rBV	199894	332129	64.94%	9.668%
17	10.764	2919	2931	2945	rBV2	74739	119150	23.30%	3.468%
18	11.819	3246	3259	3275	rBV	187727	298572	58.38%	8.691%
19	12.070	3326	3337	3348	rVB4	4608	7424	1.45%	0.216%
20	12.201	3366	3378	3394	rVB	164992	269528	52.70%	7.846%
21	12.896	3586	3594	3601	rVB5	5017	6854	1.34%	0.200%




Sum of corrected areas: 3435283

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043300.D
Acq On : 23 Apr 2021 18:46
Operator : SY/MD
Sample : M2127-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

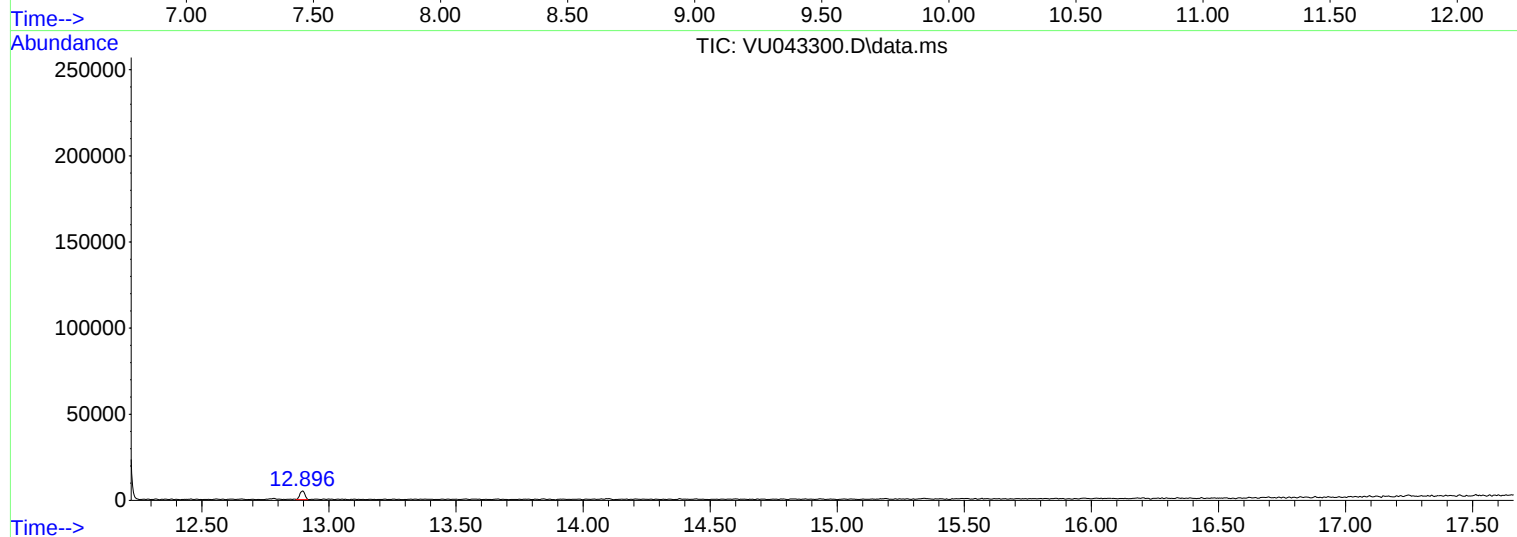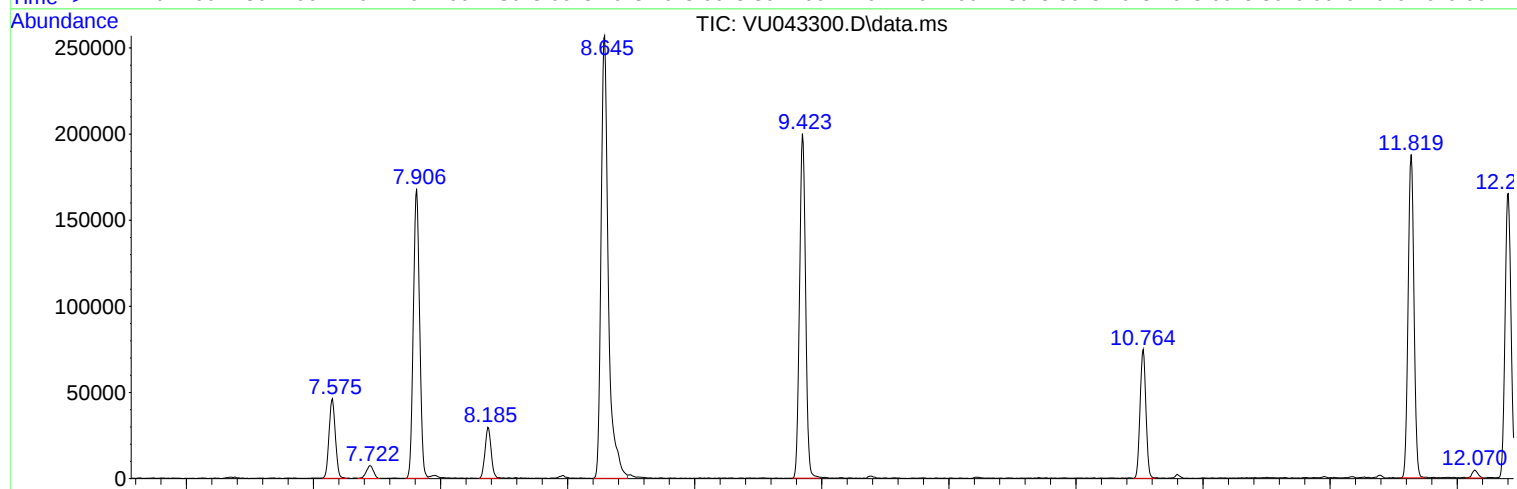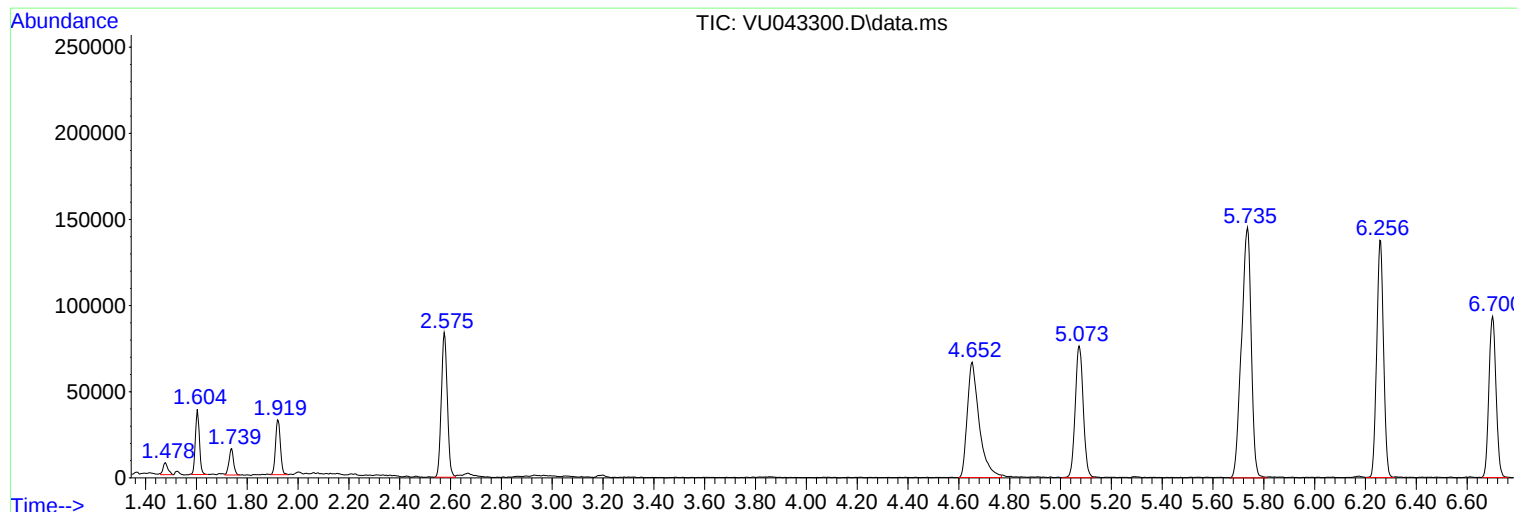

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043300.D
Acq On : 23 Apr 2021 18:46
Operator : SY/MD
Sample : M2127-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043300.D
Acq On : 23 Apr 2021 18:46
Operator : SY/MD
Sample : M2127-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AB1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------