

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
 Data File : VU043304.D
 Acq On : 23 Apr 2021 20:21
 Operator : SY/MD
 Sample : M2162-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H4507

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043304.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.395	10	17	29	rVB	218078	228673	42.43%	5.098%
2	1.604	68	82	90	rBV2	43901	68330	12.68%	1.523%
3	1.922	174	181	192	rVB	33212	43467	8.07%	0.969%
4	2.575	373	384	399	rBV	85273	140634	26.10%	3.136%
5	3.375	616	633	658	rBV2	109225	258516	47.97%	5.764%
6	4.655	1015	1031	1062	rBV2	68176	250107	46.41%	5.576%
7	5.073	1145	1161	1185	rBV	77972	179251	33.26%	3.997%
8	5.735	1345	1367	1390	rBV2	149054	392143	72.76%	8.743%
9	6.256	1515	1529	1550	rBV	137060	259507	48.15%	5.786%
10	6.552	1610	1621	1635	rVB3	9973	18104	3.36%	0.404%
11	6.700	1654	1667	1685	rVB	99300	189395	35.14%	4.223%
12	7.575	1928	1939	1952	rBV2	45925	80487	14.93%	1.795%
13	7.906	2028	2042	2059	rBV	169954	289724	53.76%	6.460%
14	8.189	2118	2130	2142	rBV	30801	51310	9.52%	1.144%
15	8.558	2233	2245	2259	rBV	271052	456476	84.70%	10.177%
16	8.645	2259	2272	2302	rVB	267046	538927	100.00%	12.016%
17	9.423	2502	2514	2537	rBV	202496	335117	62.18%	7.472%
18	10.764	2919	2931	2945	rBV	79231	125252	23.24%	2.793%
19	11.819	3247	3259	3274	rBV	191110	302330	56.10%	6.741%
20	12.198	3366	3377	3391	rBV	171876	277433	51.48%	6.186%




Sum of corrected areas: 4485183

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043304.D
Acq On : 23 Apr 2021 20:21
Operator : SY/MD
Sample : M2162-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

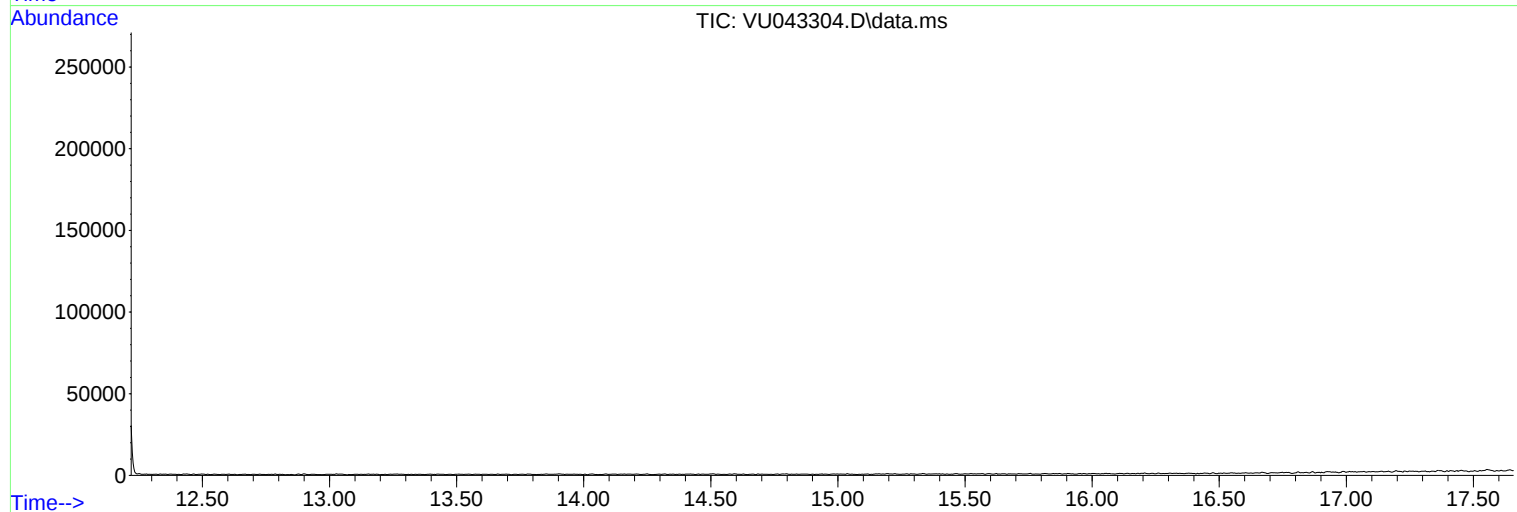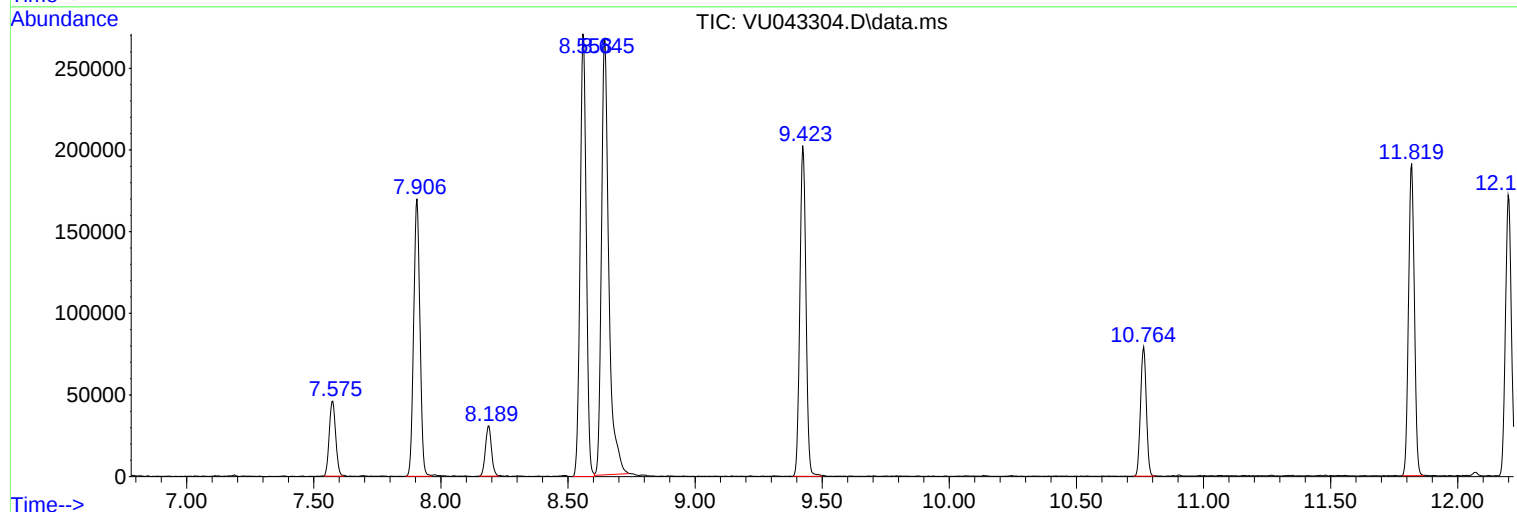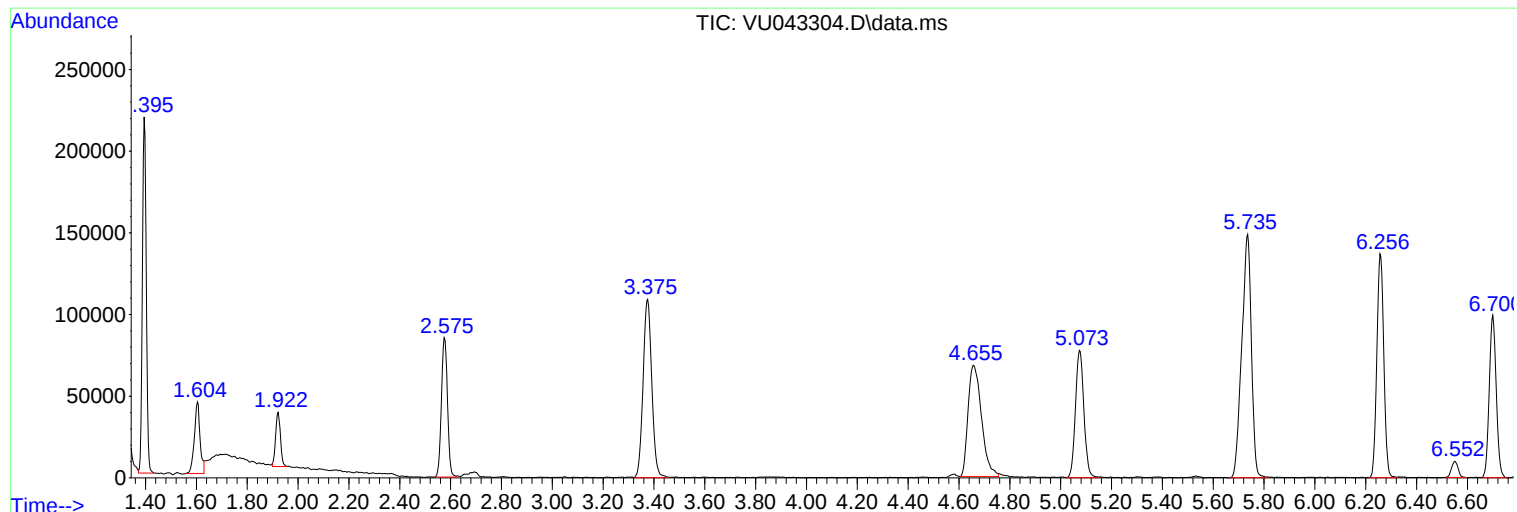

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043304.D
Acq On : 23 Apr 2021 20:21
Operator : SY/MD
Sample : M2162-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043304.D
Acq On : 23 Apr 2021 20:21
Operator : SY/MD
Sample : M2162-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H4507

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
