
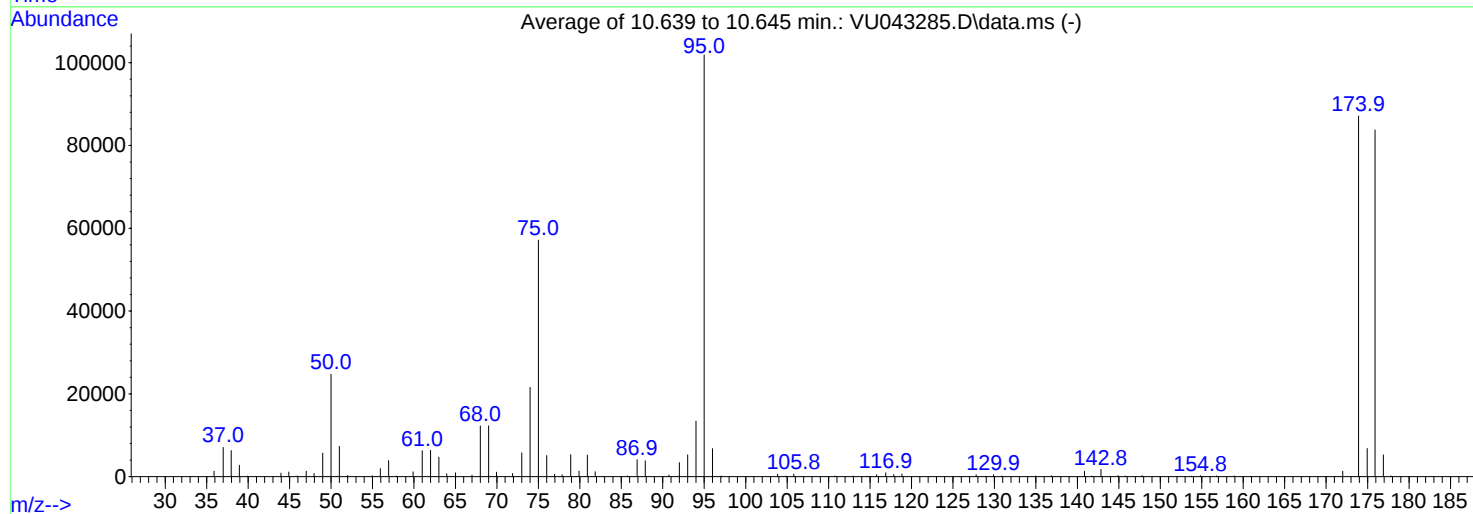


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042321\
Data File : VU043285.D
Acq On : 23 Apr 2021 09:43
Operator : SY/MD
Sample : BFB35
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB135

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Apr 24 07:55:52 2021

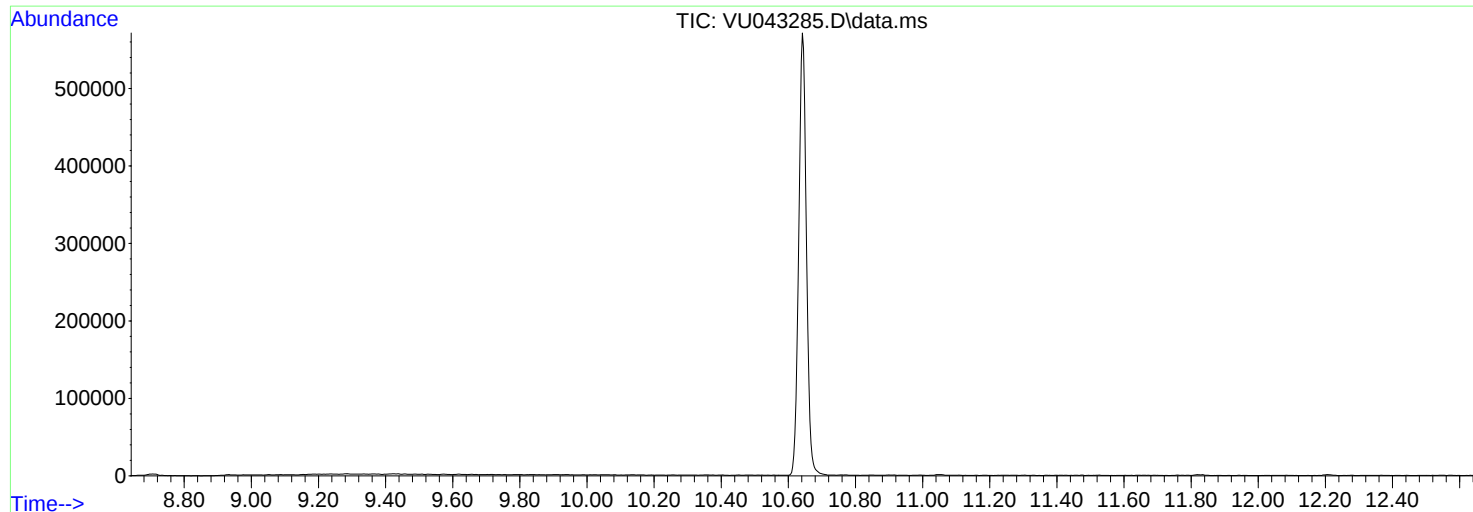

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.3	24741	PASS
75	95	30	80	56.1	57117	PASS
95	95	100	100	100.0	101885	PASS
96	95	5	9	6.6	6771	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	87128	PASS
175	174	5	9	7.8	6797	PASS
176	174	95	101	96.1	83731	PASS
177	176	5	9	6.3	5273	PASS

m/z	Abundance
35.90	401.0
37.90	190.0
43.90	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	1751.0
37.00	7080.0
38.00	6323.0
39.00	2789.0
39.90	158.0
44.00	1120.0
44.90	1089.0
45.90	121.0
47.00	1171.0
48.00	773.0
49.00	5680.0
50.00	24672.0
51.00	7127.0
52.00	314.0
55.00	264.0
55.90	1907.0
57.00	3838.0
57.90	118.0
59.90	1162.0
61.00	6338.0
62.00	6426.0
63.00	4741.0
64.00	706.0
65.00	1006.0
65.90	118.0
67.00	315.0
68.00	11938.0
69.00	12066.0
70.00	1018.0
71.90	720.0
73.00	5512.0
74.00	21088.0
75.00	56424.0
76.00	4964.0
76.90	627.0
77.80	409.0
78.90	5187.0
79.90	1290.0
80.90	5091.0
81.80	1240.0
85.80	137.0
86.90	3871.0
87.90	3565.0
90.70	403.0
92.00	3155.0
93.00	5210.0
94.00	13007.0
95.00	98376.0
96.00	6736.0
97.00	156.0
103.90	569.0
104.80	173.0
105.80	596.0
110.00	106.0
110.70	134.0
112.90	181.0
114.60	110.0
115.80	376.0
116.90	947.0
117.90	504.0
118.80	657.0
127.80	434.0
128.90	129.0
129.90	423.0
130.90	159.0
134.90	107.0
136.80	272.0
140.80	1198.0
141.70	166.0
142.90	1593.0
144.00	126.0
144.90	295.0
145.70	164.0
147.80	240.0
153.70	119.0
154.80	250.0
156.80	203.0
158.90	161.0
160.90	141.0
171.10	237.0
172.00	1310.0
173.90	81888.0
174.90	6498.0
175.90	79264.0
176.90	5221.0
177.80	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
36.00	1660.0
37.00	6769.0
38.00	6456.0
38.90	2691.0
40.00	139.0
44.00	1024.0
44.90	1083.0
45.90	160.0
47.00	1475.0
47.90	787.0
49.00	5459.0
50.00	24088.0
51.00	7346.0
52.00	233.0
54.90	198.0
56.00	1895.0
56.90	3736.0
57.90	181.0
59.90	1136.0
61.00	6009.0
62.00	6088.0
63.00	4540.0
63.90	698.0
65.00	865.0
67.00	365.0
68.00	12122.0
69.00	12171.0
69.90	1102.0
71.90	782.0
73.00	5807.0
74.00	21280.0
75.00	55952.0
76.00	5056.0
77.00	488.0
77.90	524.0
78.90	5202.0
79.90	1371.0
80.90	5209.0
81.90	1151.0
82.90	127.0
85.70	220.0
86.90	4192.0
87.90	3963.0
90.80	390.0
92.00	3533.0
93.00	5138.0
94.00	13331.0
95.00	101672.0
96.00	6504.0
96.90	105.0
97.10	101.0
103.80	558.0
104.90	165.0
105.80	648.0
106.90	127.0
110.80	154.0
113.00	107.0
114.90	103.0
115.80	540.0
116.90	841.0
117.80	515.0
118.90	684.0
127.80	446.0
129.90	516.0
130.90	176.0
135.00	191.0
136.90	215.0
140.00	107.0
140.90	1369.0
141.80	164.0
142.80	1811.0
144.90	262.0
145.80	166.0
147.80	273.0
153.80	110.0
154.90	245.0
156.80	182.0
158.90	209.0
172.00	1248.0
173.90	89232.0
175.00	6807.0
175.90	85368.0
176.90	5104.0
177.80	198.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135

m/z	Abundance
35.90	1770.0
37.00	7432.0
38.00	6706.0
38.90	2794.0
40.00	137.0
44.00	1109.0
44.90	1143.0
45.90	153.0
47.00	1343.0
48.00	777.0
49.00	5873.0
50.00	25464.0
51.00	7474.0
52.00	297.0
55.00	237.0
56.00	1985.0
57.00	3987.0
57.90	167.0
59.90	1180.0
61.00	6448.0
62.00	6564.0
63.00	4903.0
64.00	713.0
65.00	949.0
67.00	337.0
68.00	12732.0
69.00	12684.0
69.90	1118.0
71.90	801.0
73.00	5968.0
74.00	22392.0
75.00	58976.0
76.00	5321.0
77.00	583.0
77.80	484.0
78.90	5521.0
79.90	1372.0
80.90	5388.0
81.80	1246.0
82.90	110.0
85.80	194.0
86.90	4228.0
87.90	3988.0
90.70	385.0
92.00	3520.0
93.00	5470.0
94.00	13945.0
95.00	105608.0
96.00	7073.0
97.10	132.0
103.90	590.0
104.90	165.0
105.80	629.0
110.00	100.0
110.70	165.0
113.00	166.0
114.60	113.0
114.90	108.0
115.80	488.0
116.90	982.0
117.80	537.0
118.80	685.0
127.80	477.0
129.90	500.0
130.90	174.0
135.00	168.0
136.80	255.0
140.90	1351.0
141.70	172.0
142.80	1806.0
144.00	112.0
144.90	310.0
145.80	154.0
147.80	265.0
153.70	123.0
154.80	268.0
156.80	214.0
158.90	200.0
160.90	102.0
172.00	1395.0
173.90	90264.0
174.90	7087.0
175.90	86560.0
176.90	5493.0
177.80	235.0

Instrument :
MSVOA_U
ClientSampleId :
BFB135