

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042419\

Data File : VU031489.D

Acq On : 24 Apr 2019 22:47

Operator : JC/SP

Sample : K2536-12

Misc : 25.0mL/MSVOA U/WATER

ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 25 10:58:00 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Thu Apr 25 06:05:25 2019

Response via : Initial Calibration

Instrument :

MSVOA_U

ClientSampleId :


C0XG2

Manual Integrations

APPROVED

MMDadoda

4/25/2019 10:57:29 AM

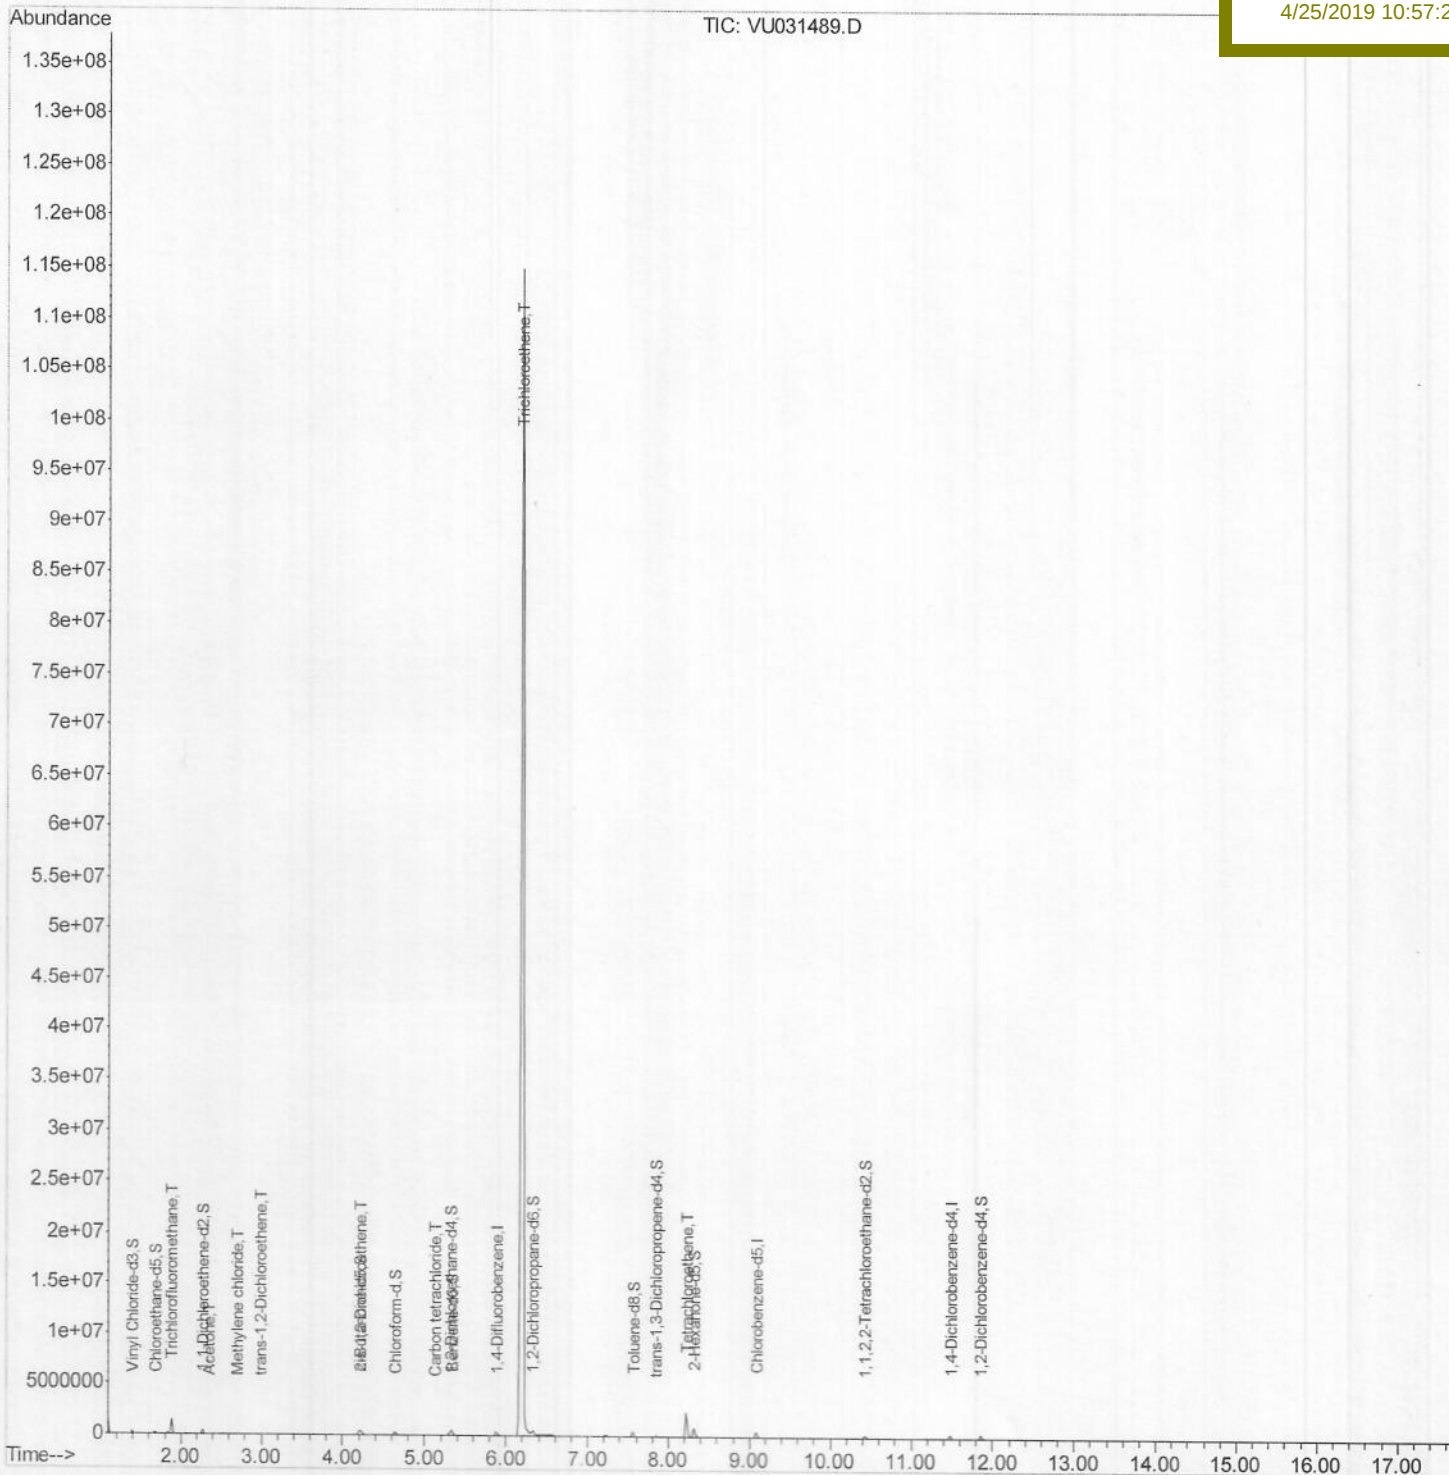




Data File : VU031489.D
Acq On : 24 Apr 2019 22:47
Operator : JC/SP
Sample : K2536-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 25 06:12:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 06:05:25 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
C0XG2

Manual Integrations
APPROVED

MMDadoda
4/25/2019 10:57:29 AM

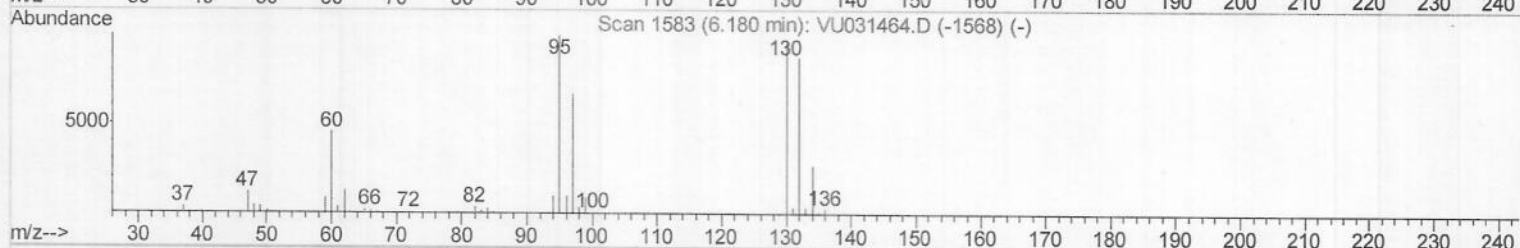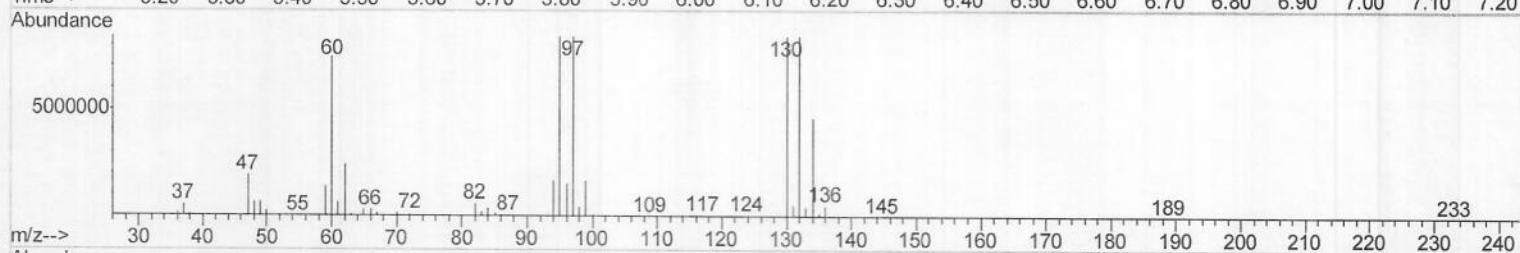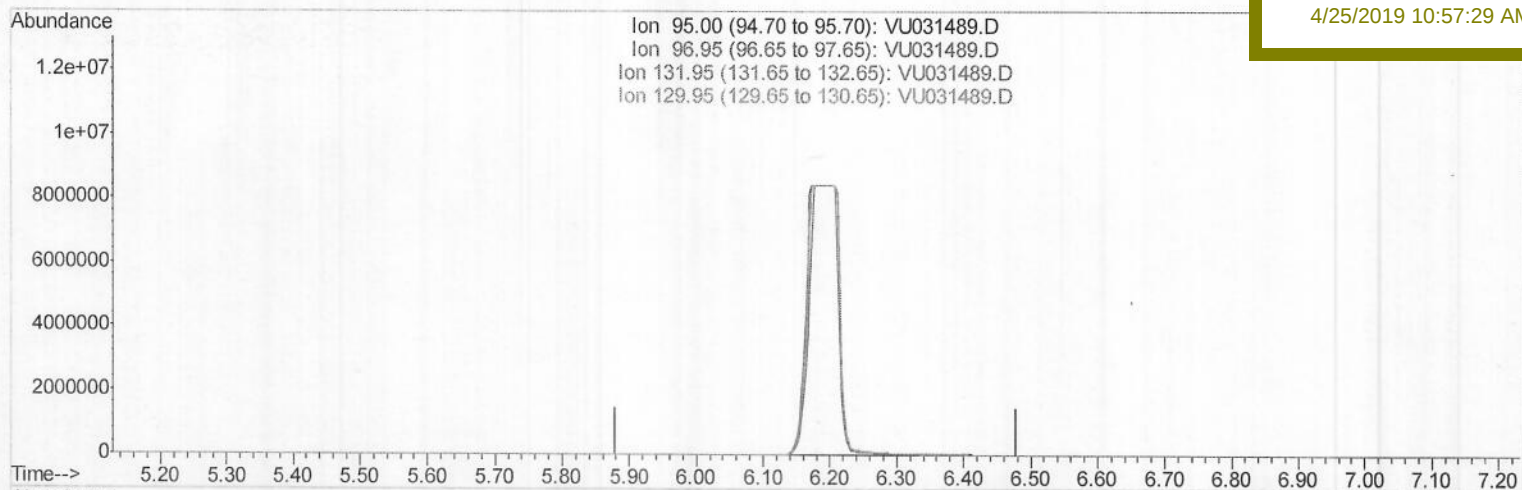

(34) Trichloroethene (T)

6.180min (-6.180) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
96.95	63.30	0.00#
131.95	85.60	0.00#
129.95	95.80	0.00#




Data File : VU031489.D
Acq On : 24 Apr 2019 22:47
Operator : JC/SP
Sample : K2536-12
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Quant Time: Apr 25 06:12:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 06:05:25 2019
Response via : Initial Calibration

Instrument :
MSVOA_U
ClientSampleId :
C0XG2

Manual Integrations
APPROVED

MMDadoda
4/25/2019 10:57:29 AM

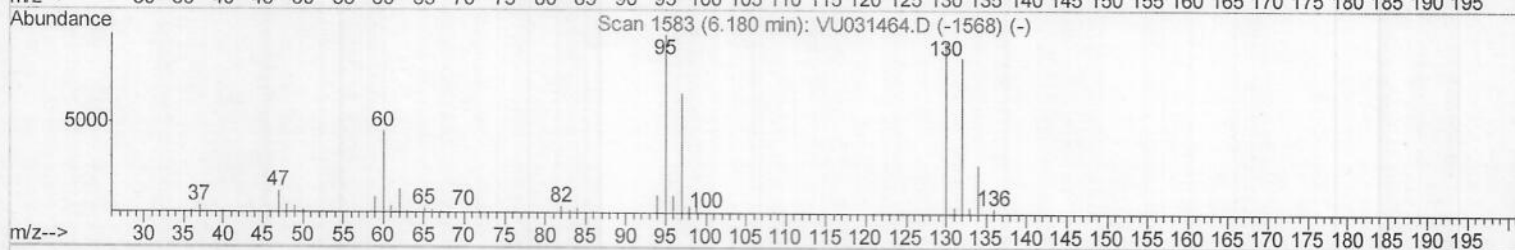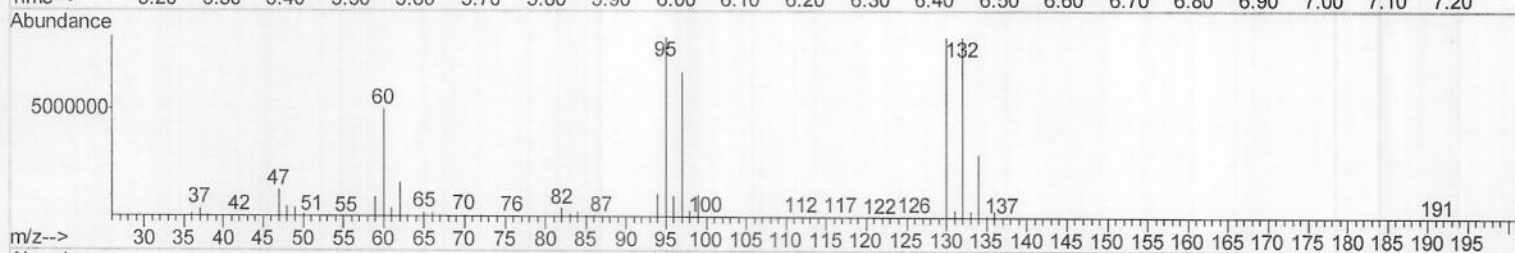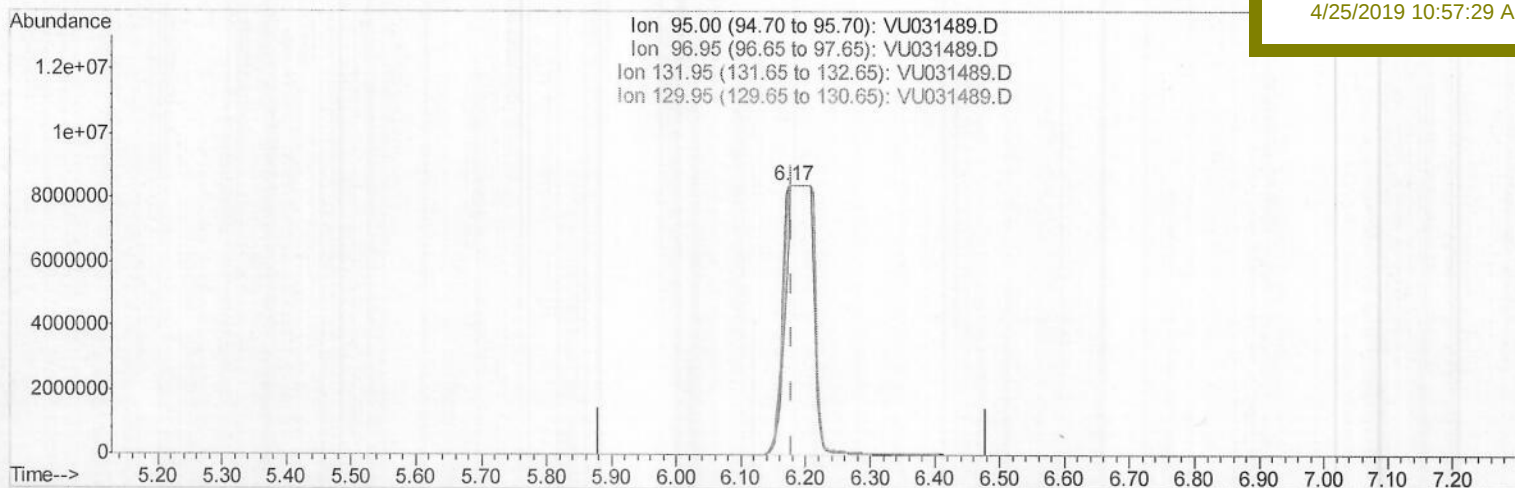

(34) Trichloroethene (T)

6.173min (-0.006) 1157.06ug/L m

response 28214514

Ion	Exp%	Act%
95.00	100	100
96.95	63.30	80.15
131.95	85.60	100.00
129.95	95.80	100.00

M.D
5/1/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042419\
 Data File : VU031489.D
 Acq On : 24 Apr 2019 22:47
 Operator : JC/SP
 Sample : K2536-12
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COXG2

Quant Time: Apr 25 10:58:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 06:05:25 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

MMDadoda
 4/25/2019 10:57:29 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	292487	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	299424	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	110519	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	129451	5.53	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	110.60%		
7) Chloroethane-d5	1.68	69	104551	5.85	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	117.00%		
11) 1,1-Dichloroethene-d2	2.27	63	188802	4.28	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	85.60%		
20) 2-Butanone-d5	4.21	46	374946	59.72	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	119.44%		
24) Chloroform-d	4.64	84	218178	5.88	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	117.60%		
26) 1,2-Dichloroethane-d4	5.31	65	124879	6.32	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	126.40%		
32) Benzene-d6	5.33	84	422685	5.20	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	104.00%		
36) 1,2-Dichloropropane-d6	6.33	67	150198	5.68	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	113.60%		
41) Toluene-d8	7.56	98	349483	4.85	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.00%		
43) trans-1,3-Dichloropropene-	7.85	79	50278	4.85	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	97.00%		
46) 2-Hexanone-d5	8.31	63	265615	52.00	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	104.00%		
57) 1,1,2,2-Tetrachloroethane-	10.43	84	112841	5.36	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	107.20%		
64) 1,2-Dichlorobenzene-d4	11.86	152	111695	5.65	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	113.00%		

Target Compounds

					Ovalue	
9) Trichlorofluoromethane	1.88	101	903318	25.699	ug/L	98
13) Acetone	2.35	43	10508	2.356	ug/L	87
16) Methylene chloride	2.69	84	3937	0.171	ug/L	97
18) trans-1,2-Dichloroethene	2.98	96	6194	0.289	ug/L	94
22) cis-1,2-Dichloroethene	4.22	96	148474	6.705	ug/L	93
31) Carbon tetrachloride	5.13	117	19465	0.661	ug/L	99
34) Trichloroethene	6.17	95	28214514m	1157.057	ug/L	98
47) Tetrachloroethene	8.22	164	565739	33.203	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

M.D
 5/2/19