

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042419\
 Data File : VU031480.D
 Acq On : 24 Apr 2019 19:07
 Operator : JC/SP
 Sample : K2517-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GAHY7

Quant Time: Apr 25 07:01:26 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 06:05:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	308078	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	311303	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	114933	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	134898	5.47	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	109.40%
7) Chloroethane-d5	1.68	69	103364	5.49	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	109.80%
11) 1,1-Dichloroethene-d2	2.27	63	194742	4.20	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	84.00%
20) 2-Butanone-d5	4.19	46	381234	57.65	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	115.30%
24) Chloroform-d	4.64	84	217848	5.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.40%
26) 1,2-Dichloroethane-d4	5.31	65	122308	5.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	117.60%
32) Benzene-d6	5.33	84	434544	5.14	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.80%
36) 1,2-Dichloropropane-d6	6.33	67	149023	5.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.40%
41) Toluene-d8	7.56	98	345605	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.20%
43) trans-1,3-Dichloropropene-	7.85	79	48003	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.31	63	243216	45.80	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.60%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	112291	5.13	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	102.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	118782	5.78	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.60%


Target Compounds				Ovalue
51) Chlorobenzene	9.12	112	11249	0.192 ug/L # 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042419\
Data File : VU031480.D
Acq On : 24 Apr 2019 19:07
Operator : JC/SP
Sample : K2517-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GAHY7

Quant Time: Apr 25 07:01:26 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 06:05:25 2019
Response via : Initial Calibration

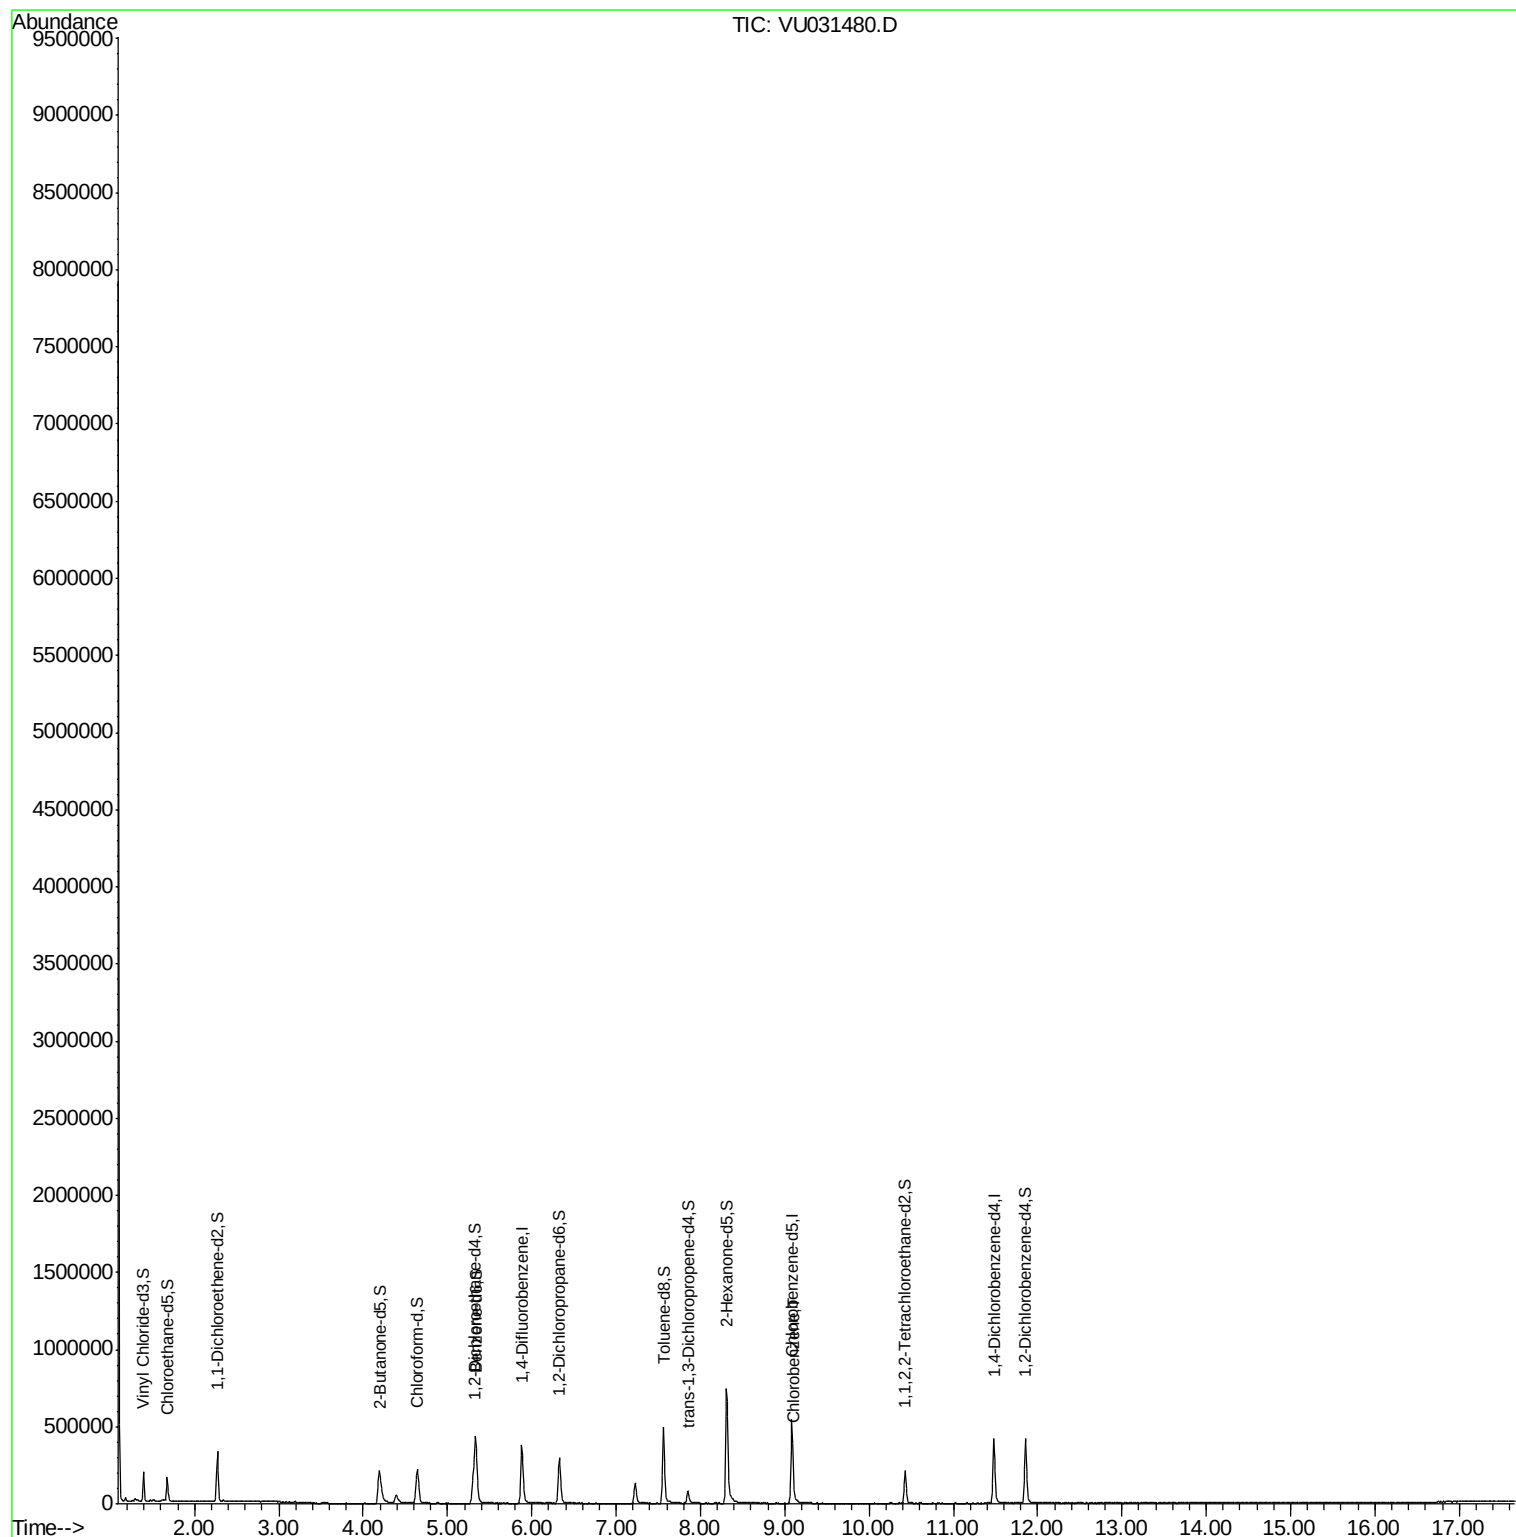

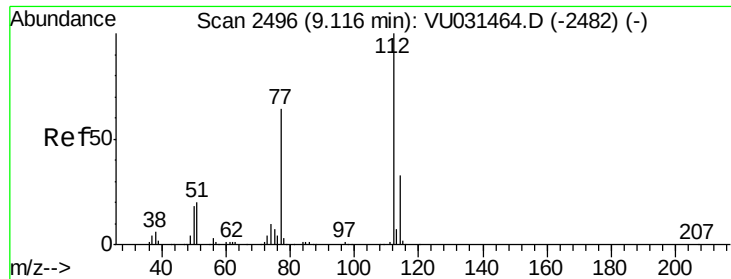

#51
 Chlorobenzene
 Concen: 0.192 ug/L
 RT: 9.12 min Scan# 2497
 Delta R.T. 0.00 min
 Lab File: VU031480.D
 Acq: 24 Apr 2019 19:07

Instrument :
 MSVOA_U
 ClientSampleId :
 GAHY7

Tot Ion	Ion	Ratio	Lower	Upper
112	100			
114	34.9	21.9	40.7	
77	75.6	48.9	73.3	

