

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042419\
 Data File : VU031486.D
 Acq On : 24 Apr 2019 21:33
 Operator : JC/SP
 Sample : K2536-06
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X61

Quant Time: Apr 25 07:16:57 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 06:05:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	304630	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	302176	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	111807	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.39	65	124149	5.09	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	101.80%
7) Chloroethane-d5	1.68	69	98075	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	105.40%
11) 1,1-Dichloroethene-d2	2.27	63	182075	3.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	79.40%
20) 2-Butanone-d5	4.19	46	361166	55.24	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	110.48%
24) Chloroform-d	4.64	84	211217	5.46	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	109.20%
26) 1,2-Dichloroethane-d4	5.31	65	117465	5.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	114.20%
32) Benzene-d6	5.33	84	418881	5.10	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.00%
36) 1,2-Dichloropropane-d6	6.33	67	141697	5.31	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	106.20%
41) Toluene-d8	7.56	98	323747	4.45	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.00%
43) trans-1,3-Dichloropropene-	7.85	79	46323	4.43	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.60%
46) 2-Hexanone-d5	8.31	63	226778	43.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.98%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	107932	5.08	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	101.60%
64) 1,2-Dichlorobenzene-d4	11.86	152	116001	5.80	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.00%


Target Compounds					Ovalue
13) Acetone	2.33	43	55363	11.916 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042419\
Data File : VU031486.D
Acq On : 24 Apr 2019 21:33
Operator : JC/SP
Sample : K2536-06
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X61

Quant Time: Apr 25 07:16:57 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 06:05:25 2019
Response via : Initial Calibration

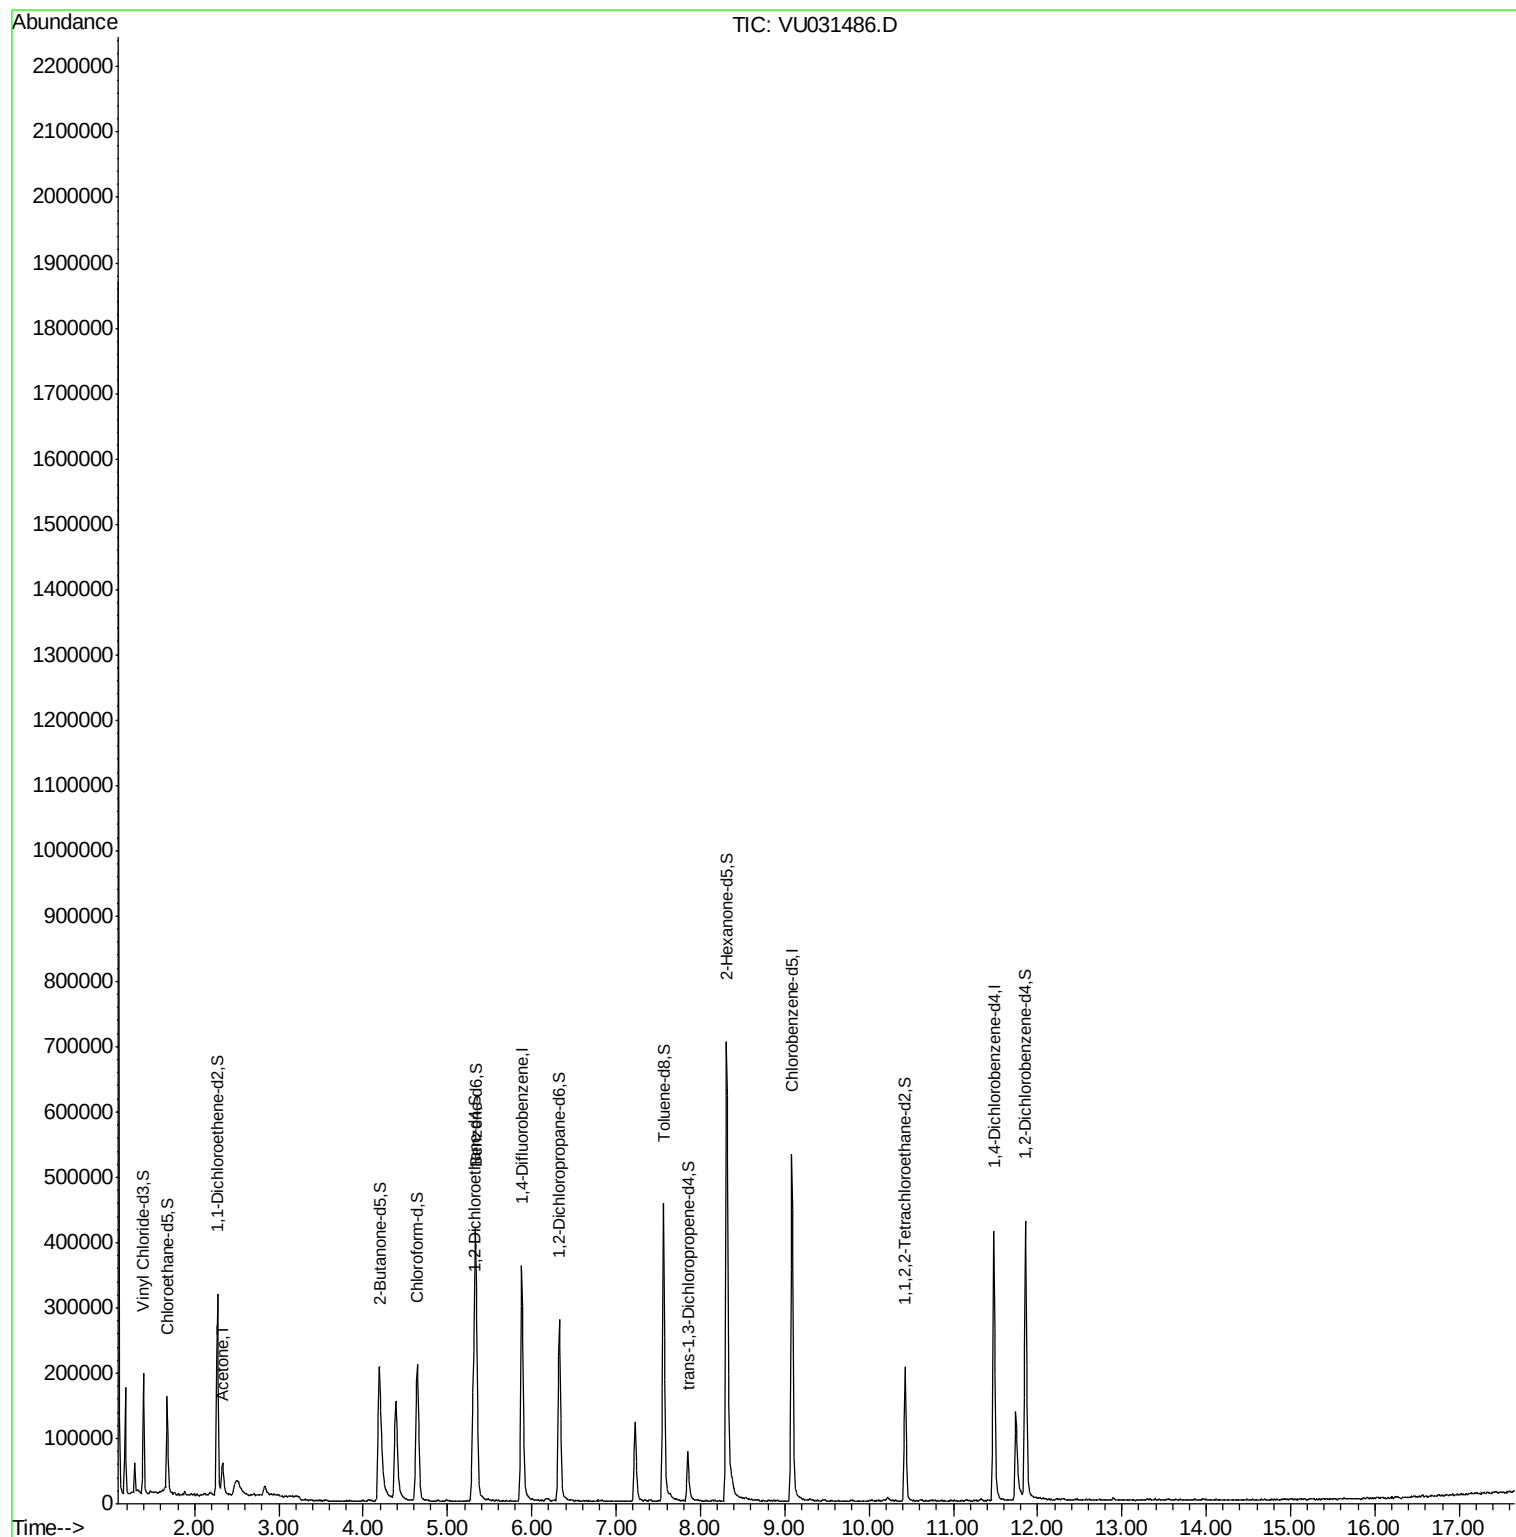

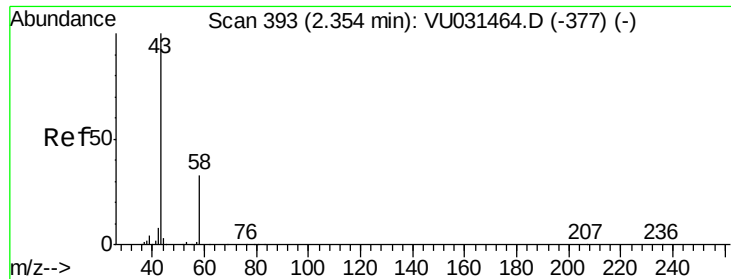

#13

Acetone

Concen: 11.916 ug/L

RT: 2.33 min Scan# 386

Delta R.T. -0.02 min

Lab File: VU031486.D

Acq: 24 Apr 2019 21:33

Instrument :

MSVOA_U

ClientSampleId :

C0X61

Tot Ion: 43 Resp: 55363

Ion Ratio Lower Upper

43 100

58 30.1 0.0 62.4

