


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042419\
 Data File : VU031457.D
 Acq On : 24 Apr 2019 08:33
 Operator : JC/SP
 Sample : BFB03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB03

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR042419WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Apr 25 06:05:25 2019

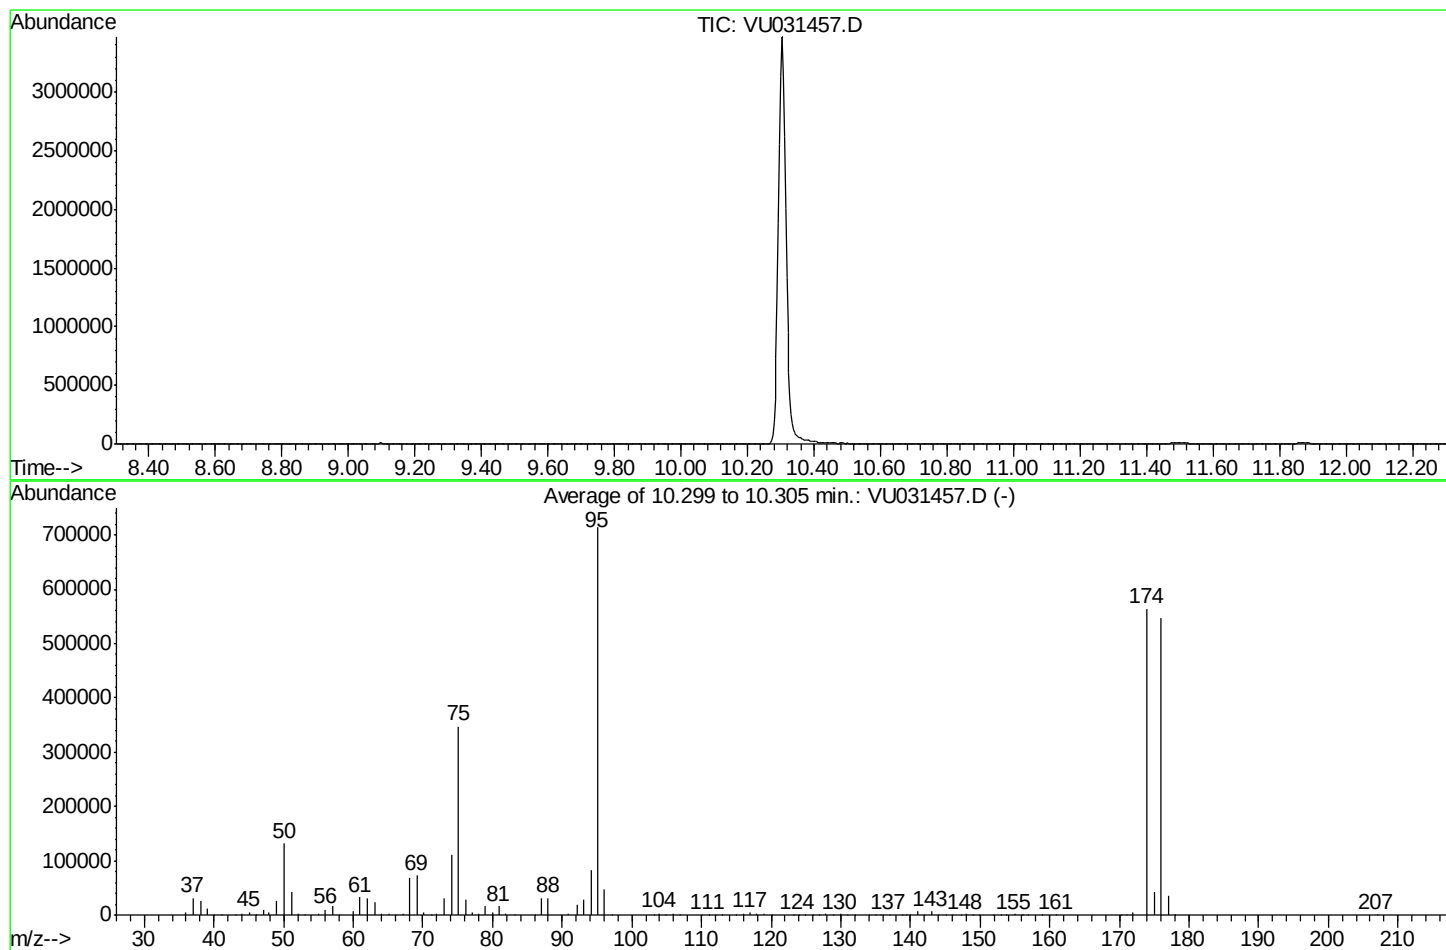

AutoFind: Scans 2864, 2865, 2866; Background Corrected with Scan 2850

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	130973	PASS
75	95	30	80	48.7	347562	PASS
95	95	100	100	100.0	714005	PASS
96	95	5	9	6.6	46853	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.1	564501	PASS
175	174	5	9	7.5	42501	PASS
176	174	95	101	96.7	546133	PASS
177	176	5	9	6.5	35381	PASS

Scan 2850 (10.254 min): VU031457.D
BFB03

m/z	Abundance
40.00	1525.0
44.00	1024.0
77.00	189.0
207.10	174.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	5151.0
37.00	30768.0
38.10	24752.0
39.10	10831.0
40.00	1948.0
41.20	101.0
43.00	301.0
44.00	3572.0
45.00	5522.0
46.00	534.0
47.10	8432.0
47.90	3769.0
49.00	25976.0
50.10	125656.0
51.10	39392.0
52.00	1504.0
53.00	327.0
55.00	1585.0
56.00	8995.0
57.10	16600.0
58.00	987.0
60.00	5945.0
61.00	31680.0
62.10	29752.0
63.10	22480.0
64.10	2707.0
65.00	2841.0
66.00	440.0
67.10	1566.0
68.00	63392.0
69.10	67952.0
70.10	5061.0
71.20	279.0
72.00	3014.0
73.00	29752.0
74.10	105408.0
75.10	326784.0
76.10	27656.0
77.10	3689.0
78.00	3003.0
78.90	14580.0
80.00	4494.0
81.00	15431.0
81.90	3151.0
83.20	105.0
87.00	28912.0
88.00	29192.0
90.90	1999.0
92.10	17728.0
93.10	27120.0
94.10	76872.0
95.10	669568.0
96.10	44648.0
97.00	1219.0
103.10	263.0
104.00	2866.0
104.90	697.0
106.00	2543.0
106.80	465.0
109.90	264.0
111.00	489.0
112.00	352.0
113.00	363.0
115.00	665.0
116.00	2064.0
117.00	3692.0
117.90	2023.0
119.00	3205.0
120.00	125.0
123.20	199.0
123.90	267.0
125.00	155.0
126.00	140.0
126.90	126.0
127.90	1988.0
128.90	824.0
130.00	2094.0
130.90	806.0
132.10	187.0
134.10	130.0
135.00	808.0
135.80	111.0
136.20	159.0
136.90	1023.0
138.90	282.0
140.00	371.0
141.00	6175.0
141.90	871.0
143.00	7066.0
144.00	686.0
145.00	1108.0
146.00	826.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

147.20	480.0
147.90	1465.0
149.00	325.0
149.90	592.0
151.90	383.0
153.00	411.0
153.80	233.0
155.00	1673.0
156.20	150.0
156.90	895.0
158.90	635.0
160.90	697.0
170.90	547.0
171.90	3897.0
174.00	516480.0
175.00	38736.0
176.00	496768.0
177.00	33328.0
178.00	1051.0
206.90	274.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	5697.0
37.00	32256.0
38.10	28280.0
39.10	11478.0
40.00	2096.0
43.00	309.0
44.00	3835.0
45.10	5860.0
46.00	562.0
47.10	8898.0
47.90	4219.0
49.10	27640.0
50.10	135552.0
51.10	42864.0
52.00	1726.0
53.00	319.0
55.00	1782.0
56.00	10025.0
57.00	17712.0
58.00	1005.0
60.00	6695.0
61.00	33416.0
62.10	32616.0
63.10	23960.0
64.10	2830.0
65.10	2785.0
66.00	420.0
67.20	1629.0
68.00	70976.0
69.10	76080.0
70.10	5191.0
71.10	322.0
72.00	3313.0
73.00	31432.0
74.10	115056.0
75.10	359232.0
76.10	29296.0
77.10	4150.0
78.00	3415.0
78.90	16275.0
80.00	4782.0
80.90	16363.0
81.90	3449.0
83.10	189.0
86.00	860.0
87.00	31264.0
88.00	32904.0
91.00	2224.0
92.10	19440.0
93.10	30064.0
94.10	85032.0
95.10	736640.0
96.10	48184.0
97.00	1190.0
103.10	303.0
104.00	3089.0
104.90	765.0
106.00	2760.0
106.90	521.0
109.90	285.0
111.00	550.0
112.00	351.0
112.90	405.0
115.00	873.0
116.00	2376.0
117.00	4172.0
117.90	2093.0
119.00	3593.0
120.00	163.0
123.20	190.0
123.90	345.0
125.00	214.0
126.00	153.0
126.80	168.0
127.90	2211.0
128.90	1131.0
130.00	2316.0
130.90	690.0
132.10	188.0
135.00	1000.0
135.70	144.0
136.20	137.0
137.00	1107.0
138.90	234.0
139.30	252.0
140.00	487.0
141.00	6607.0
141.90	1066.0
143.00	7113.0
144.00	618.0
145.00	1113.0
146.00	920.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

147.20	489.0
148.00	1595.0
149.00	409.0
149.90	676.0
151.90	392.0
153.00	519.0
153.80	244.0
155.00	1931.0
156.20	175.0
156.90	1163.0
158.90	611.0
160.90	851.0
170.40	178.0
170.90	565.0
172.00	3893.0
174.00	582656.0
175.00	43936.0
176.00	564288.0
177.00	36456.0
178.00	1102.0
207.00	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

m/z	Abundance
36.00	6015.0
37.00	30856.0
38.10	28552.0
39.10	10955.0
40.00	2193.0
41.10	113.0
43.00	309.0
44.00	4184.0
45.10	5800.0
45.90	562.0
47.10	8984.0
47.90	4378.0
49.10	27016.0
50.10	131712.0
51.10	42160.0
52.00	1832.0
53.10	269.0
55.00	1846.0
56.00	9613.0
57.00	16936.0
58.00	807.0
60.00	6522.0
61.00	32000.0
62.10	32272.0
63.10	23672.0
64.10	2731.0
65.10	2341.0
66.10	318.0
67.10	1586.0
68.00	71432.0
69.10	74480.0
70.00	4677.0
71.10	314.0
72.00	3407.0
73.00	30680.0
74.10	113352.0
75.10	356672.0
76.10	28968.0
77.10	4237.0
78.00	3346.0
79.00	16664.0
80.00	4533.0
81.00	16240.0
81.90	3498.0
83.00	237.0
86.00	1003.0
87.00	30808.0
88.00	32144.0
91.00	2145.0
92.10	18960.0
93.10	30024.0
94.10	85304.0
95.10	735808.0
96.10	47728.0
97.10	1079.0
103.10	339.0
104.00	2797.0
104.90	765.0
106.00	2714.0
106.90	469.0
110.00	238.0
111.00	544.0
112.00	245.0
112.90	420.0
115.00	999.0
116.00	2379.0
117.00	4052.0
118.00	2179.0
118.90	3460.0
120.00	160.0
123.20	122.0
123.90	431.0
124.90	227.0
126.00	132.0
126.80	173.0
127.90	2097.0
128.90	1190.0
130.00	2386.0
130.90	665.0
132.00	132.0
135.00	1034.0
135.80	115.0
136.10	156.0
137.00	1120.0
138.70	202.0
139.30	266.0
140.00	544.0
141.00	6310.0
141.90	1055.0
143.00	6251.0
144.00	420.0
145.00	1036.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03

146.00	862.0
147.20	380.0
148.00	1635.0
149.00	394.0
149.90	716.0
152.00	332.0
153.00	488.0
153.80	270.0
155.00	1813.0
155.90	228.0
156.90	1327.0
159.00	576.0
160.90	837.0
170.30	235.0
171.00	517.0
172.00	3339.0
174.00	594368.0
175.00	44832.0
176.00	577344.0
177.00	36360.0
178.00	986.0
207.20	156.0

Instrument :
MSVOA_U
ClientSampleId :
BFB03