

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037869.D
 Acq On : 24 Apr 2020 14:31
 Operator : JC/MD
 Sample : L2395-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Manual Integrations
 APPROVED

MMDadoda
 4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 25 01:13:34 2020
 Response via : Initial Calibration

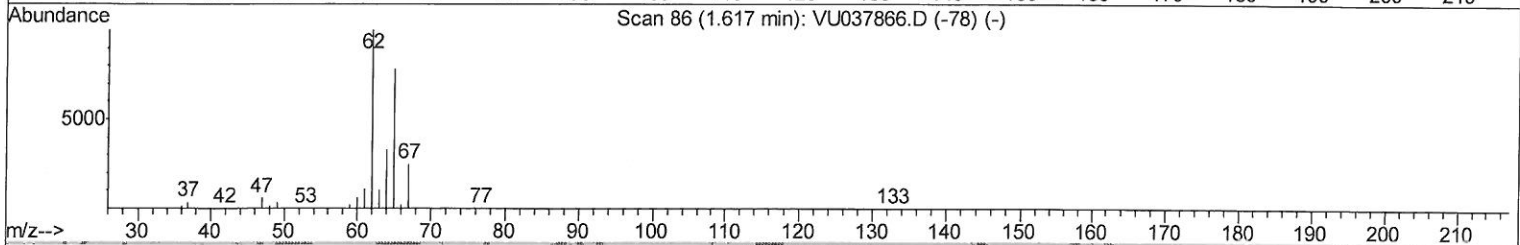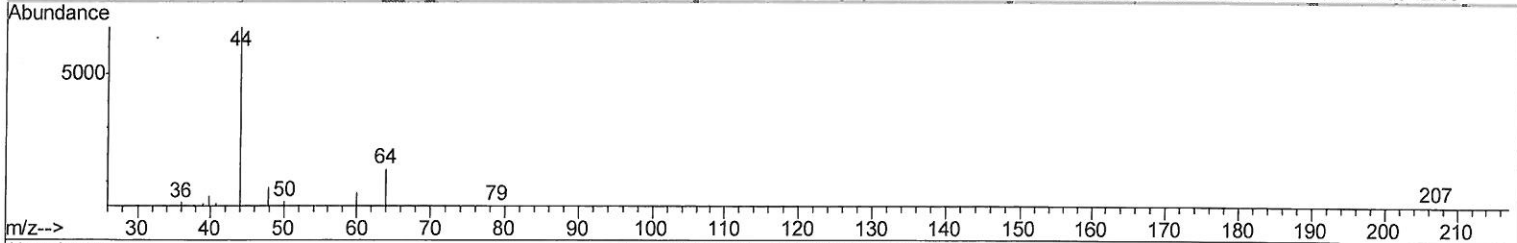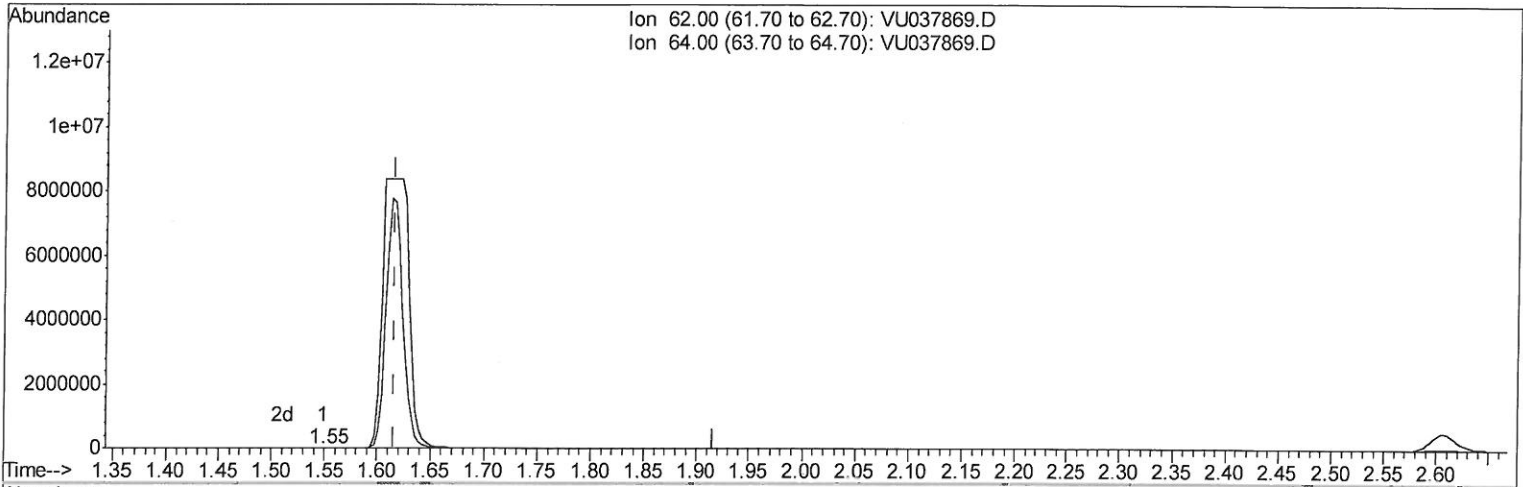

TIC: VU037869.D

(5) Vinyl chloride (T)

1.549min (-0.067) 0.02ug/L

response 75

Ion	Exp%	Act%
62.00	100	100
64.00	33.10	997.96#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037869.D
 Acq On : 24 Apr 2020 14:31
 Operator : JC/MD
 Sample : L2395-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0D86

Manual Integrations
APPROVED

MMDadoda
 4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 25 01:13:34 2020
 Response via : Initial Calibration

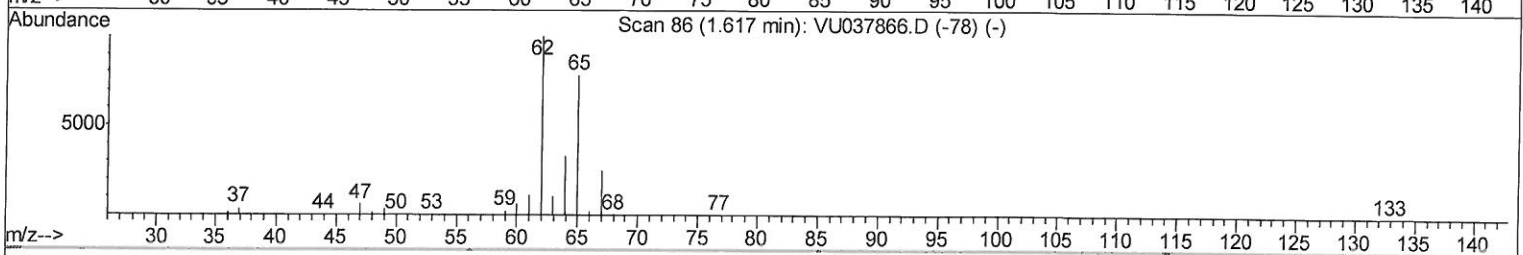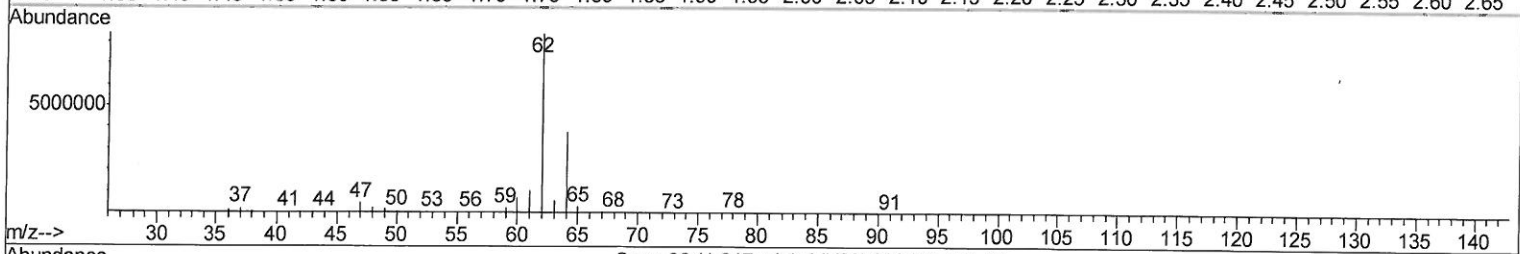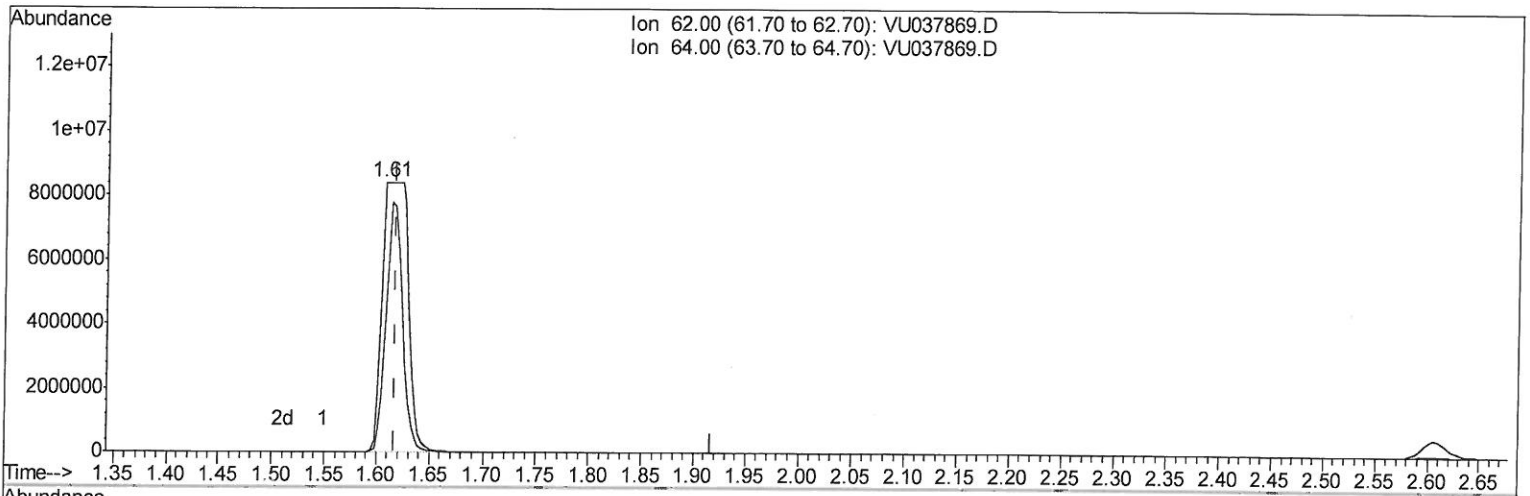

TIC: VU037869.D

(5) Vinyl chloride (T)

1.607min (-0.010) 3892.28ug/L m

response 14398187

Ion	Exp%	Act%
62.00	100	100
64.00	33.10	45.22#
0.00	0.00	0.00
0.00	0.00	0.00

04/27/2020

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037869.D
 Acq On : 24 Apr 2020 14:31
 Operator : JC/MD
 Sample : L2395-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
ClientSampleId :
 C0D86

Manual Integrations
APPROVED

MMDadoda
 4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 25 01:13:34 2020
 Response via : Initial Calibration

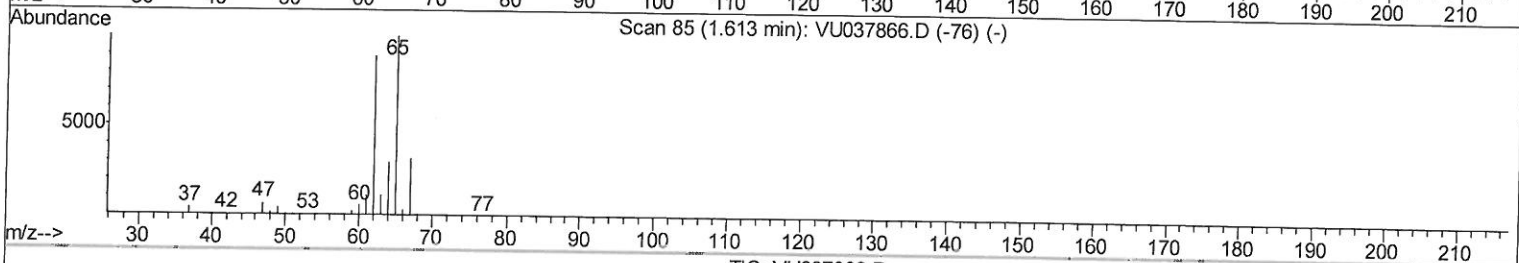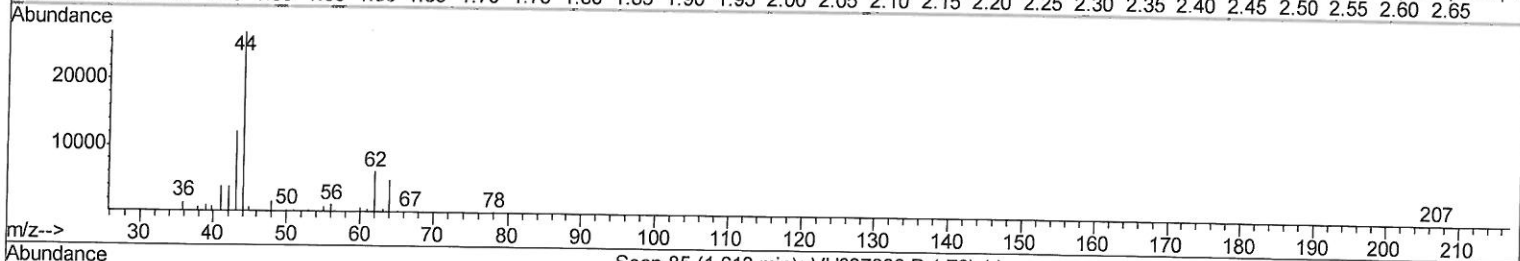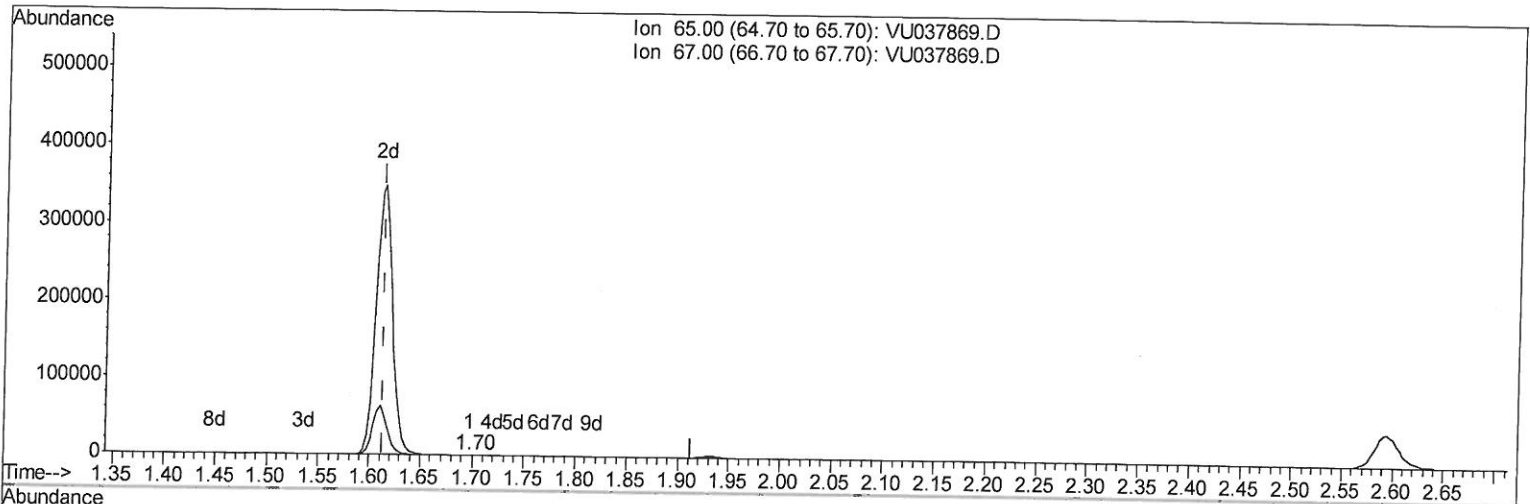

TIC: VU037869.D

(4) Vinyl Chloride-d3 (S)
 1.697min (+0.084) 0.07ug/L
 response 227

Ion	Exp%	Act%
65.00	100	100
67.00	31.60	35.24
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037869.D
Acq On : 24 Apr 2020 14:31
Operator : JC/MD
Sample : L2395-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

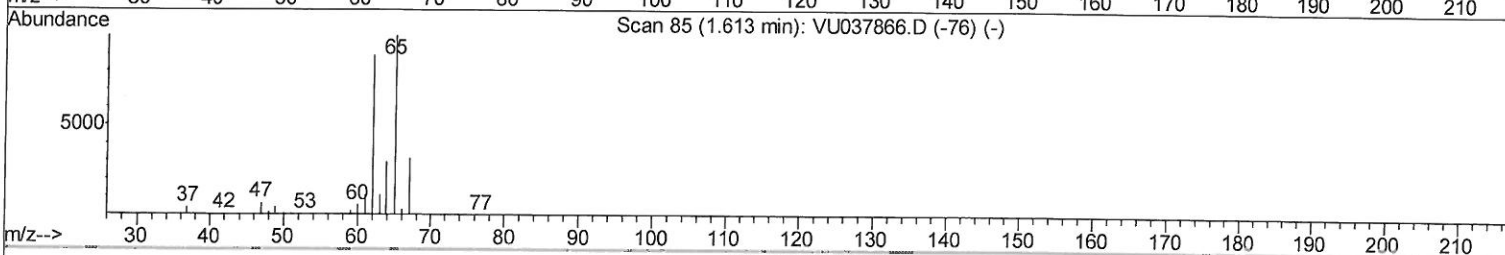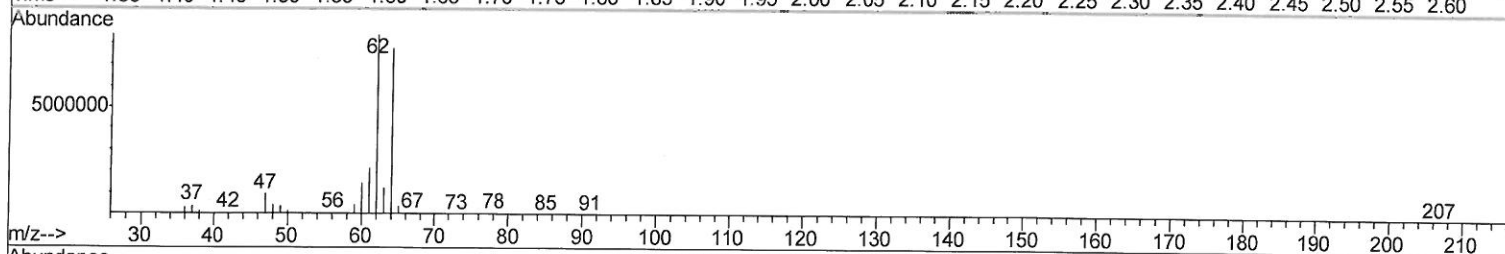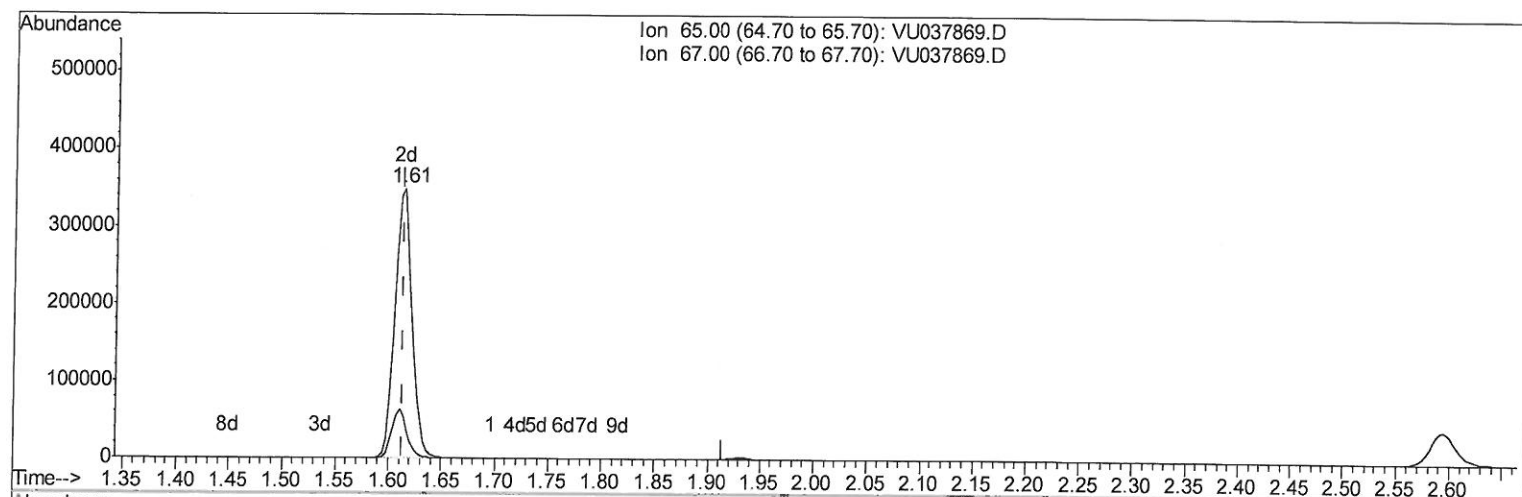

TIC: VU037869.D

(4) Vinyl Chloride-d3 (S)

1.613min (+0.000) 118.88ug/L m

response 387289

Ion	Exp%	Act%
65.00	100	100
67.00	31.60	0.02#
0.00	0.00	0.00
0.00	0.00	0.00

204/27/2059

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037869.D
Acq On : 24 Apr 2020 14:31
Operator : JC/MD
Sample : L2395-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

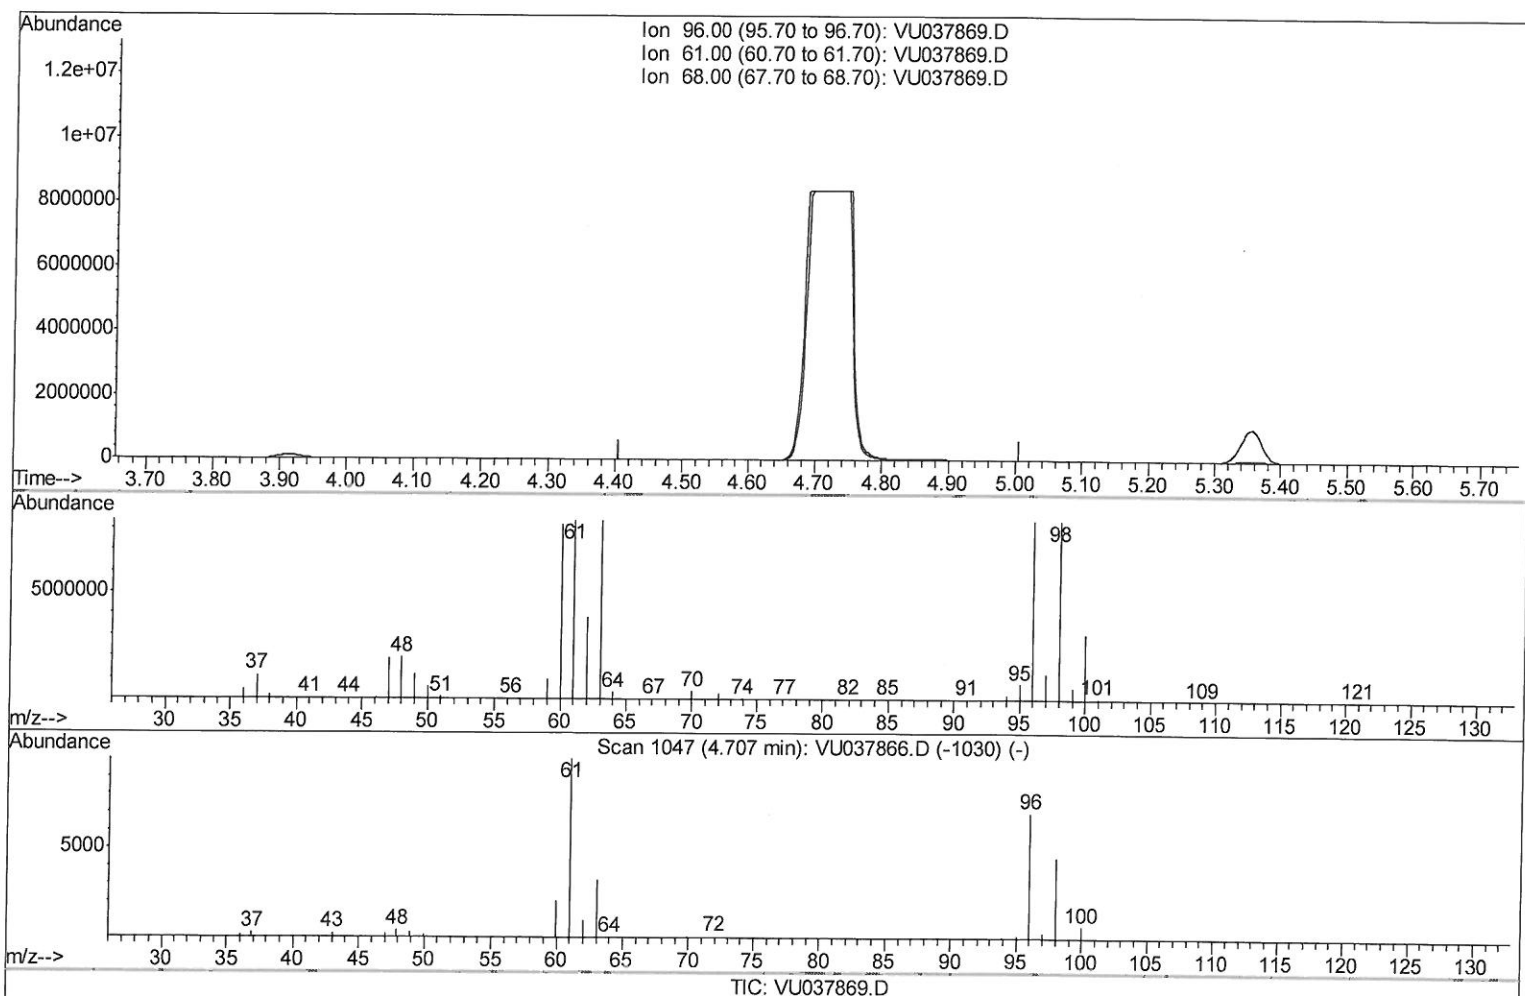

(20) cis-1,2-Dichloroethene (T)

4.707min (-4.707) 0.00ug/L

response 0

Ion	Exp%	Act%
96.00	100	0.00
61.00	143.40	0.00#
68.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037869.D
Acq On : 24 Apr 2020 14:31
Operator : JC/MD
Sample : L2395-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:15:34 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

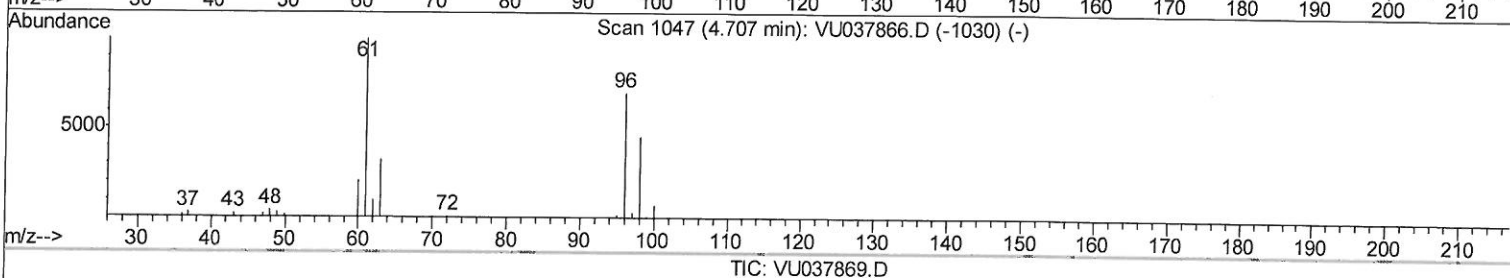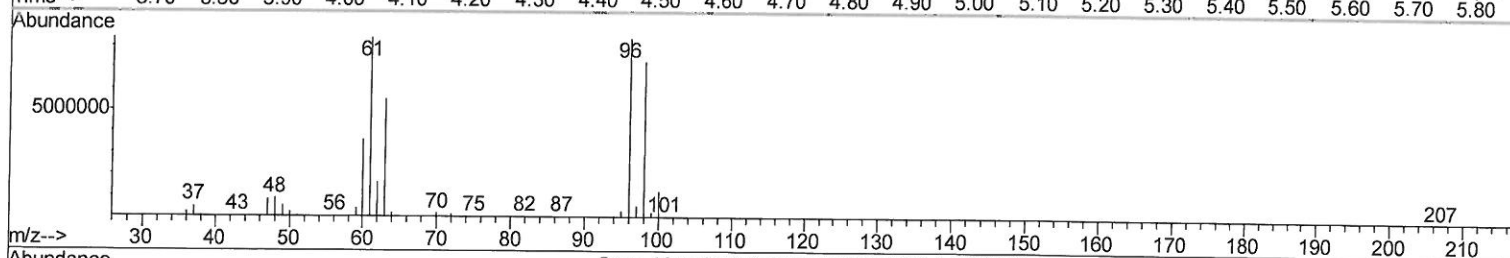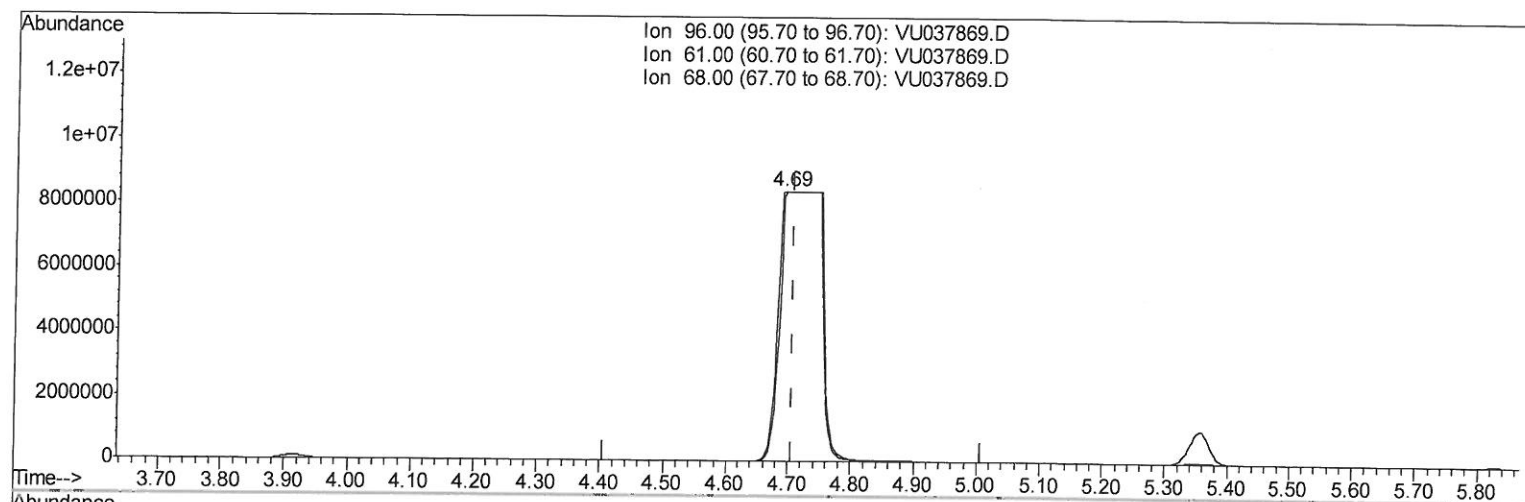

TIC: VU037869.D

(20) cis-1,2-Dichloroethene (T)

4.694min (-0.013) 13541.12ug/L m *>04/27/2020*
response 37525755

Ion	Exp%	Act%
96.00	100	100
61.00	143.40	100.00#
68.00	0.00	0.00#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037869.D
 Acq On : 24 Apr 2020 14:31
 Operator : JC/MD
 Sample : L2395-01
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Manual Integrations
 APPROVED

MMDadoda
 4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:44:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 25 01:13:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	372858	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	366545	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	151968	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	387289m	118.88	ug/L	0.00	04/27/2020
Spiked Amount 50.000	Range 60 - 135		Recovery =	237.76%	#		
7) Chloroethane-d5	1.93	69	144044	57.05	ug/L	0.00	
Spiked Amount 50.000	Range 70 - 130		Recovery =	114.10%			
11) 1,1-Dichloroethene-d2	2.61	63	4129213	783.06	ug/L	0.01	
Spiked Amount 50.000	Range 60 - 125		Recovery =	1566.12%	#		
21) 2-Butanone-d5	4.80	46	142	0.06	ug/L	0.14	
Spiked Amount 100.000	Range 40 - 130		Recovery =	0.06%	#		
24) Chloroform-d	5.11	84	287232	57.88	ug/L	0.00	
Spiked Amount 50.000	Range 70 - 125		Recovery =	115.76%			
26) 1,2-Dichloroethane-d4	5.74	65	202964	59.07	ug/L	0.00	
Spiked Amount 50.000	Range 70 - 125		Recovery =	118.14%			
32) Benzene-d6	5.76	84	616730	59.50	ug/L	0.00	
Spiked Amount 50.000	Range 70 - 125		Recovery =	119.00%			
36) 1,2-Dichloropropane-d6	6.72	67	208205	60.05	ug/L	0.00	
Spiked Amount 50.000	Range 70 - 120		Recovery =	120.10%	#		
41) Toluene-d8	7.92	98	573158	60.16	ug/L	0.00	
Spiked Amount 50.000	Range 80 - 120		Recovery =	120.32%	#		
43) trans-1,3-Dichloropropene-	8.20	79	110722	62.05	ug/L	0.00	
Spiked Amount 50.000	Range 60 - 125		Recovery =	124.10%			
47) 2-Hexanone-d5	8.65	63	229552	121.63	ug/L	0.00	
Spiked Amount 100.000	Range 45 - 130		Recovery =	121.63%			
57) 1,1,2,2-Tetrachloroethane-	10.77	84	224271	46.49	ug/L	0.00	
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.98%			
64) 1,2-Dichlorobenzene-d4	12.20	152	169346	57.27	ug/L	0.00	
Spiked Amount 50.000	Range 80 - 120		Recovery =	114.54%			

Target Compounds

						Ovalue
5) Vinyl chloride	1.61	62	14398187m	3892.276	ug/L	
10) 1,1,2-Trichloro-1,2,2-trif	2.61	101	16662	7.270	ug/L #	31
12) 1,1-Dichloroethene	2.61	96	6643596	2934.886	ug/L #	68
13) Acetone	2.66	43	37148	24.121	ug/L	94
15) Methyl Acetate	2.98	43	3203	0.860	ug/L #	75
16) Methylene chloride	3.08	84	11135	4.140	ug/L	85
17) trans-1,2-Dichloroethene	3.39	96	809847	319.966	ug/L	97
19) 1,1-Dichloroethane	3.92	63	3887543	761.962	ug/L	100
20) cis-1,2-Dichloroethene	4.69	96	37525755m	13541.119	ug/L	
27) 1,2-Dichloroethane	5.83	62	110436	27.010	ug/L	100
30) 1,1,1-Trichloroethane	5.36	97	4718166	1152.599	ug/L	99
33) Benzene	5.81	78	29511	2.653	ug/L	100
34) Trichloroethene	6.57	95	534495	195.862	ug/L	99
40) 4-Methyl-2-pentanone	7.82	43	24624	4.660	ug/L	99
42) Toluene	7.99	91	351797	30.160	ug/L	99
45) 1,1,2-Trichloroethane	8.42	97	207003	78.092	ug/L	99
52) Ethylbenzene	9.59	91	642453	49.183	ug/L	99

04/27/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037869.D
Acq On : 24 Apr 2020 14:31
Operator : JC/MD
Sample : L2395-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:44:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
53) m,p-Xylene	9.71	106	1095764	222.801	ug/L	100
54) o-xylene	10.12	106	602356	125.231	ug/L	97
56) Isopropylbenzene	10.50	105	20466	1.608	ug/L	98
59) 1,2,3-Trichloropropane	10.84	75	7085	1.736	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037869.D
Acq On : 24 Apr 2020 14:31
Operator : JC/MD
Sample : L2395-01
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:01:57 PM

Quant Time: Apr 25 01:44:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

