




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037881.D
Acq On : 24 Apr 2020 19:04
Operator : JC/MD
Sample : L2395-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:02:34 PM

Quant Time: Apr 25 01:17:31 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

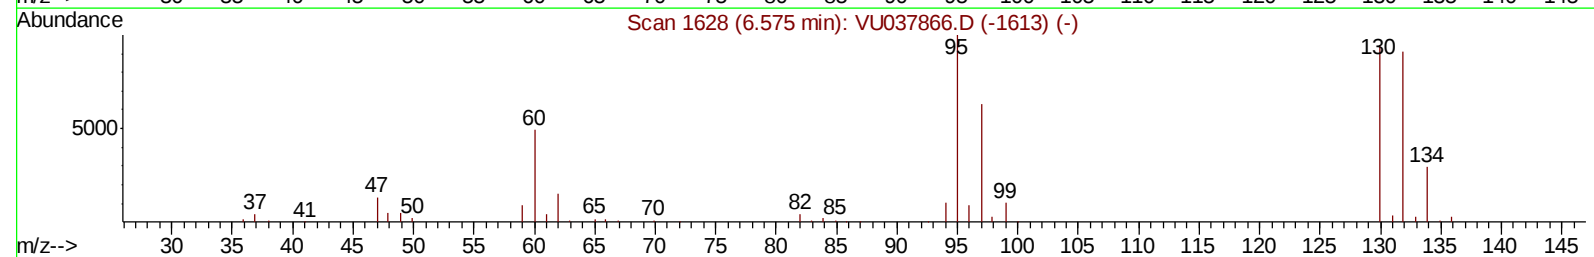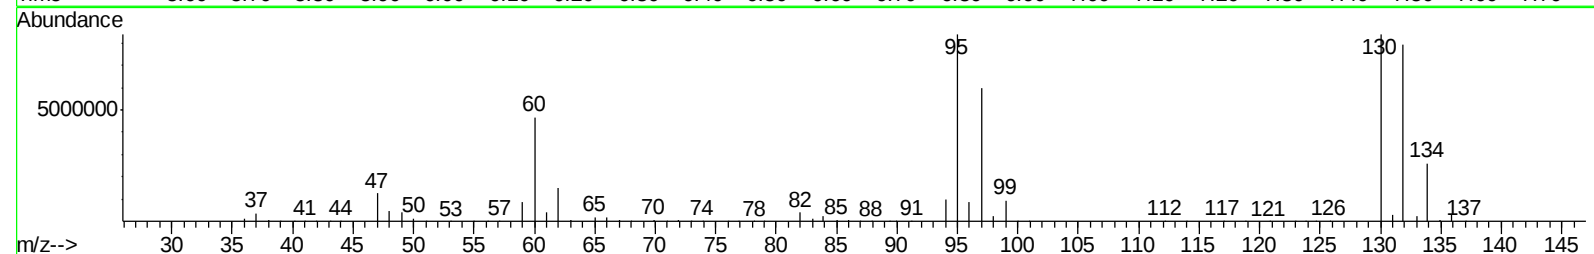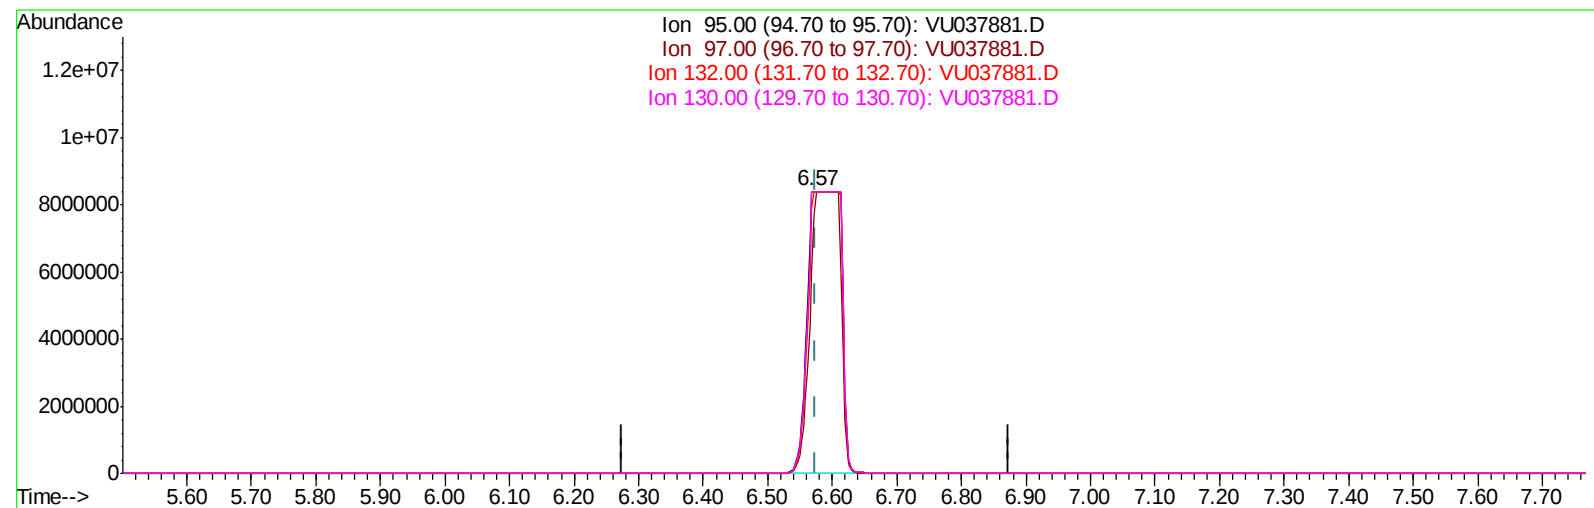

TIC: VU037881.D

(34) Trichloroethene (T)

6.568min (-0.006) 6624.81ug/L m

response 30174643

Ion	Exp%	Act%
95.00	100	100
97.00	63.50	71.22
132.00	92.80	94.25
130.00	93.60	100.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037881.D
 Acq On : 24 Apr 2020 19:04
 Operator : JC/MD
 Sample : L2395-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA0

Manual Integrations
 APPROVED

MMDadoda
 4/28/2020 12:02:34 PM

Quant Time: Apr 25 04:19:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Apr 25 01:13:34 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	619921	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	611790	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	210544	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	244151	45.07	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.14%
7) Chloroethane-d5	1.93	69	197958	47.16	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.32%
11) 1,1-Dichloroethene-d2	2.60	63	2174624	248.04	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	496.08%#
21) 2-Butanone-d5	4.66	46	498595	116.17	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	116.17%
24) Chloroform-d	5.10	84	384553	46.61	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.22%
26) 1,2-Dichloroethane-d4	5.74	65	268330	46.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.94%
32) Benzene-d6	5.76	84	824400	47.65	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.30%
36) 1,2-Dichloropropane-d6	6.73	67	279295	48.27	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	96.54%
41) Toluene-d8	7.92	98	761886	47.91	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.82%
43) trans-1,3-Dichloropropene-	8.20	79	139556	46.86	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	93.72%
47) 2-Hexanone-d5	8.65	63	378978	120.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	120.31%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	296200	36.79	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	73.58%
64) 1,2-Dichlorobenzene-d4	12.20	152	278917	68.08	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	136.16%#

Target Compounds

					Ovalue
5) Vinyl chloride	1.62	62	11315	1.840	ug/L # 35
12) 1,1-Dichloroethene	2.60	96	3184063	846.012	ug/L # 71
13) Acetone	2.66	43	11219	4.381	ug/L 100
16) Methylene chloride	3.08	84	1156457	258.591	ug/L 98
17) trans-1,2-Dichloroethene	3.39	96	4746	1.128	ug/L 99
19) 1,1-Dichloroethane	3.91	63	140410	16.552	ug/L 100
20) cis-1,2-Dichloroethene	4.71	96	1182403	256.624	ug/L 100
27) 1,2-Dichloroethane	5.83	62	14439	2.124	ug/L 97
30) 1,1,1-Trichloroethane	5.36	97	5238005	766.647	ug/L 99
34) Trichloroethene	6.57	95	30174643m	6624.815	ug/L
42) Toluene	7.99	91	47363	2.433	ug/L 100
45) 1,1,2-Trichloroethane	8.42	97	55603	12.568	ug/L 97
46) Tetrachloroethene	8.57	164	6561	1.971	ug/L 96
52) Ethylbenzene	9.59	91	53260	2.443	ug/L 99
54) o-xylene	10.11	106	86809	10.813	ug/L 96

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037881.D
Acq On : 24 Apr 2020 19:04
Operator : JC/MD
Sample : L2395-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:02:34 PM

Quant Time: Apr 25 04:19:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037881.D
Acq On : 24 Apr 2020 19:04
Operator : JC/MD
Sample : L2395-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:02:34 PM

Quant Time: Apr 25 04:19:25 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

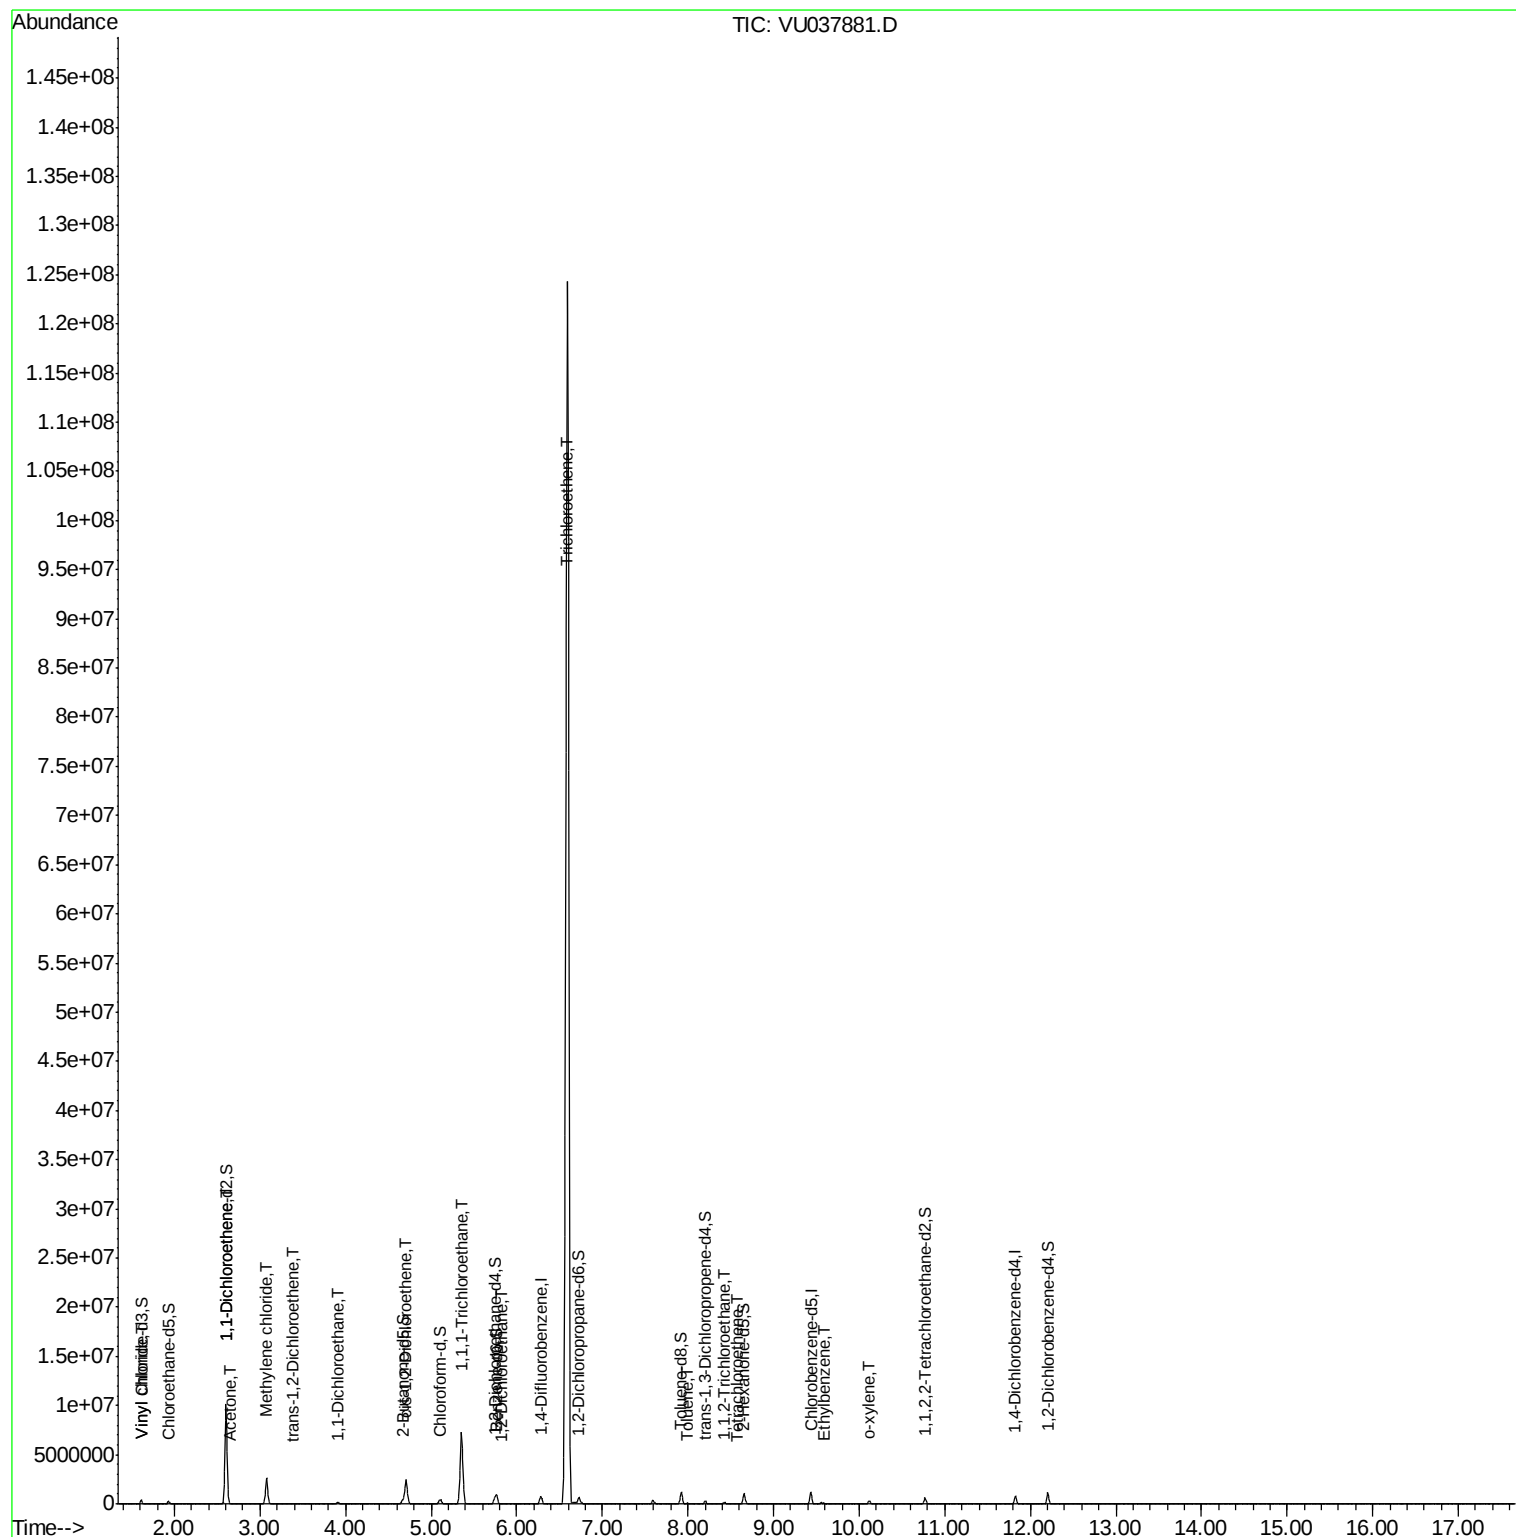




Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037881.D
Acq On : 24 Apr 2020 19:04
Operator : JC/MD
Sample : L2395-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0

Manual Integrations
APPROVED

MMDadoda
4/28/2020 12:02:34 PM

Quant Time: Apr 25 01:17:31 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Apr 25 01:13:34 2020
Response via : Initial Calibration

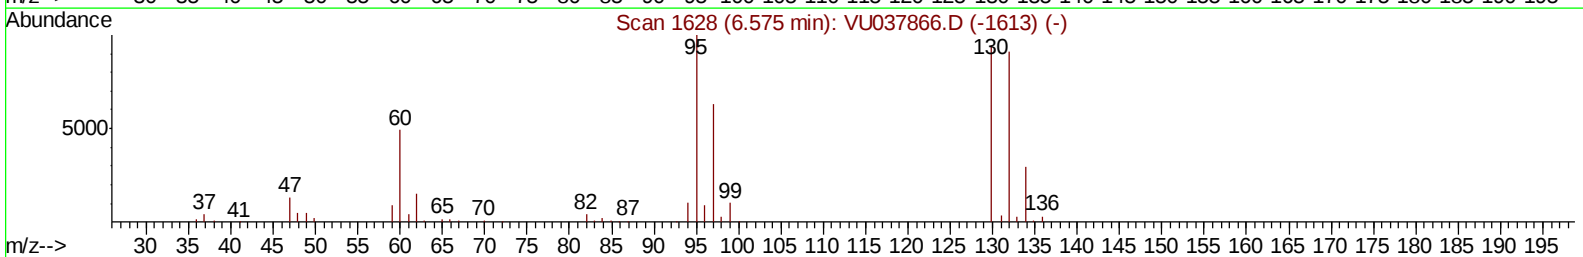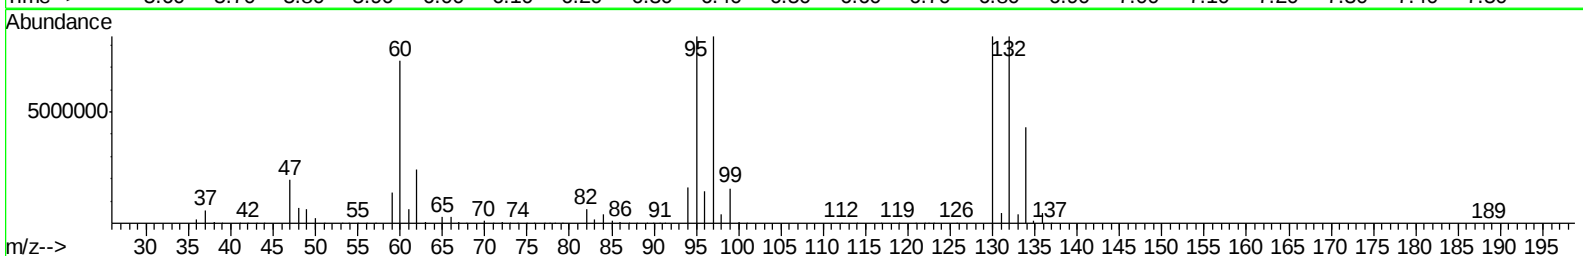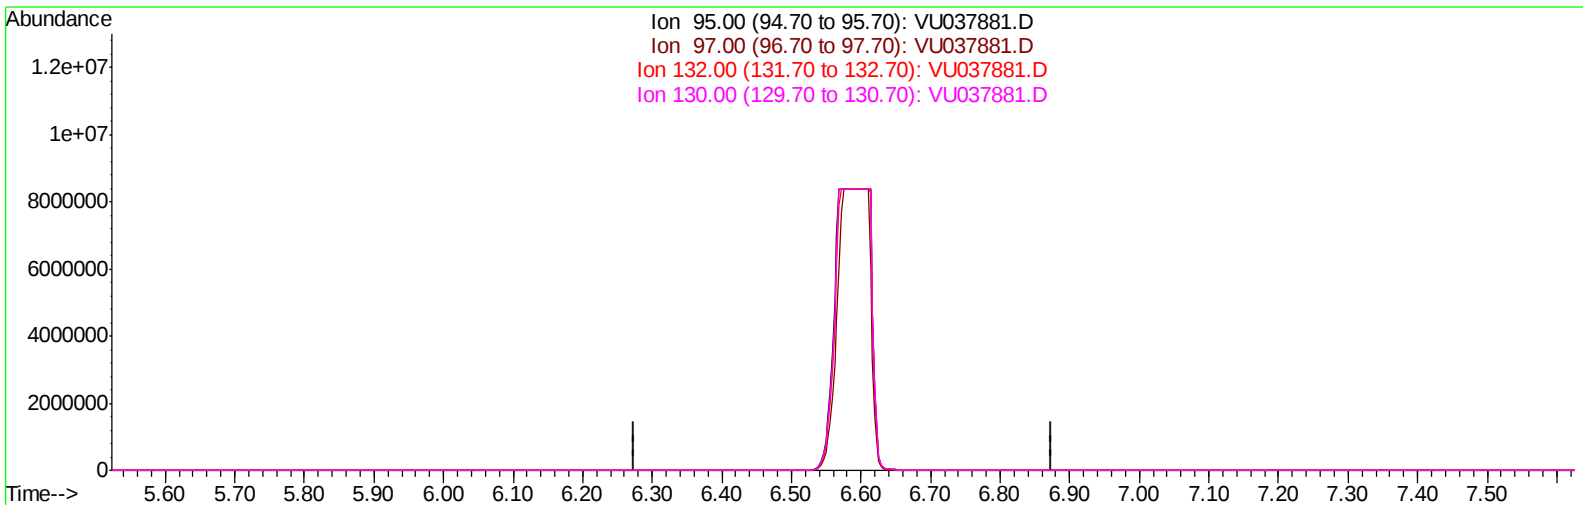

TIC: VU037881.D

(34) Trichloroethene (T)

6.575min (-6.575) 0.00ug/L

response 0

Ion	Exp%	Act%
95.00	100	0.00
97.00	63.50	0.00#
132.00	92.80	0.00#
130.00	93.60	0.00#