

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037871.D
 Acq On : 24 Apr 2020 15:17
 Operator : JC/MD
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	98	rVB	352430	375268	15.97%	1.933%
2	1.932	175	184	194	rVB	252060	330580	14.06%	1.702%
3	2.523	365	368	371	rBV3	1010	720	0.03%	0.004%
4	2.591	376	389	411	rVV	463429	767091	32.64%	3.950%
5	2.777	444	447	449	rBV	995	718	0.03%	0.004%
6	2.900	481	485	491	rVB6	486	588	0.03%	0.003%
7	2.945	495	499	502	rBV4	724	580	0.02%	0.003%
8	3.076	534	540	546	rBV5	1313	2072	0.09%	0.011%
9	3.215	573	583	598	rVB3	8139	18152	0.77%	0.093%
10	3.273	598	601	606	rVB2	644	493	0.02%	0.003%
11	3.379	627	634	636	rBV3	1820	1784	0.08%	0.009%
12	3.527	677	680	685	rVB3	493	386	0.02%	0.002%
13	3.572	690	694	697	rVB	543	465	0.02%	0.002%
14	3.736	739	745	747	rBV	793	467	0.02%	0.002%
15	3.826	766	773	775	rBV3	468	528	0.02%	0.003%
16	3.890	790	793	798	rBV3	512	540	0.02%	0.003%
17	3.954	811	813	816	rVB2	790	387	0.02%	0.002%
18	3.977	818	820	826	rVB4	418	357	0.02%	0.002%
19	4.137	868	870	876	rBV2	632	437	0.02%	0.002%
20	4.263	904	909	910	rBV2	484	425	0.02%	0.002%
21	4.272	910	912	915	rVV2	660	347	0.01%	0.002%
22	4.292	916	918	922	rVV2	588	393	0.02%	0.002%
23	4.311	922	924	928	rVV	570	388	0.02%	0.002%
24	4.346	931	935	940	rBV3	363	480	0.02%	0.002%
25	4.565	998	1003	1008	rBV3	570	574	0.02%	0.003%
26	4.594	1008	1012	1015	rBV3	501	393	0.02%	0.002%
27	4.665	1017	1034	1044	rBV	273202	666249	28.35%	3.431%
28	4.896	1104	1106	1115	rVB2	523	476	0.02%	0.002%
29	4.935	1115	1118	1123	rBV5	535	438	0.02%	0.002%
30	5.102	1153	1170	1193	rBV	405731	882410	37.54%	4.544%
31	5.327	1237	1240	1241	rBV2	590	387	0.02%	0.002%
32	5.411	1261	1266	1273	rVB5	1438	1942	0.08%	0.010%
33	5.526	1298	1302	1306	rVV3	354	359	0.02%	0.002%
34	5.758	1351	1374	1394	rBV2	892940	2350440	100.00%	12.104%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037871.D
 Acq On : 24 Apr 2020 15:17
 Operator : JC/MD
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.279	1519	1536	1556	rBV	847983	1590998	67.69%	8.193%
36	6.401	1571	1574	1578	rVB2	1064	839	0.04%	0.004%
37	6.430	1578	1583	1589	rVB3	729	855	0.04%	0.004%
38	6.469	1590	1595	1599	rVB4	616	547	0.02%	0.003%
39	6.568	1614	1626	1638	rBV7	10070	21547	0.92%	0.111%
40	6.723	1658	1674	1694	rBV	566646	1096224	46.64%	5.645%
41	6.835	1707	1709	1715	rVB7	1913	1530	0.07%	0.008%
42	7.015	1763	1765	1769	rBV2	733	493	0.02%	0.003%
43	7.160	1808	1810	1814	rVV2	582	416	0.02%	0.002%
44	7.211	1816	1826	1832	rVB7	1785	3236	0.14%	0.017%
45	7.385	1876	1880	1883	rVB2	632	443	0.02%	0.002%
46	7.404	1883	1886	1889	rBV2	528	460	0.02%	0.002%
47	7.459	1896	1903	1908	rBV2	891	1020	0.04%	0.005%
48	7.591	1928	1944	1963	rBV	346835	600311	25.54%	3.091%
49	7.690	1971	1975	1976	rBV3	668	411	0.02%	0.002%
50	7.703	1976	1979	1981	rVV3	921	649	0.03%	0.003%
51	7.809	2006	2012	2013	rBV4	1344	1122	0.05%	0.006%
52	7.922	2030	2047	2064	rBV	1135485	1935579	82.35%	9.968%
53	8.105	2101	2104	2109	rVB5	774	585	0.02%	0.003%
54	8.202	2120	2134	2151	rBV	247031	415077	17.66%	2.138%
55	8.263	2151	2153	2159	rVB6	1434	1302	0.06%	0.007%
56	8.494	2215	2225	2231	rBV4	4334	7050	0.30%	0.036%
57	8.568	2246	2248	2249	rBV	863	438	0.02%	0.002%
58	8.655	2260	2275	2303	rBV	837982	1463903	62.28%	7.539%
59	8.812	2321	2324	2330	rVB5	588	596	0.03%	0.003%
60	8.935	2355	2362	2376	rBV5	2270	3924	0.17%	0.020%
61	9.012	2381	2386	2390	rVB4	499	460	0.02%	0.002%
62	9.124	2417	2421	2424	rBV2	599	496	0.02%	0.003%
63	9.153	2427	2430	2433	rBV2	668	375	0.02%	0.002%
64	9.176	2433	2437	2439	rBV2	462	354	0.02%	0.002%
65	9.224	2447	2452	2455	rBV3	506	533	0.02%	0.003%
66	9.247	2456	2459	2464	rVB2	356	347	0.01%	0.002%
67	9.436	2503	2518	2534	rBV	1216356	1980625	84.27%	10.200%
68	9.591	2561	2566	2569	rVV2	1358	1156	0.05%	0.006%
69	9.713	2594	2604	2615	rBV2	4285	6640	0.28%	0.034%
70	9.790	2624	2628	2630	rBV2	706	469	0.02%	0.002%
71	9.861	2645	2650	2654	rBV4	369	353	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037871.D
 Acq On : 24 Apr 2020 15:17
 Operator : JC/MD
 Sample : VIBLK40
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK40

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	9.919	2662	2668	2671	rBV2	333	394	0.02%	0.002%
73	10.121	2722	2731	2740	rVB7	2983	5199	0.22%	0.027%
74	10.311	2786	2790	2792	rBV2	476	367	0.02%	0.002%
75	10.359	2802	2805	2809	rBV3	565	522	0.02%	0.003%
76	10.501	2843	2849	2857	rVB5	1415	1945	0.08%	0.010%
77	10.584	2869	2875	2883	rVB3	1215	1721	0.07%	0.009%
78	10.771	2920	2933	2951	rBV	727225	1148115	48.85%	5.912%
79	10.902	2965	2974	2985	rVB4	4336	6711	0.29%	0.035%
80	11.124	3040	3043	3049	rVB3	1089	1086	0.05%	0.006%
81	11.153	3049	3052	3055	rBV3	645	370	0.02%	0.002%
82	11.738	3227	3234	3236	rBV3	1247	1235	0.05%	0.006%
83	11.758	3236	3240	3248	rVB3	2187	2318	0.10%	0.012%
84	11.825	3248	3261	3280	rBV	1233433	1970351	83.83%	10.147%
85	11.922	3288	3291	3296	rBV4	600	498	0.02%	0.003%
86	11.980	3307	3309	3317	rVB	746	632	0.03%	0.003%
87	12.015	3317	3320	3322	rBV2	582	396	0.02%	0.002%
88	12.076	3334	3339	3350	rVB6	1787	2588	0.11%	0.013%
89	12.150	3359	3362	3365	rBV	501	367	0.02%	0.002%
90	12.205	3365	3379	3397	rVV	1075703	1711988	72.84%	8.816%
91	12.889	3588	3592	3596	rBV3	542	505	0.02%	0.003%
92	12.960	3611	3614	3617	rVB	572	369	0.02%	0.002%
93	13.031	3634	3636	3640	rVB2	908	500	0.02%	0.003%
94	13.237	3694	3700	3710	rBV8	2585	3543	0.15%	0.018%
95	13.327	3725	3728	3732	rVV3	872	718	0.03%	0.004%
96	13.571	3800	3804	3806	rBV2	448	425	0.02%	0.002%
97	13.861	3889	3894	3899	rBV5	1976	2314	0.10%	0.012%
98	14.221	4002	4006	4008	rBV3	607	469	0.02%	0.002%
99	14.362	4042	4050	4057	rBV5	2390	3498	0.15%	0.018%
100	14.996	4244	4247	4250	rBV3	968	630	0.03%	0.003%


Sum of corrected areas: 19418451

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037871.D
Acq On : 24 Apr 2020 15:17
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

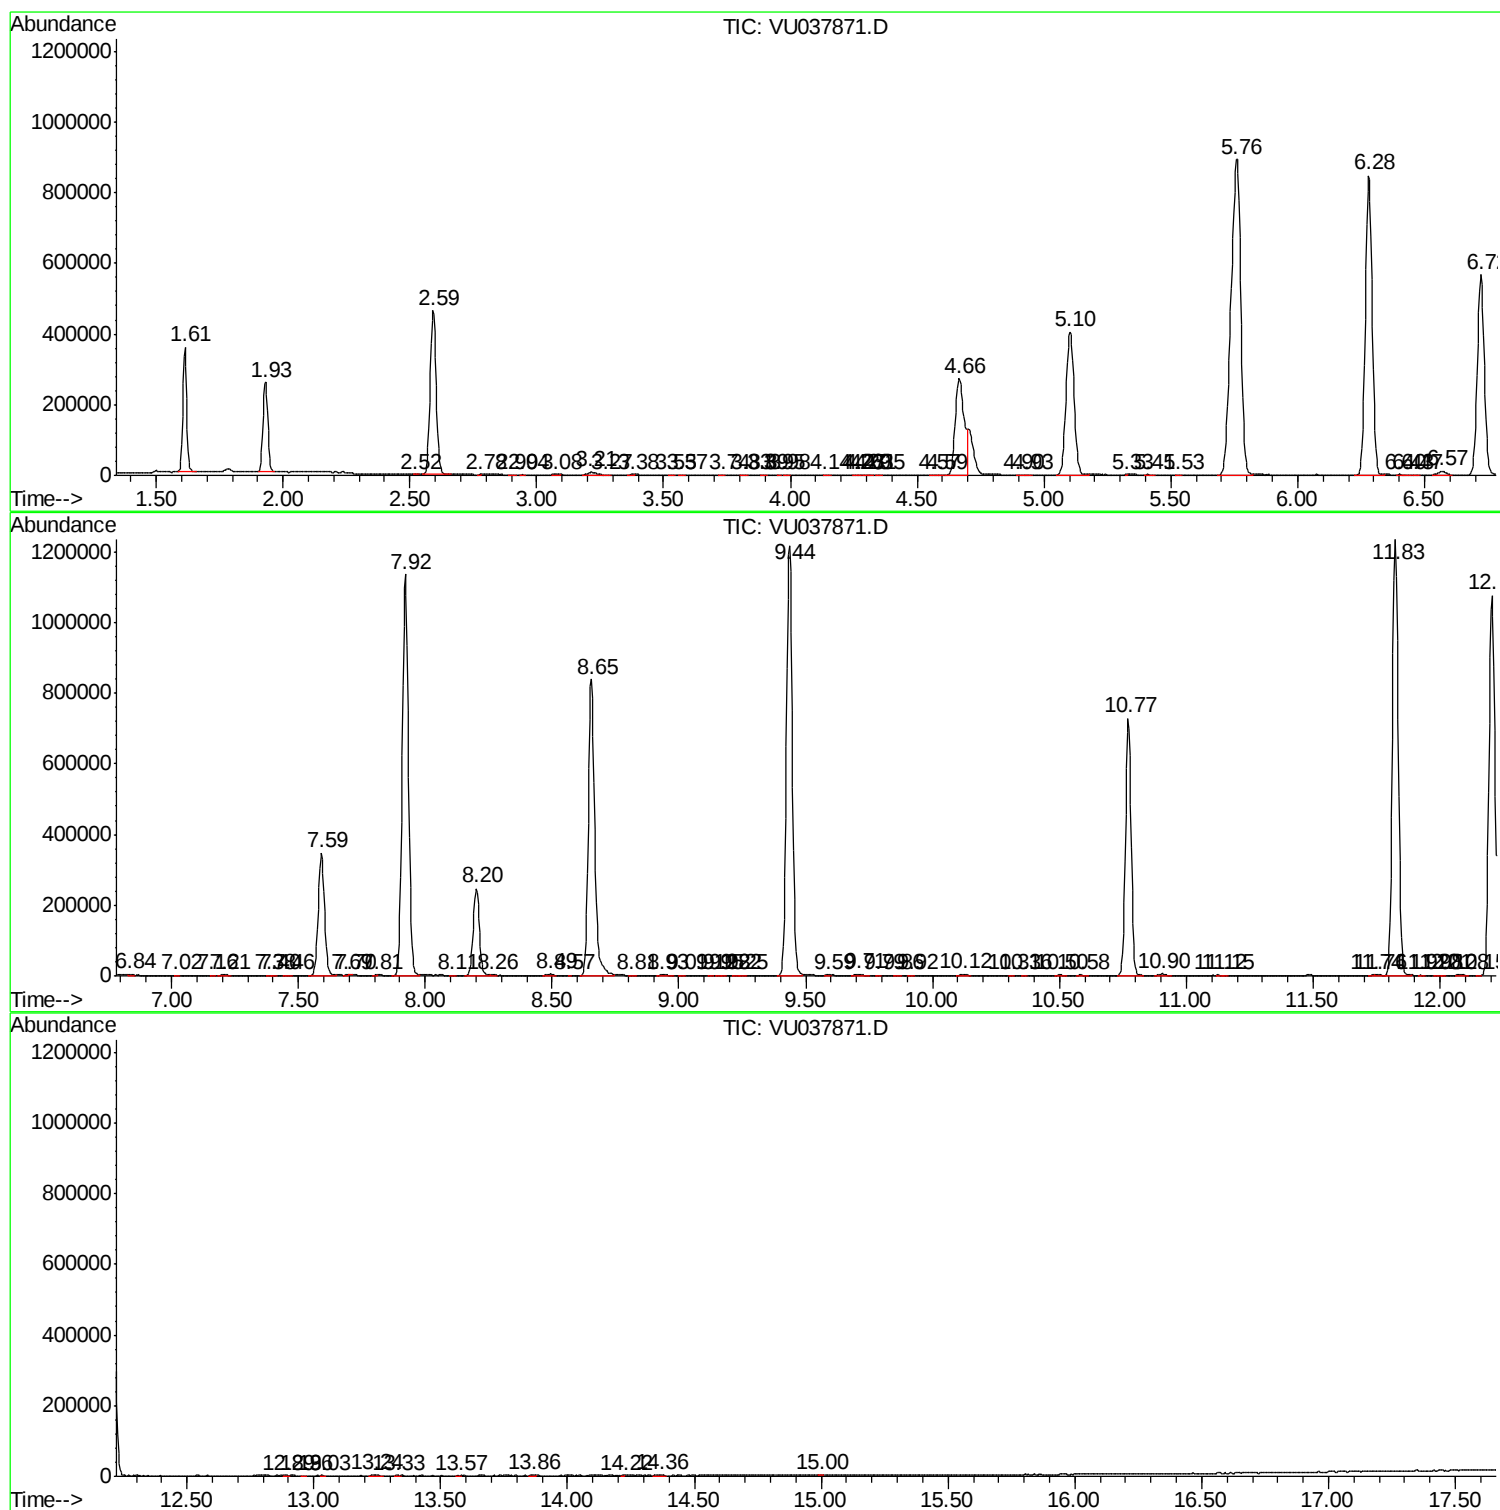

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037871.D
Acq On : 24 Apr 2020 15:17
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037871.D
Acq On : 24 Apr 2020 15:17
Operator : JC/MD
Sample : VIBLK40
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK40

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
