

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037872.D
 Acq On : 24 Apr 2020 15:40
 Operator : JC/MD
 Sample : L2395-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.405	15	20	27	rVB	18829	18011	0.77%	0.088%
2	1.614	77	85	99	rVB	357818	386739	16.54%	1.880%
3	1.932	175	184	200	rVB	253561	338967	14.49%	1.648%
4	2.318	297	304	305	rBV5	2322	2282	0.10%	0.011%
5	2.591	377	389	407	rVV2	488233	850016	36.34%	4.132%
6	2.723	427	430	435	rVB6	1734	1499	0.06%	0.007%
7	2.787	444	450	451	rBV2	4148	3960	0.17%	0.019%
8	2.948	495	500	503	rBV3	725	673	0.03%	0.003%
9	2.993	512	514	520	rVB3	797	596	0.03%	0.003%
10	3.076	531	540	551	rBV7	3157	5284	0.23%	0.026%
11	3.218	575	584	601	rVB4	6447	15713	0.67%	0.076%
12	3.314	610	614	620	rVB2	498	448	0.02%	0.002%
13	3.347	620	624	630	rBV4	610	613	0.03%	0.003%
14	3.388	630	637	639	rBV5	1971	2076	0.09%	0.010%
15	3.671	721	725	728	rVB2	756	593	0.03%	0.003%
16	3.793	761	763	769	rVB2	584	452	0.02%	0.002%
17	3.826	769	773	776	rBV	437	445	0.02%	0.002%
18	4.035	835	838	844	rBV3	504	475	0.02%	0.002%
19	4.205	886	891	896	rVB3	590	686	0.03%	0.003%
20	4.231	896	899	902	rBV2	762	483	0.02%	0.002%
21	4.318	924	926	932	rVV3	441	434	0.02%	0.002%
22	4.440	958	964	966	rBV3	527	439	0.02%	0.002%
23	4.665	1018	1034	1080	rVV2	274388	830741	35.52%	4.038%
24	4.877	1097	1100	1105	rBV3	505	405	0.02%	0.002%
25	4.925	1110	1115	1118	rVB3	449	408	0.02%	0.002%
26	4.957	1118	1125	1128	rBV4	1148	1359	0.06%	0.007%
27	5.028	1144	1147	1150	rBV2	825	627	0.03%	0.003%
28	5.102	1153	1170	1190	rBV	405666	889263	38.02%	4.323%
29	5.353	1234	1248	1263	rBV2	17911	41957	1.79%	0.204%
30	5.408	1263	1265	1272	rVB4	1376	1525	0.07%	0.007%
31	5.761	1351	1375	1399	rBV2	889233	2338883	100.00%	11.370%
32	5.996	1444	1448	1455	rBV4	958	1221	0.05%	0.006%
33	6.137	1487	1492	1493	rBV2	765	556	0.02%	0.003%
34	6.154	1495	1497	1501	rVB3	852	576	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037872.D
 Acq On : 24 Apr 2020 15:40
 Operator : JC/MD
 Sample : L2395-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.279	1520	1536	1555	rBV	742479	1393711	59.59%	6.775%
36	6.414	1574	1578	1580	rBV2	753	489	0.02%	0.002%
37	6.459	1590	1592	1597	rVB2	655	535	0.02%	0.003%
38	6.572	1609	1627	1651	rBV	1132868	2107825	90.12%	10.247%
39	6.723	1658	1674	1695	rBV	558524	1081715	46.25%	5.259%
40	7.186	1815	1818	1820	rBV3	1004	620	0.03%	0.003%
41	7.465	1901	1905	1911	rVB3	417	456	0.02%	0.002%
42	7.591	1929	1944	1962	rBV	344630	595529	25.46%	2.895%
43	7.703	1974	1979	1980	rBV2	1108	974	0.04%	0.005%
44	7.819	2013	2015	2022	rVB3	1290	1137	0.05%	0.006%
45	7.922	2032	2047	2062	rBV	1141989	1919920	82.09%	9.333%
46	7.993	2063	2069	2083	rVB2	15005	26650	1.14%	0.130%
47	8.115	2105	2107	2113	rVB4	878	800	0.03%	0.004%
48	8.202	2121	2134	2158	rBV	242585	409107	17.49%	1.989%
49	8.327	2170	2173	2178	rBV3	565	634	0.03%	0.003%
50	8.382	2187	2190	2194	rBV4	659	562	0.02%	0.003%
51	8.420	2196	2202	2211	rVV4	2519	3607	0.15%	0.018%
52	8.491	2212	2224	2237	rVB	24661	44400	1.90%	0.216%
53	8.571	2242	2249	2251	rBV5	1237	1123	0.05%	0.005%
54	8.655	2261	2275	2300	rBV	835909	1484708	63.48%	7.218%
55	8.848	2333	2335	2338	rBV2	656	476	0.02%	0.002%
56	9.015	2383	2387	2392	rBV2	432	484	0.02%	0.002%
57	9.121	2414	2420	2422	rBV	446	401	0.02%	0.002%
58	9.227	2449	2453	2458	rBV3	902	873	0.04%	0.004%
59	9.301	2464	2476	2481	rBV4	1304	2394	0.10%	0.012%
60	9.436	2504	2518	2550	rBV	1048972	1736295	74.24%	8.441%
61	9.658	2582	2587	2590	rBV4	1373	1316	0.06%	0.006%
62	9.713	2594	2604	2610	rBV5	3416	5873	0.25%	0.029%
63	9.870	2648	2653	2657	rBV2	393	401	0.02%	0.002%
64	10.044	2704	2707	2712	rVB	547	412	0.02%	0.002%
65	10.073	2712	2716	2722	rBV2	721	770	0.03%	0.004%
66	10.115	2723	2729	2732	rBV5	2427	2799	0.12%	0.014%
67	10.211	2754	2759	2766	rVB3	446	607	0.03%	0.003%
68	10.247	2766	2770	2773	rBV3	715	598	0.03%	0.003%
69	10.340	2796	2799	2802	rBV2	631	521	0.02%	0.003%
70	10.362	2802	2806	2811	rVB4	1417	1564	0.07%	0.008%
71	10.398	2811	2817	2823	rBV2	469	742	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037872.D
 Acq On : 24 Apr 2020 15:40
 Operator : JC/MD
 Sample : L2395-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D91

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	10.771	2920	2933	2950	rBV	708039	1131516	48.38%	5.501%
73	10.903	2964	2974	2985	rVB2	27373	44459	1.90%	0.216%
74	11.041	3013	3017	3020	rVV2	553	395	0.02%	0.002%
75	11.099	3031	3035	3037	rBV2	726	485	0.02%	0.002%
76	11.288	3089	3094	3098	rBV3	683	753	0.03%	0.004%
77	11.427	3133	3137	3141	rVB3	973	670	0.03%	0.003%
78	11.475	3148	3152	3155	rBV5	881	853	0.04%	0.004%
79	11.565	3177	3180	3186	rVB4	617	561	0.02%	0.003%
80	11.703	3216	3223	3228	rVV4	2745	3390	0.14%	0.016%
81	11.761	3235	3241	3248	rVB5	2168	2765	0.12%	0.013%
82	11.825	3248	3261	3281	rVB	859574	1384114	59.18%	6.729%
83	12.079	3332	3340	3345	rBV4	1609	2123	0.09%	0.010%
84	12.205	3364	3379	3393	rBV	869507	1382086	59.09%	6.719%
85	12.282	3401	3403	3411	rVV3	525	447	0.02%	0.002%
86	12.333	3415	3419	3426	rBV4	1062	1246	0.05%	0.006%
87	12.427	3443	3448	3452	rBV2	377	474	0.02%	0.002%
88	12.693	3524	3531	3537	rBV6	1887	2469	0.11%	0.012%
89	12.796	3554	3563	3574	rVB	11750	18644	0.80%	0.091%
90	12.857	3577	3582	3584	rBV3	517	434	0.02%	0.002%
91	12.909	3591	3598	3607	rBV7	4690	6425	0.27%	0.031%
92	13.041	3636	3639	3641	rBV2	589	475	0.02%	0.002%
93	13.211	3688	3692	3694	rBV2	577	457	0.02%	0.002%
94	13.240	3695	3701	3711	rVB6	3065	4758	0.20%	0.023%
95	13.288	3711	3716	3719	rBV2	673	758	0.03%	0.004%
96	13.587	3805	3809	3810	rBV	621	450	0.02%	0.002%
97	13.709	3844	3847	3851	rBV2	737	658	0.03%	0.003%
98	13.864	3890	3895	3903	rVB6	2887	3953	0.17%	0.019%
99	14.356	4044	4048	4059	rVB6	3419	4327	0.19%	0.021%
100	14.941	4227	4230	4237	rBV4	933	1102	0.05%	0.005%


Sum of corrected areas: 20570680

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037872.D
Acq On : 24 Apr 2020 15:40
Operator : JC/MD
Sample : L2395-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

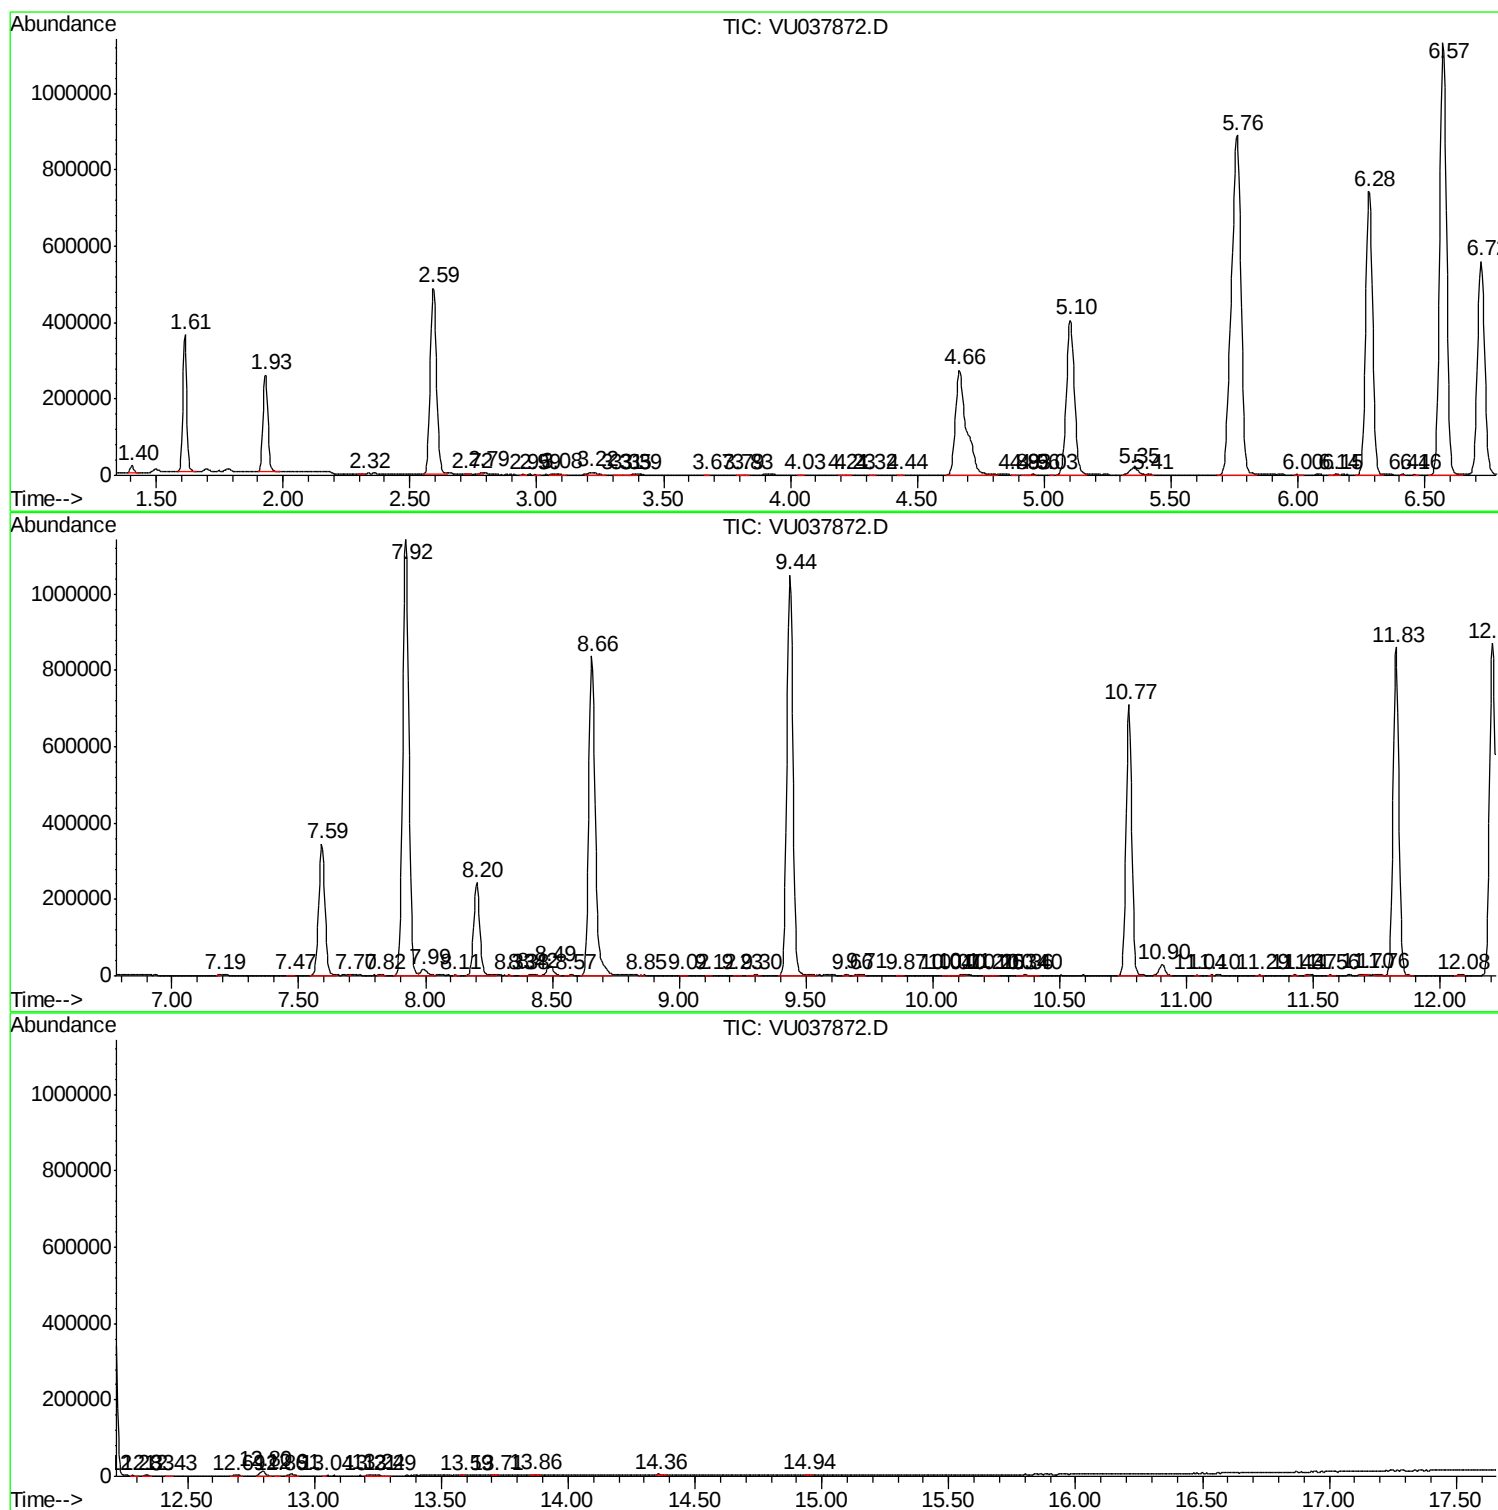

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037872.D
Acq On : 24 Apr 2020 15:40
Operator : JC/MD
Sample : L2395-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037872.D
Acq On : 24 Apr 2020 15:40
Operator : JC/MD
Sample : L2395-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D91

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc