

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037876.D
 Acq On : 24 Apr 2020 17:10
 Operator : JC/MD
 Sample : L2395-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.372	6	10	16	rBV3	9304	9247	0.39%	0.046%
2	1.613	78	85	95	rBV	359497	378176	16.13%	1.892%
3	1.932	176	184	195	rVB	258457	336113	14.34%	1.682%
4	2.359	312	317	322	rVB2	5310	6066	0.26%	0.030%
5	2.591	377	389	403	rBV	471907	789941	33.69%	3.953%
6	2.716	425	428	434	rBV5	1246	1298	0.06%	0.006%
7	2.790	442	451	455	rBV3	4092	6449	0.28%	0.032%
8	3.227	578	587	597	rVB4	6787	13875	0.59%	0.069%
9	3.311	610	613	619	rVB3	785	648	0.03%	0.003%
10	3.385	631	636	640	rBV4	2146	2382	0.10%	0.012%
11	3.613	702	707	708	rBV2	1155	914	0.04%	0.005%
12	3.761	748	753	757	rBV2	688	783	0.03%	0.004%
13	3.819	767	771	773	rBV2	530	319	0.01%	0.002%
14	3.858	781	783	786	rBV	435	316	0.01%	0.002%
15	3.909	791	799	812	rVB2	2343	5288	0.23%	0.026%
16	4.009	826	830	832	rBV3	591	455	0.02%	0.002%
17	4.134	865	869	876	rBV3	476	608	0.03%	0.003%
18	4.243	900	903	910	rBV3	329	408	0.02%	0.002%
19	4.546	995	997	1000	rBV2	604	398	0.02%	0.002%
20	4.568	1000	1004	1011	rVV3	842	1002	0.04%	0.005%
21	4.665	1018	1034	1070	rBV	276854	706844	30.15%	3.537%
22	4.809	1077	1079	1084	rVB2	919	543	0.02%	0.003%
23	4.931	1114	1117	1126	rBV3	703	850	0.04%	0.004%
24	5.018	1142	1144	1148	rVB2	616	334	0.01%	0.002%
25	5.102	1153	1170	1191	rBV	404428	873349	37.25%	4.370%
26	5.353	1233	1248	1259	rBV5	6931	15755	0.67%	0.079%
27	5.494	1288	1292	1297	rVB3	552	531	0.02%	0.003%
28	5.632	1332	1335	1340	rBV	430	427	0.02%	0.002%
29	5.761	1352	1375	1393	rBV2	891245	2344656	100.00%	11.732%
30	5.964	1437	1438	1442	rVV2	556	339	0.01%	0.002%
31	5.983	1442	1444	1447	rVV2	875	599	0.03%	0.003%
32	6.005	1447	1451	1457	rVB5	1276	1526	0.07%	0.008%
33	6.057	1464	1467	1468	rBV2	927	476	0.02%	0.002%
34	6.108	1480	1483	1486	rBV2	673	493	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037876.D
 Acq On : 24 Apr 2020 17:10
 Operator : JC/MD
 Sample : L2395-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.144	1486	1494	1495	rBV4	976	929	0.04%	0.005%
36	6.282	1521	1537	1556	rBV	753082	1406870	60.00%	7.040%
37	6.571	1612	1627	1649	rVV	971648	1795095	76.56%	8.982%
38	6.722	1659	1674	1693	rBV	555721	1081574	46.13%	5.412%
39	7.050	1773	1776	1778	rBV2	423	334	0.01%	0.002%
40	7.201	1817	1823	1824	rBV3	1956	1503	0.06%	0.008%
41	7.333	1861	1864	1865	rBV	504	332	0.01%	0.002%
42	7.591	1931	1944	1963	rBV	346398	598589	25.53%	2.995%
43	7.703	1973	1979	1981	rBV7	1343	1414	0.06%	0.007%
44	7.812	2011	2013	2017	rVB4	722	397	0.02%	0.002%
45	7.922	2030	2047	2064	rBV	1142043	1936721	82.60%	9.691%
46	8.150	2113	2118	2119	rBV2	502	404	0.02%	0.002%
47	8.201	2121	2134	2151	rBV	244129	407439	17.38%	2.039%
48	8.320	2166	2171	2175	rVB4	935	1040	0.04%	0.005%
49	8.349	2175	2180	2185	rVB4	854	909	0.04%	0.005%
50	8.491	2214	2224	2238	rVB4	3930	8593	0.37%	0.043%
51	8.558	2242	2245	2247	rBV	598	398	0.02%	0.002%
52	8.655	2262	2275	2301	rBV	854348	1487456	63.44%	7.443%
53	8.909	2352	2354	2358	rVB2	584	317	0.01%	0.002%
54	8.941	2359	2364	2367	rBV2	564	467	0.02%	0.002%
55	9.044	2393	2396	2399	rBV	582	323	0.01%	0.002%
56	9.179	2436	2438	2445	rVB4	689	731	0.03%	0.004%
57	9.269	2463	2466	2468	rBV	496	315	0.01%	0.002%
58	9.436	2504	2518	2541	rBV	1086015	1763400	75.21%	8.824%
59	9.587	2556	2565	2571	rBV2	4093	5441	0.23%	0.027%
60	9.658	2583	2587	2588	rBV2	913	705	0.03%	0.004%
61	9.709	2594	2603	2611	rBV2	5487	8449	0.36%	0.042%
62	10.002	2690	2694	2699	rBV3	645	608	0.03%	0.003%
63	10.028	2699	2702	2706	rVB	596	371	0.02%	0.002%
64	10.118	2723	2730	2744	rVB5	5528	8483	0.36%	0.042%
65	10.320	2790	2793	2799	rVB2	442	484	0.02%	0.002%
66	10.359	2799	2805	2811	rBV3	695	893	0.04%	0.004%
67	10.494	2843	2847	2849	rBV	862	644	0.03%	0.003%
68	10.539	2858	2861	2863	rBV	536	312	0.01%	0.002%
69	10.770	2920	2933	2949	rVV	700702	1139902	48.62%	5.704%
70	10.902	2968	2974	2985	rVB5	3687	5802	0.25%	0.029%
71	11.105	3032	3037	3040	rBV	698	652	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042420\
 Data File : VU037876.D
 Acq On : 24 Apr 2020 17:10
 Operator : JC/MD
 Sample : L2395-10
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D95

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	11.163	3052	3055	3061	rVB	317	311	0.01%	0.002%
73	11.433	3137	3139	3144	rVB2	846	514	0.02%	0.003%
74	11.484	3148	3155	3160	rVB6	1162	1280	0.05%	0.006%
75	11.513	3160	3164	3171	rBV	442	761	0.03%	0.004%
76	11.658	3205	3209	3213	rVB2	872	777	0.03%	0.004%
77	11.758	3236	3240	3245	rBV3	828	859	0.04%	0.004%
78	11.825	3248	3261	3277	rBV	753828	1175912	50.15%	5.884%
79	11.976	3304	3308	3311	rBV3	961	783	0.03%	0.004%
80	12.076	3332	3339	3343	rBV4	1380	1868	0.08%	0.009%
81	12.204	3366	3379	3395	rBV	933974	1467634	62.59%	7.344%
82	12.314	3406	3413	3417	rBV6	1336	1723	0.07%	0.009%
83	12.410	3440	3443	3447	rBV2	487	413	0.02%	0.002%
84	12.475	3461	3463	3473	rVB4	678	778	0.03%	0.004%
85	12.565	3484	3491	3496	rBV7	1413	1937	0.08%	0.010%
86	13.134	3663	3668	3674	rVB6	2186	2741	0.12%	0.014%
87	13.243	3697	3702	3704	rBV5	1470	1448	0.06%	0.007%
88	13.275	3706	3712	3719	rVB5	4570	6918	0.30%	0.035%
89	13.346	3730	3734	3745	rVB5	2188	2967	0.13%	0.015%
90	13.606	3812	3815	3816	rBV2	1105	648	0.03%	0.003%
91	13.700	3842	3844	3847	rBV2	680	470	0.02%	0.002%
92	13.864	3890	3895	3900	rVB7	4687	5712	0.24%	0.029%
93	13.909	3902	3909	3911	rBV6	4034	4966	0.21%	0.025%
94	14.217	3996	4005	4017	rVB	22200	35101	1.50%	0.176%
95	14.314	4027	4035	4045	rVB3	19105	31149	1.33%	0.156%
96	14.703	4148	4156	4169	rBV9	8420	17779	0.76%	0.089%
97	14.841	4192	4199	4210	rBV3	10624	16217	0.69%	0.081%
98	15.056	4260	4266	4267	rBV4	6532	5150	0.22%	0.026%
99	15.237	4316	4322	4327	rBV8	7629	11057	0.47%	0.055%
100	15.314	4340	4346	4356	rVB4	10830	17434	0.74%	0.087%


Sum of corrected areas: 19985011

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042420\
Data File : VU037876.D
Acq On : 24 Apr 2020 17:10
Operator : JC/MD
Sample : L2395-10
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

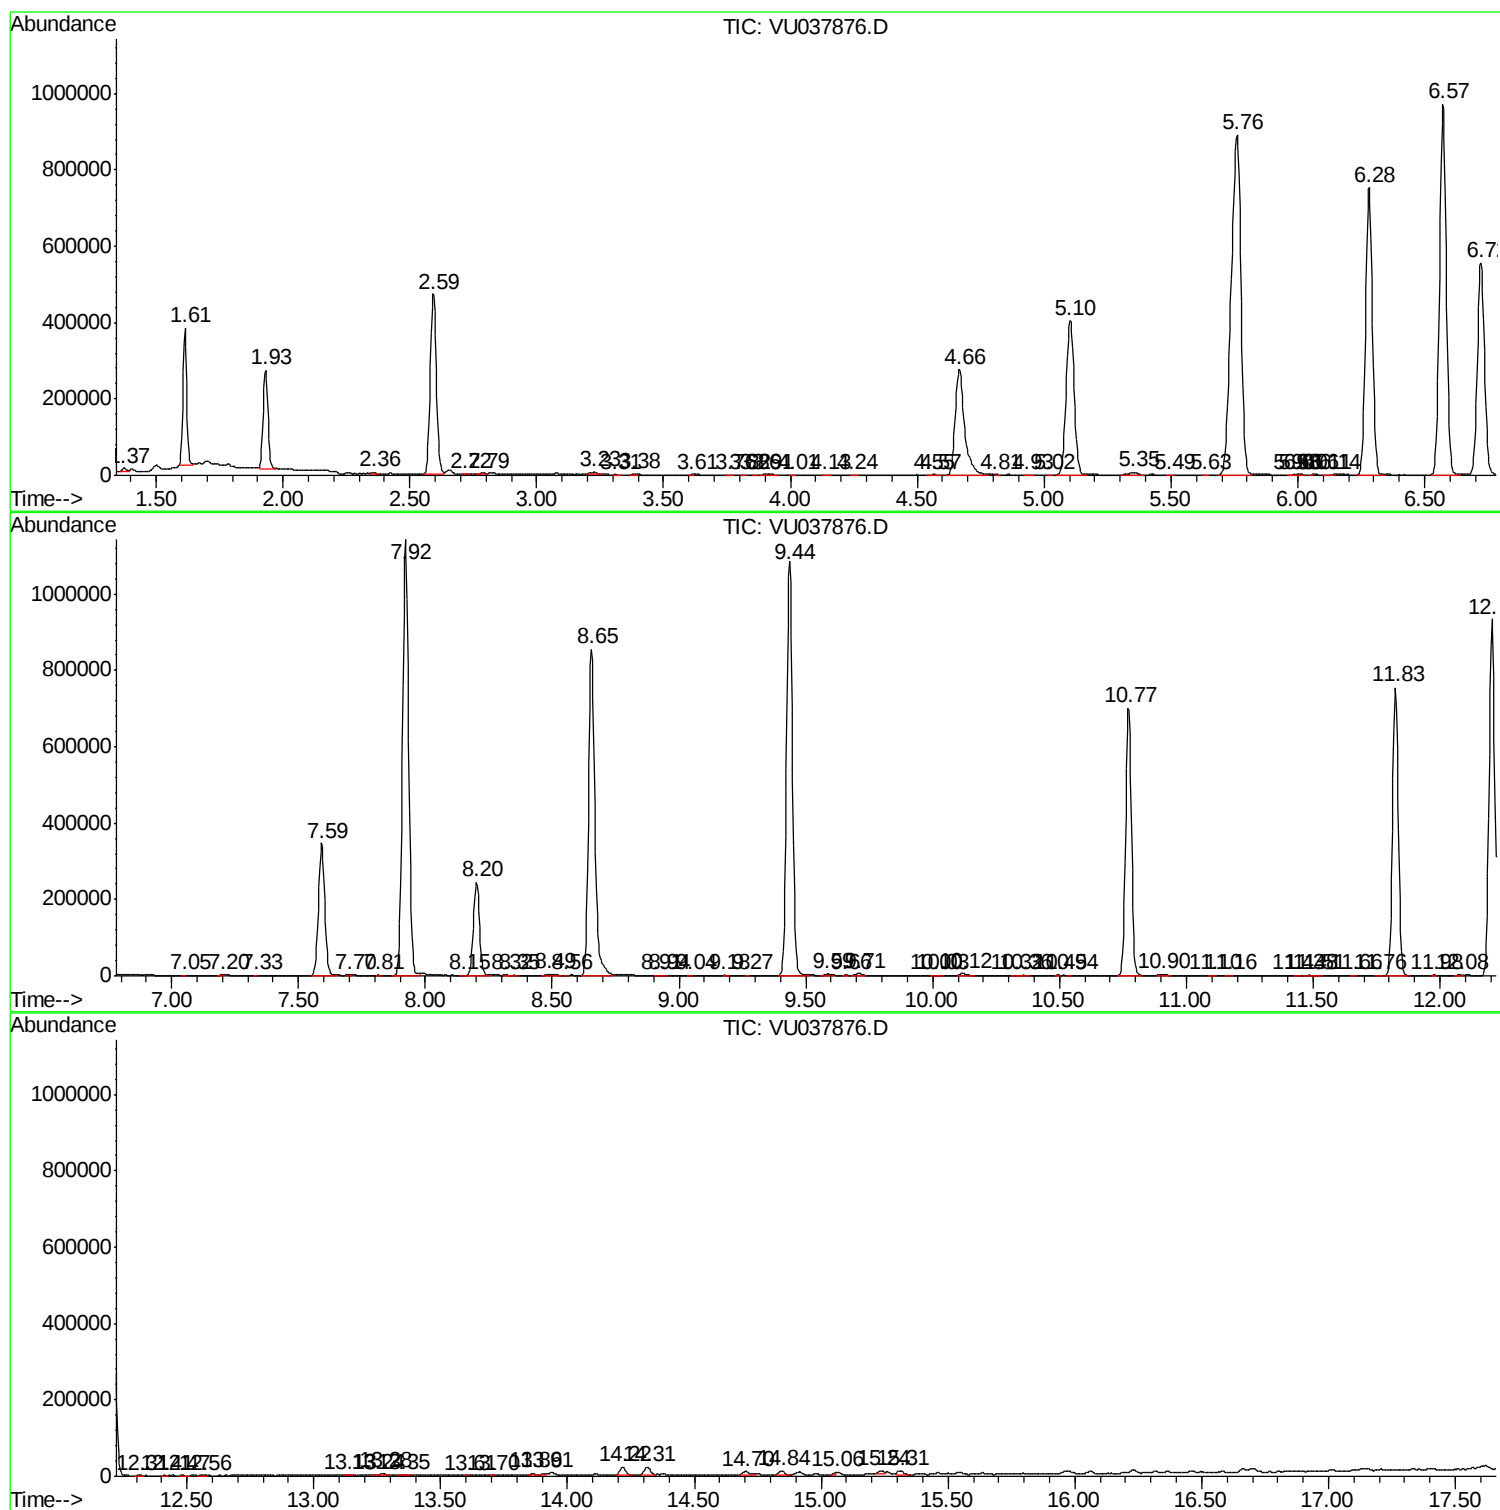

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037876.D
Acq On : 24 Apr 2020 17:10
Operator : JC/MD
Sample : L2395-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042420\
Data File : VU037876.D
Acq On : 24 Apr 2020 17:10
Operator : JC/MD
Sample : L2395-10
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D95

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc