


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU042420\
 Data File : VU037865.D
 Acq On : 24 Apr 2020 08:56
 Operator : JC/MD
 Sample : BFB42
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB42

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis
 Last Update : Sat Apr 25 01:13:34 2020

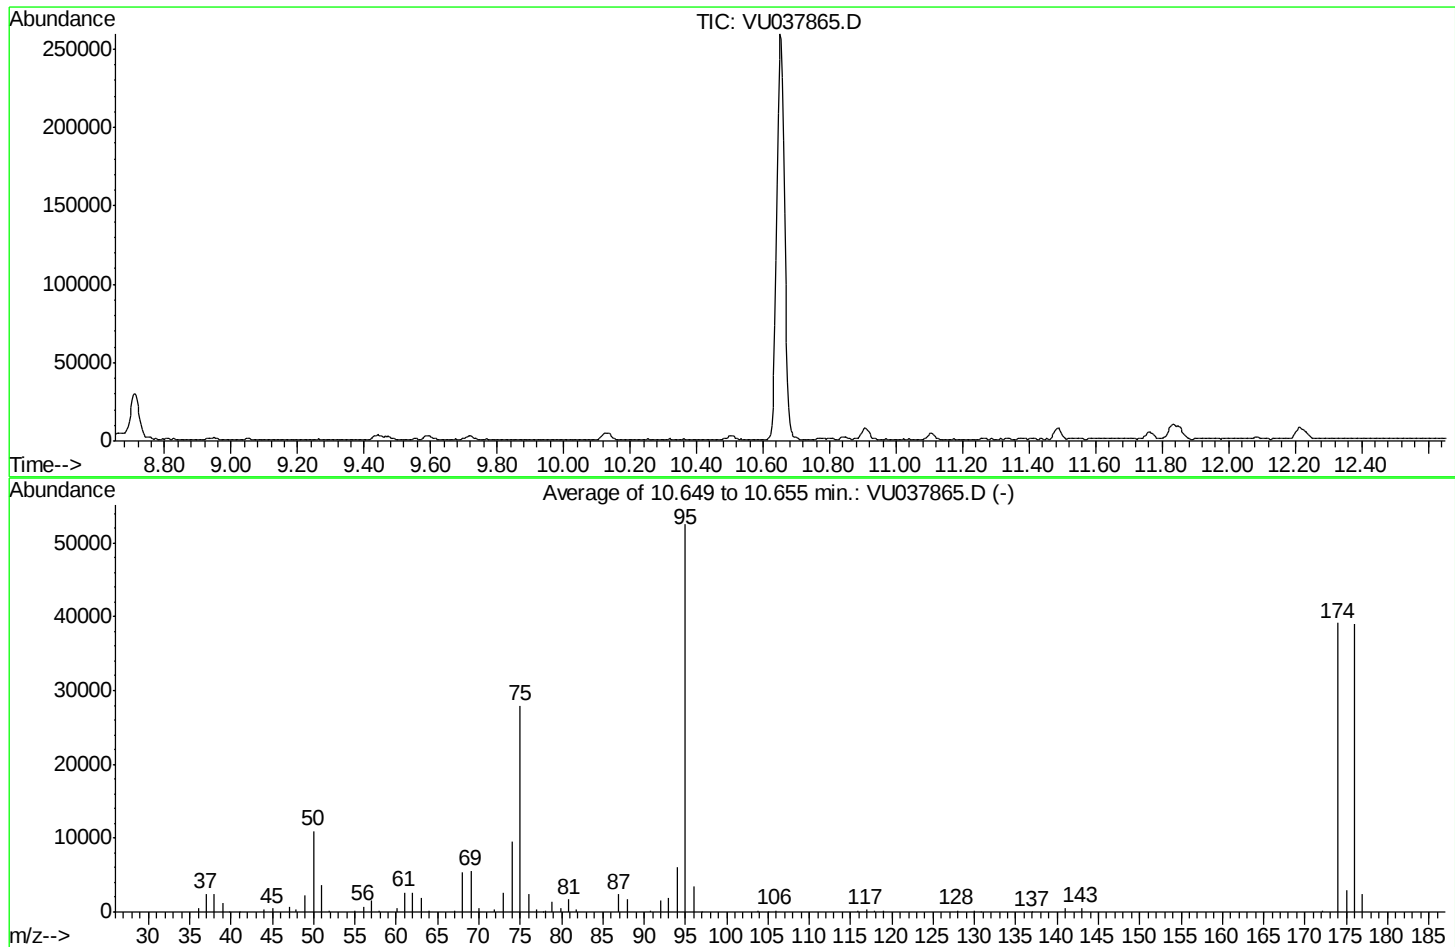

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.8	10928	PASS
75	95	30	80	53.2	27928	PASS
95	95	100	100	100.0	52509	PASS
96	95	5	9	6.6	3461	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.5	39120	PASS
175	174	5	9	7.5	2922	PASS
176	174	95	101	99.9	39069	PASS
177	176	5	9	6.3	2443	PASS

m/z	Abundance
36.00	462.0
37.00	2507.0
38.00	2401.0
39.00	1125.0
39.90	294.0
44.00	1472.0
45.00	544.0
47.00	685.0
47.90	305.0
49.00	2297.0
50.00	10876.0
51.00	3373.0
52.00	120.0
54.90	240.0
56.00	694.0
57.00	1741.0
57.90	102.0
60.00	512.0
61.00	2615.0
62.00	2501.0
63.00	1778.0
64.00	128.0
67.10	167.0
68.00	5223.0
69.00	5519.0
70.00	531.0
71.90	320.0
73.00	2330.0
74.00	8921.0
75.00	27456.0
76.00	2392.0
76.90	474.0
78.10	216.0
78.90	1349.0
79.90	617.0
80.90	1713.0
81.90	342.0
87.00	2251.0
88.00	1832.0
90.70	168.0
92.00	1489.0
93.00	1910.0
94.00	5871.0
95.00	49888.0
96.00	3186.0
103.80	185.0
105.00	109.0
105.90	198.0
115.90	206.0
117.00	337.0
117.90	193.0
118.90	232.0
127.90	189.0
130.00	140.0
137.00	119.0
141.00	438.0
142.90	514.0
172.20	201.0
174.00	37248.0
175.00	2824.0
176.00	36856.0
177.00	2166.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	477.0
37.00	2482.0
38.00	2510.0
39.00	1272.0
39.90	236.0
41.10	106.0
43.90	1275.0
45.00	515.0
47.00	620.0
47.90	323.0
49.00	2342.0
50.00	11176.0
51.00	3690.0
51.90	191.0
54.90	166.0
56.00	813.0
57.00	1650.0
57.90	118.0
60.00	480.0
61.00	2735.0
62.00	2615.0
63.00	1965.0
64.00	138.0
67.10	196.0
68.00	5521.0
69.10	5796.0
70.00	585.0
71.90	367.0
73.00	2727.0
74.00	9834.0
75.00	28616.0
76.00	2516.0
76.90	455.0
78.00	232.0
78.90	1463.0
79.90	568.0
80.90	1734.0
81.90	410.0
87.00	2441.0
88.00	1729.0
90.80	219.0
92.00	1512.0
93.00	2063.0
94.00	6130.0
95.00	53856.0
96.00	3560.0
103.90	209.0
105.90	283.0
115.90	210.0
116.90	322.0
117.90	153.0
118.90	281.0
127.90	209.0
129.90	105.0
137.00	133.0
141.00	475.0
142.90	525.0
172.20	210.0
174.00	40376.0
175.00	2941.0
176.00	40320.0
177.00	2479.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

m/z	Abundance
36.00	478.0
37.00	2457.0
38.00	2382.0
39.00	1238.0
39.80	209.0
41.10	110.0
43.90	1068.0
45.00	436.0
47.00	591.0
47.90	324.0
49.00	2220.0
50.00	10734.0
51.00	3745.0
51.90	232.0
54.80	114.0
56.00	838.0
57.00	1423.0
57.90	118.0
60.10	446.0
61.00	2614.0
62.00	2683.0
63.00	1834.0
64.00	177.0
67.10	216.0
68.00	5338.0
69.10	5524.0
70.00	534.0
71.90	310.0
73.00	2765.0
74.00	10097.0
75.00	27712.0
76.00	2536.0
76.90	373.0
77.80	275.0
78.90	1419.0
79.90	459.0
80.90	1634.0
81.80	442.0
86.90	2375.0
88.00	1688.0
90.90	244.0
92.00	1554.0
93.00	1987.0
94.00	6157.0
95.00	53784.0
96.00	3637.0
96.90	130.0
103.90	218.0
105.90	295.0
115.90	171.0
116.90	384.0
117.90	131.0
118.90	253.0
127.90	196.0
129.90	109.0
130.80	115.0
141.00	525.0
143.00	535.0
172.10	180.0
174.00	39736.0
175.00	3001.0
176.00	40032.0
177.00	2684.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42

Scan 2883 (10.610 min): VU037865.D
BFB42

m/z	Abundance
39.90	186.0
43.90	848.0

Instrument :
MSVOA_U
ClientSampleId :
BFB42