

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053845.D
 Acq On : 24 Apr 2023 16:31
 Operator : JC/MD
 Sample : 02392-12 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE32

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053845.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	97	rVB	55315	64815	14.33%	1.532%
2	1.912	170	178	194	rBV	46708	61890	13.69%	1.463%
3	2.565	370	381	398	rVB2	92369	158723	35.10%	3.752%
4	3.047	520	531	543	rBV3	6282	11791	2.61%	0.279%
5	4.636	1012	1025	1059	rBV2	44606	154221	34.10%	3.646%
6	5.060	1140	1157	1183	rBV	81862	180605	39.94%	4.269%
7	5.723	1341	1363	1383	rBV2	155318	398923	88.22%	9.430%
8	6.243	1511	1525	1552	rBV	159557	308797	68.29%	7.300%
9	6.539	1604	1617	1642	rBV2	153402	294389	65.10%	6.959%
10	6.687	1649	1663	1685	rBV	92860	186662	41.28%	4.412%
11	7.562	1924	1935	1952	rBV	48016	83294	18.42%	1.969%
12	7.896	2026	2039	2059	rBV	190163	338689	74.90%	8.006%
13	8.176	2116	2126	2147	rBV2	28244	49659	10.98%	1.174%
14	8.468	2206	2217	2229	rBV2	2907	5369	1.19%	0.127%
15	8.549	2229	2242	2257	rBV	264673	452212	100.00%	10.690%
16	8.629	2257	2267	2299	rVB	169532	328650	72.68%	7.769%
17	9.414	2499	2511	2528	rBV	223828	373165	82.52%	8.821%
18	10.751	2916	2927	2941	rBV2	67622	111817	24.73%	2.643%
19	11.809	3244	3256	3278	rBV	227737	375414	83.02%	8.874%
20	12.189	3362	3374	3396	rBV	174054	291251	64.41%	6.885%




Sum of corrected areas: 4230336

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053845.D
Acq On : 24 Apr 2023 16:31
Operator : JC/MD
Sample : 02392-12 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

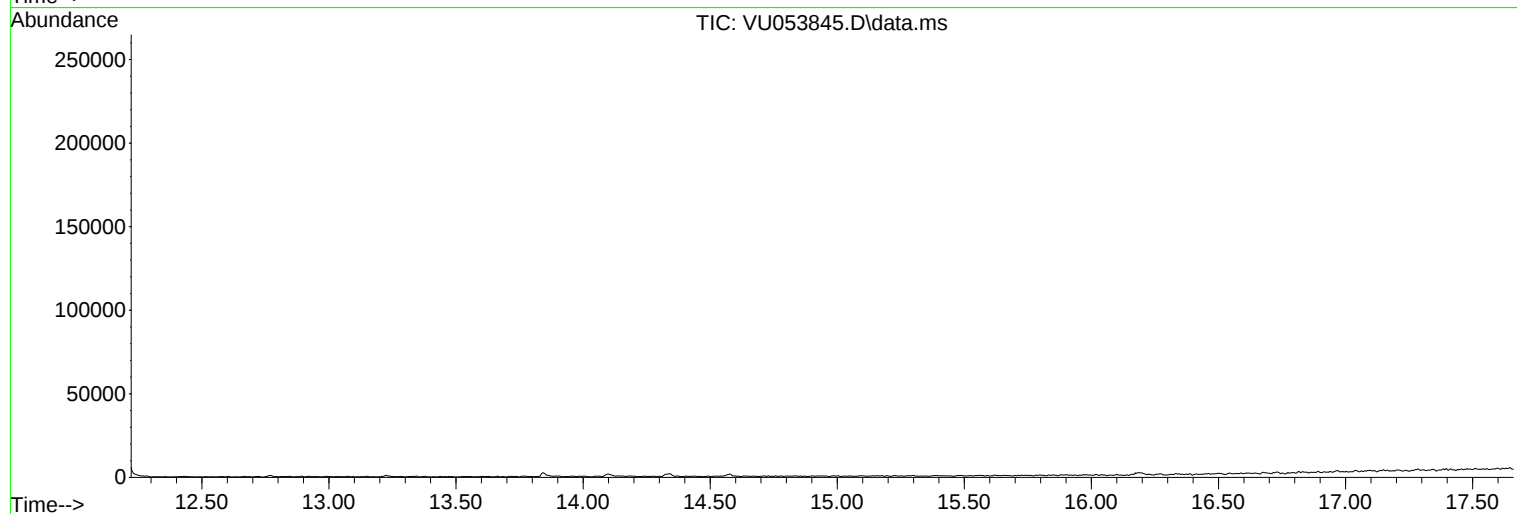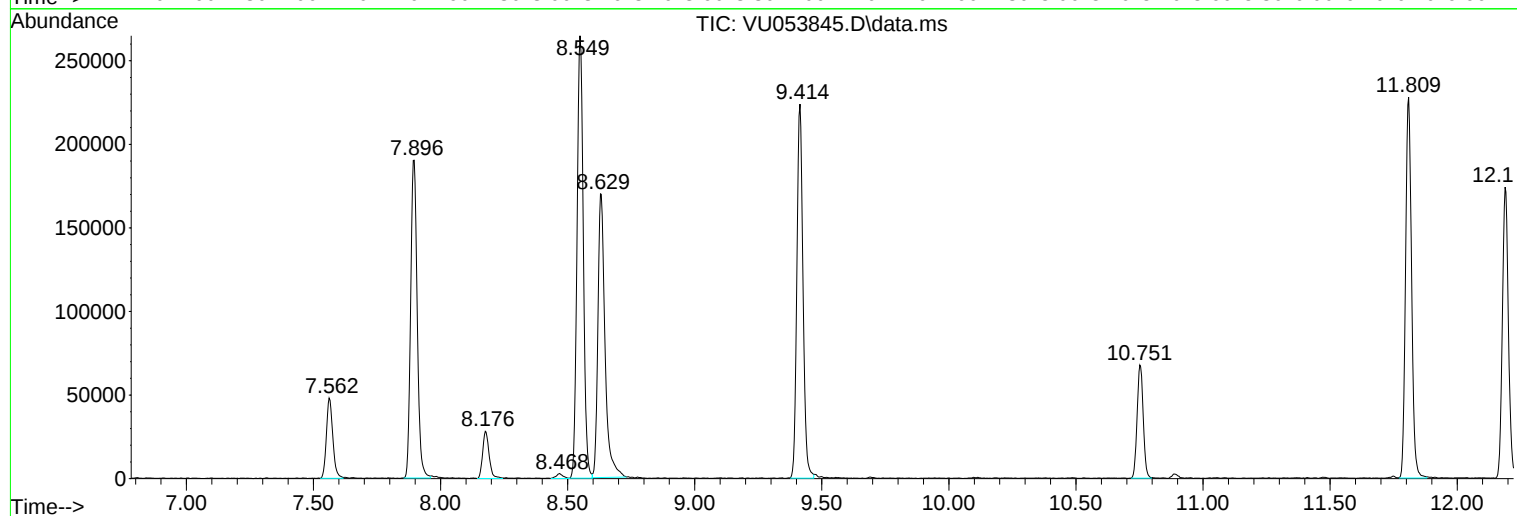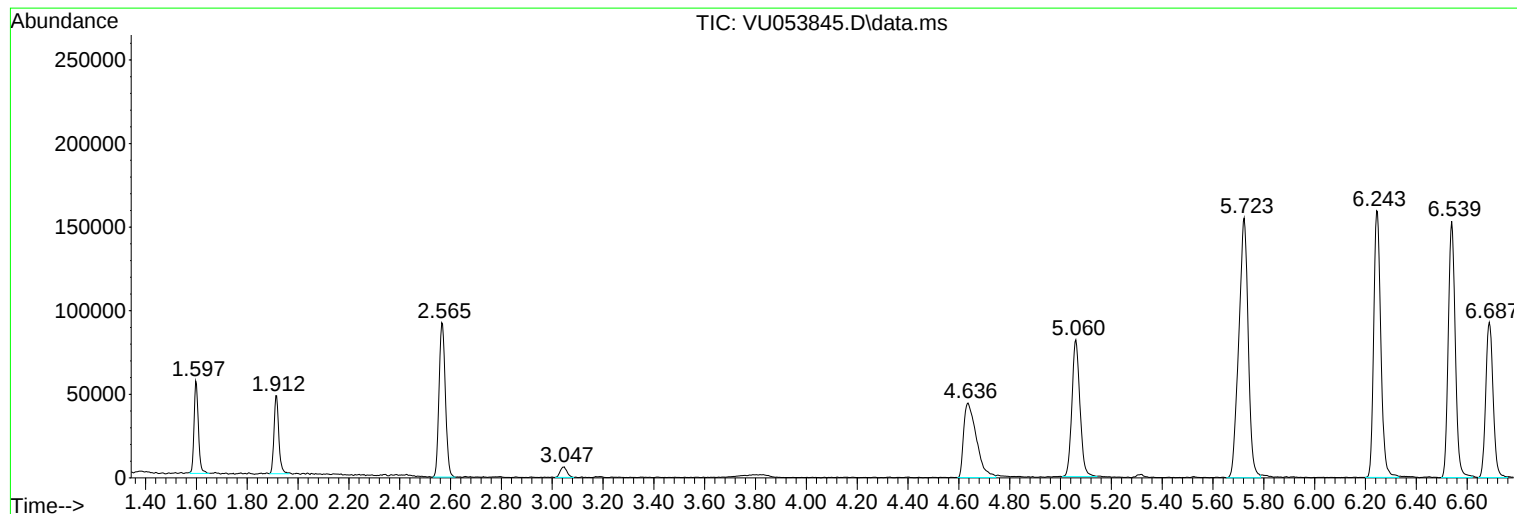

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053845.D
Acq On : 24 Apr 2023 16:31
Operator : JC/MD
Sample : 02392-12 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053845.D
Acq On : 24 Apr 2023 16:31
Operator : JC/MD
Sample : 02392-12 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------