

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053846.D
 Acq On : 24 Apr 2023 16:55
 Operator : JC/MD
 Sample : 02392-13 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE33

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	93	rBV	53522	60777	10.80%	1.495%
2	1.916	170	179	188	rBV	45225	59409	10.56%	1.462%
3	2.568	368	382	399	rBV	86184	143956	25.59%	3.542%
4	3.044	520	530	542	rBV4	5439	10518	1.87%	0.259%
5	4.636	1013	1025	1065	rBV2	40626	135531	24.09%	3.335%
6	5.060	1141	1157	1182	rVB	77302	177841	31.61%	4.376%
7	5.722	1343	1363	1390	rBV2	148722	385134	68.46%	9.476%
8	6.247	1509	1526	1547	rBV	169686	325504	57.86%	8.009%
9	6.542	1606	1618	1632	rBV	27130	49746	8.84%	1.224%
10	6.687	1650	1663	1680	rBV2	90268	178125	31.66%	4.383%
11	7.562	1922	1935	1950	rBV2	45998	81978	14.57%	2.017%
12	7.896	2026	2039	2057	rBV	189377	333027	59.19%	8.194%
13	8.176	2115	2126	2144	rBV2	26044	45083	8.01%	1.109%
14	8.549	2230	2242	2257	rVV	331185	562600	100.00%	13.842%
15	8.632	2257	2268	2300	rVB	169349	330213	58.69%	8.124%
16	9.414	2499	2511	2537	rBV	231143	394819	70.18%	9.714%
17	10.751	2912	2927	2944	rBV2	66364	110416	19.63%	2.717%
18	11.809	3244	3256	3278	rBV	243291	395680	70.33%	9.735%
19	12.188	3362	3374	3392	rBV	168029	284054	50.49%	6.989%




Sum of corrected areas: 4064411

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053846.D
Acq On : 24 Apr 2023 16:55
Operator : JC/MD
Sample : 02392-13 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

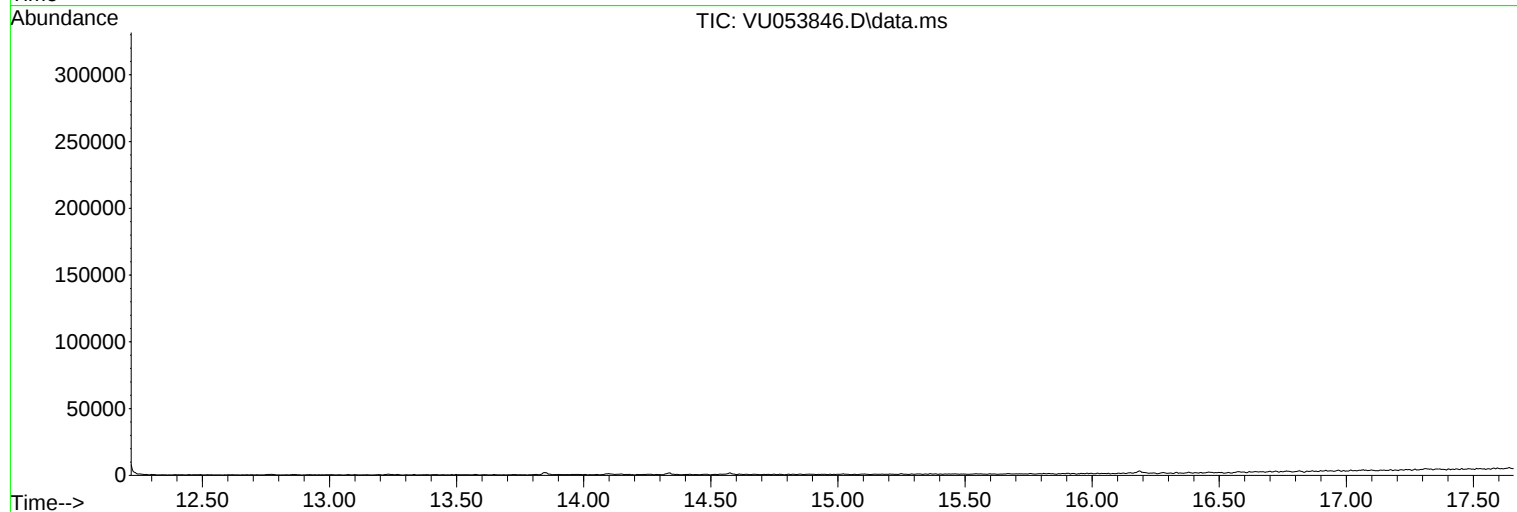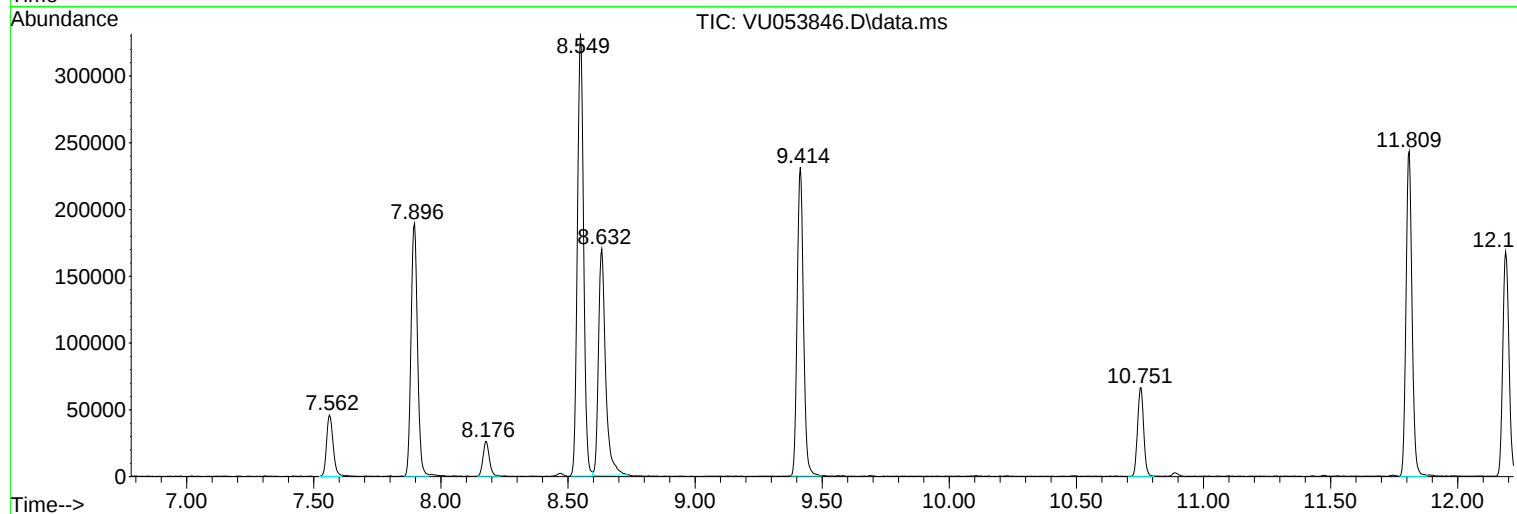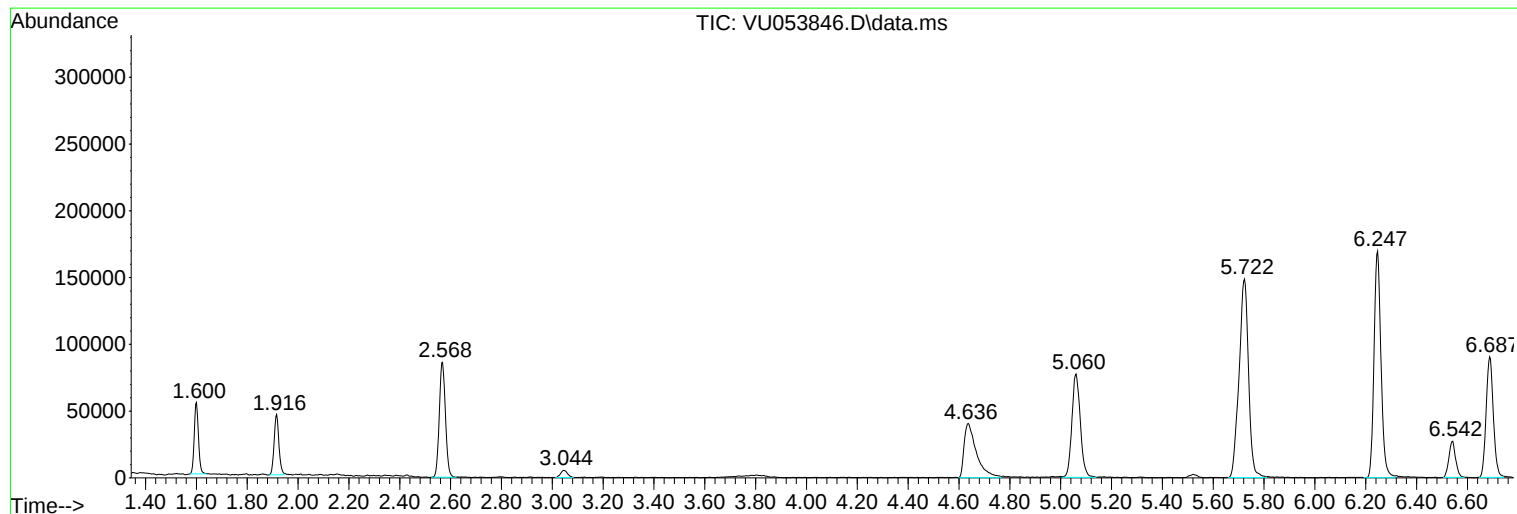

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053846.D
Acq On : 24 Apr 2023 16:55
Operator : JC/MD
Sample : 02392-13 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053846.D
Acq On : 24 Apr 2023 16:55
Operator : JC/MD
Sample : 02392-13 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE33

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc