

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053850.D
 Acq On : 24 Apr 2023 18:32
 Operator : JC/MD
 Sample : 02433-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053850.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	72	81	92	rBV	55325	63988	16.88%	1.881%
2	1.916	169	179	194	rBV	46653	63137	16.66%	1.856%
3	2.568	370	382	397	rVB	86544	140136	36.98%	4.119%
4	3.051	521	532	541	rVB4	2366	4459	1.18%	0.131%
5	4.636	1011	1025	1056	rBV	41203	128418	33.89%	3.775%
6	5.060	1141	1157	1176	rBV	78524	173355	45.74%	5.095%
7	5.722	1342	1363	1386	rBV2	145257	377861	99.71%	11.107%
8	6.247	1513	1526	1553	rBV	160358	309776	81.74%	9.105%
9	6.687	1649	1663	1684	rBV	91894	182034	48.03%	5.351%
10	7.562	1924	1935	1955	rBV2	44406	79257	20.91%	2.330%
11	7.896	2026	2039	2055	rBV	184267	328048	86.56%	9.642%
12	7.967	2055	2061	2075	rVB2	4498	8635	2.28%	0.254%
13	8.176	2113	2126	2147	rBV2	26652	45164	11.92%	1.328%
14	8.468	2209	2217	2230	rVB3	4381	7743	2.04%	0.228%
15	8.632	2256	2268	2298	rBV2	167003	326276	86.10%	9.590%
16	9.414	2499	2511	2537	rBV	220659	374499	98.82%	11.008%
17	10.751	2915	2927	2944	rBV	68430	112523	29.69%	3.307%
18	10.886	2961	2969	2982	rBV3	7655	12075	3.19%	0.355%
19	11.809	3240	3256	3276	rBV	233807	378971	100.00%	11.139%
20	12.188	3361	3374	3393	rBV	170333	285795	75.41%	8.400%




Sum of corrected areas: 3402150

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053850.D
Acq On : 24 Apr 2023 18:32
Operator : JC/MD
Sample : 02433-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

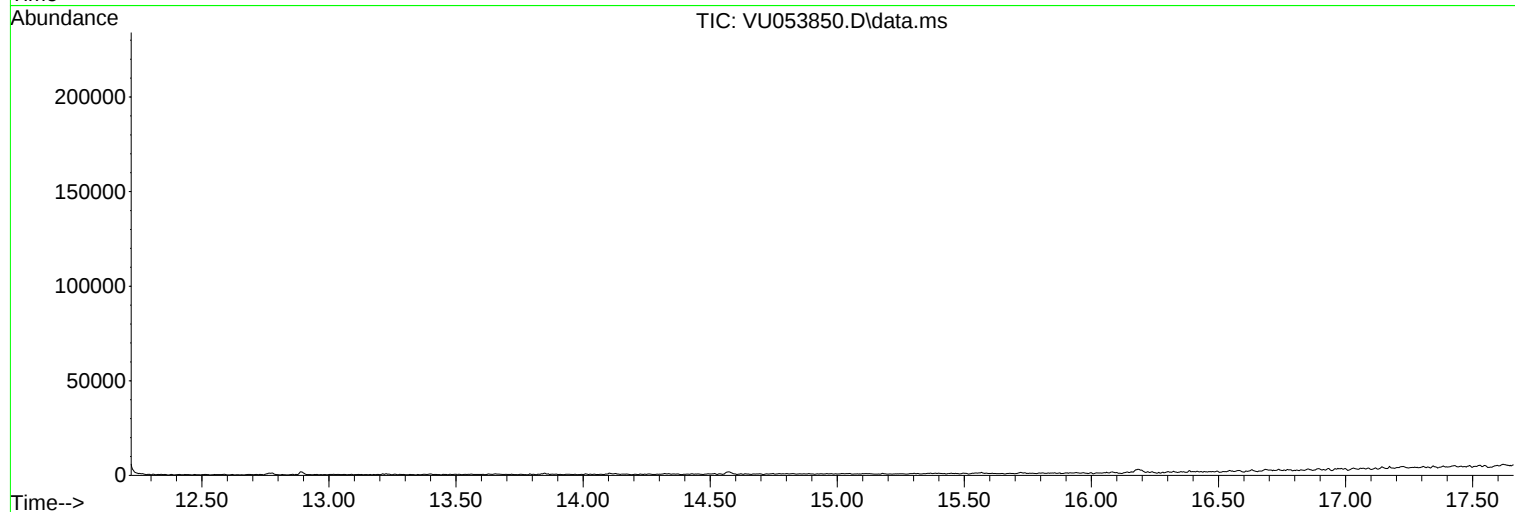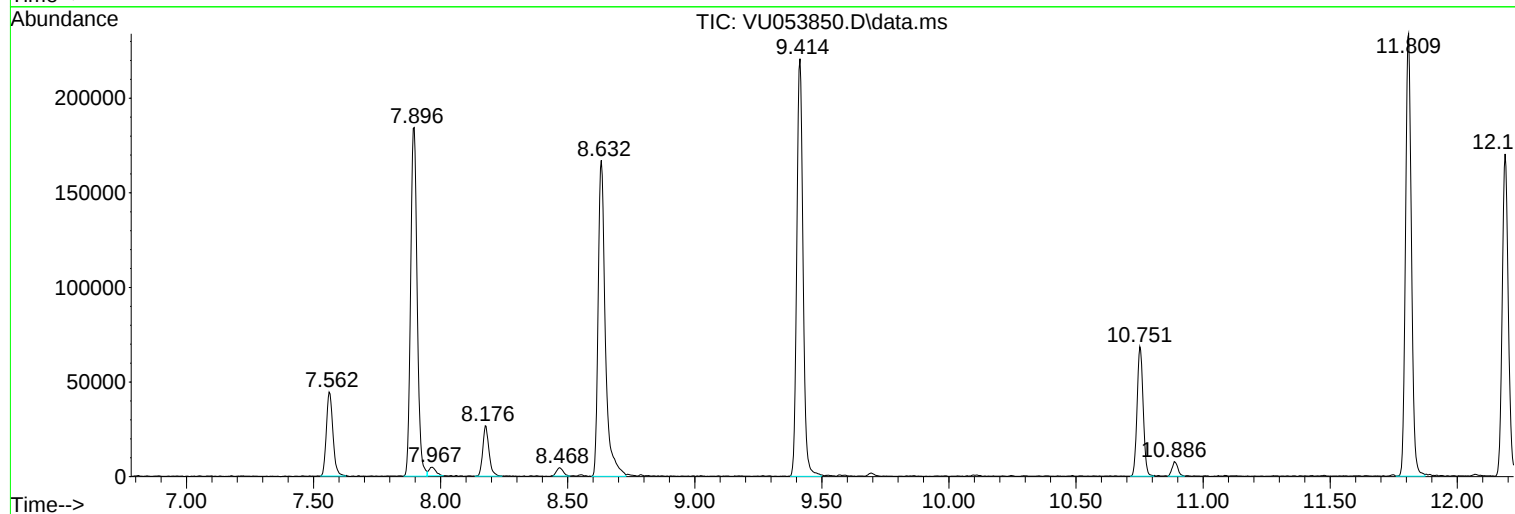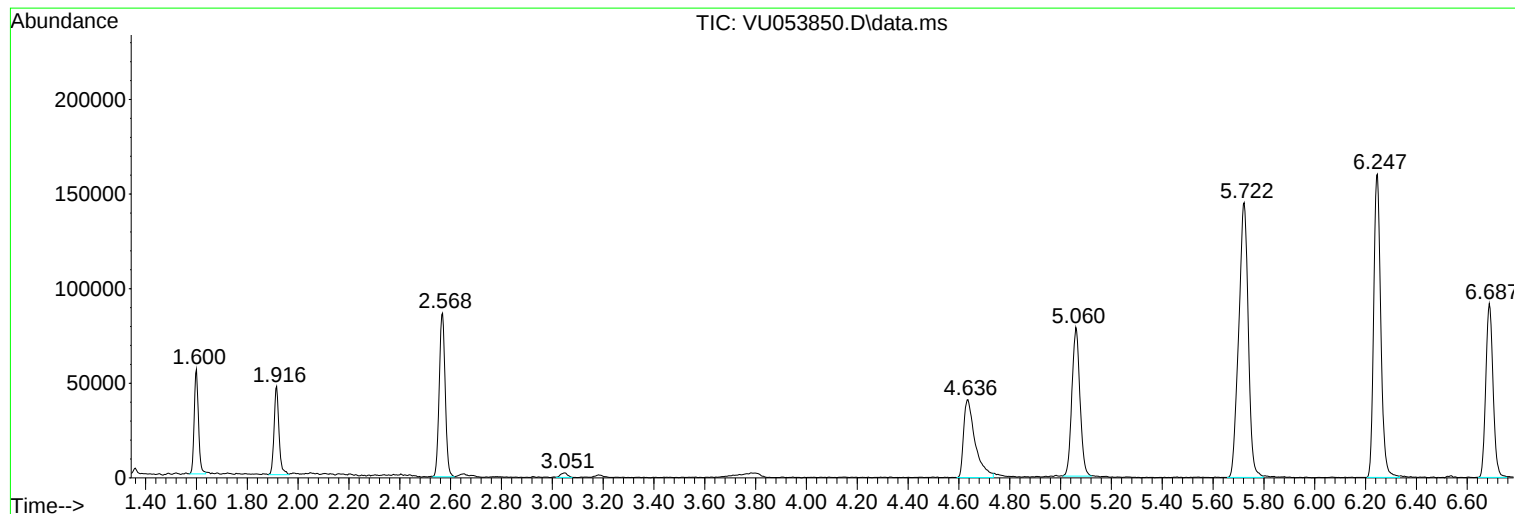

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053850.D
Acq On : 24 Apr 2023 18:32
Operator : JC/MD
Sample : 02433-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053850.D
Acq On : 24 Apr 2023 18:32
Operator : JC/MD
Sample : 02433-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc