

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053853.D
 Acq On : 24 Apr 2023 19:44
 Operator : JC/MD
 Sample : 02433-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE46

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053853.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	70	81	95	rBV	52200	62521	15.89%	1.829%
2	1.916	170	179	197	rVB	44431	61109	15.53%	1.788%
3	2.568	370	382	398	rBV	87422	141803	36.03%	4.148%
4	3.044	522	530	541	rBV4	4013	6401	1.63%	0.187%
5	4.636	1013	1025	1058	rBV	40656	132076	33.56%	3.864%
6	5.060	1142	1157	1180	rVB	78398	176604	44.87%	5.166%
7	5.723	1343	1363	1382	rBV2	153877	393553	100.00%	11.513%
8	6.247	1511	1526	1555	rBV	159176	304703	77.42%	8.914%
9	6.687	1650	1663	1686	rBV2	91104	182550	46.39%	5.340%
10	7.562	1924	1935	1953	rBV	46529	82548	20.98%	2.415%
11	7.893	2024	2038	2055	rBV	185795	333547	84.75%	9.758%
12	7.967	2055	2061	2070	rVB2	5754	10142	2.58%	0.297%
13	8.176	2116	2126	2143	rBV3	26219	45577	11.58%	1.333%
14	8.472	2206	2218	2226	rBV3	4840	8293	2.11%	0.243%
15	8.632	2256	2268	2299	rBV	168493	332191	84.41%	9.718%
16	9.414	2497	2511	2536	rBV	216448	365110	92.77%	10.681%
17	10.751	2916	2927	2945	rVB	69003	110945	28.19%	3.246%
18	10.890	2960	2970	2980	rVB4	7436	11674	2.97%	0.342%
19	11.809	3244	3256	3279	rBV	229050	366105	93.03%	10.710%
20	12.189	3361	3374	3399	rBV	173500	286728	72.86%	8.388%
21	16.185	4607	4617	4623	rBV6	2222	4142	1.05%	0.121%




Sum of corrected areas: 3418322

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053853.D
Acq On : 24 Apr 2023 19:44
Operator : JC/MD
Sample : 02433-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

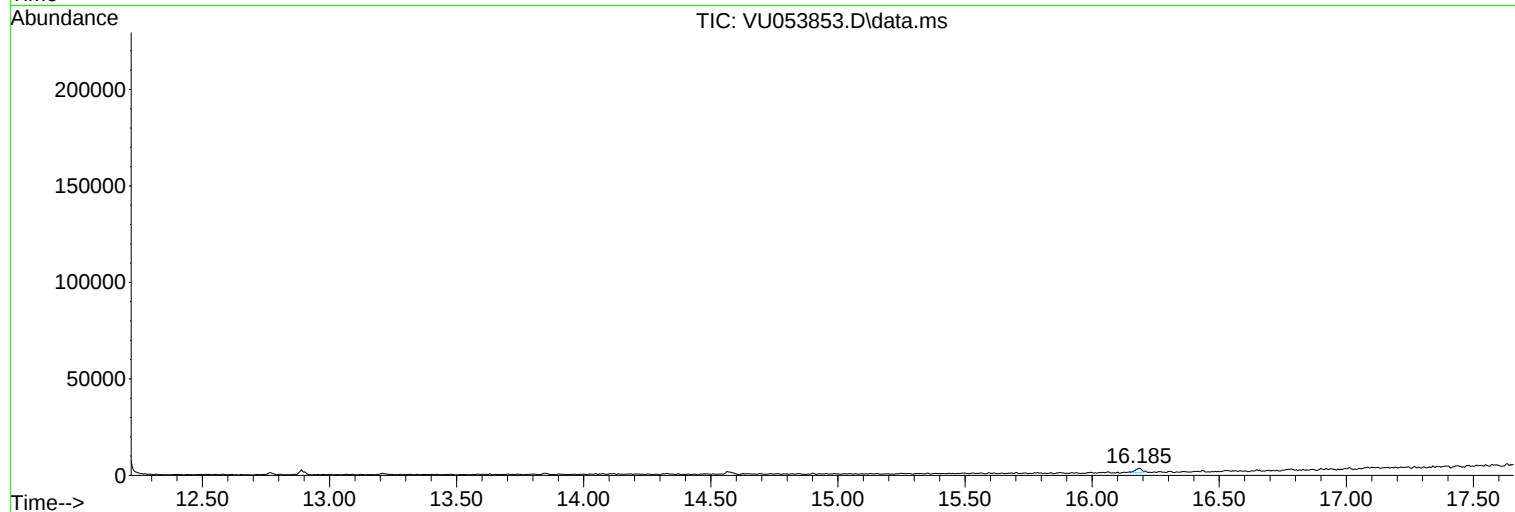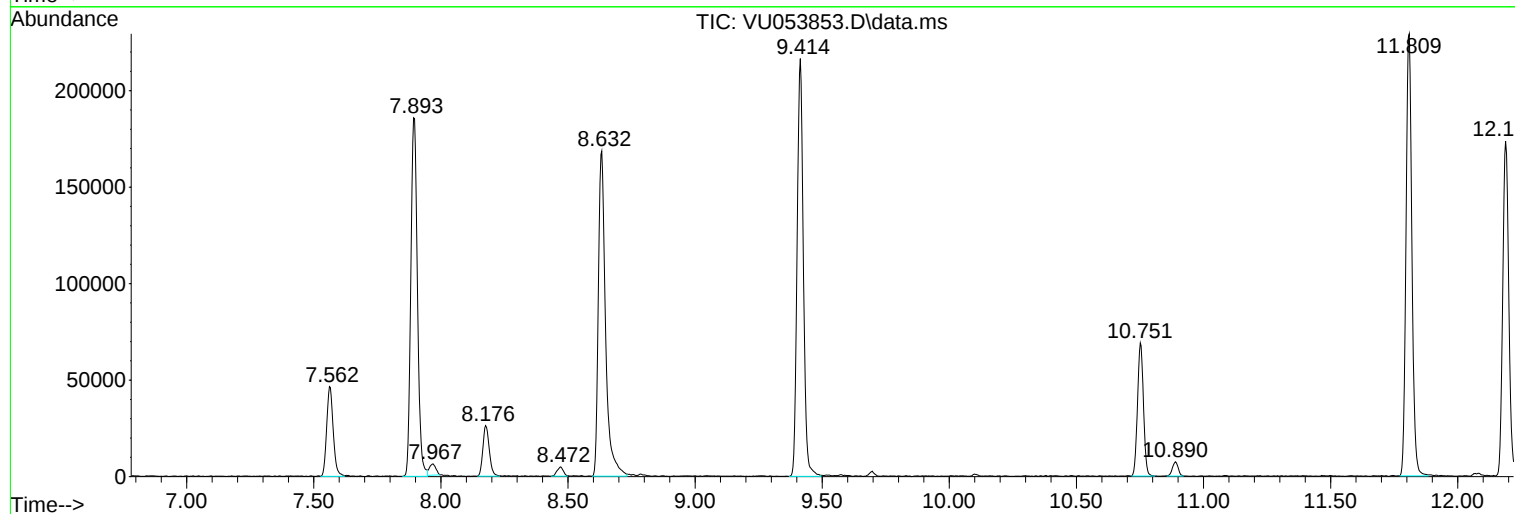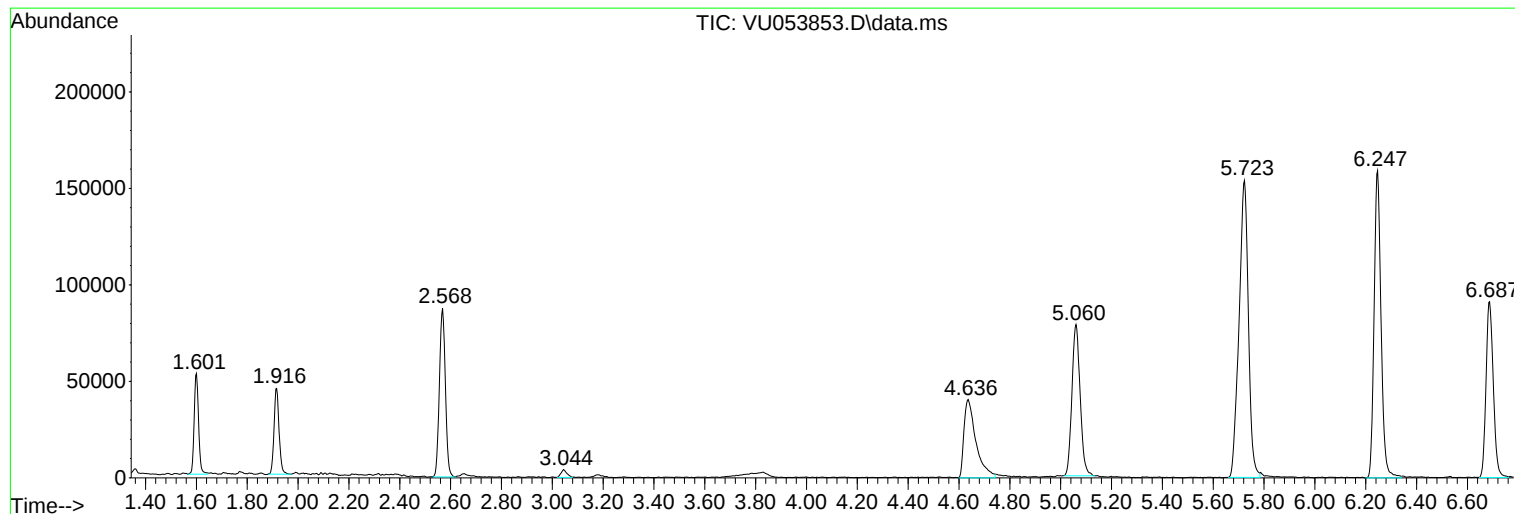

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053853.D
Acq On : 24 Apr 2023 19:44
Operator : JC/MD
Sample : 02433-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053853.D
Acq On : 24 Apr 2023 19:44
Operator : JC/MD
Sample : 02433-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE46

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
