

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053860.D
 Acq On : 24 Apr 2023 22:33
 Operator : JC/MD
 Sample : 02433-04 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE40

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053860.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	95	rVB	55233	64667	15.90%	1.833%
2	1.916	169	179	191	rBV	49103	65244	16.04%	1.849%
3	2.568	368	382	396	rBV	89938	148713	36.57%	4.214%
4	3.047	517	531	544	rBV3	20796	38789	9.54%	1.099%
5	4.639	1011	1026	1053	rBV2	39596	133845	32.91%	3.793%
6	5.060	1142	1157	1176	rVB	84833	178507	43.90%	5.059%
7	5.722	1342	1363	1386	rBV2	156542	406650	100.00%	11.524%
8	6.247	1512	1526	1551	rBV	150866	291253	71.62%	8.254%
9	6.536	1608	1616	1629	rVB5	9386	17989	4.42%	0.510%
10	6.687	1650	1663	1683	rBV3	96018	190413	46.82%	5.396%
11	7.562	1922	1935	1955	rBV	47228	84101	20.68%	2.383%
12	7.893	2026	2038	2060	rBV	197828	348333	85.66%	9.871%
13	8.176	2113	2126	2144	rBV3	26979	47561	11.70%	1.348%
14	8.472	2205	2218	2231	rBV2	3155	4932	1.21%	0.140%
15	8.549	2231	2242	2255	rBV4	18288	31755	7.81%	0.900%
16	8.632	2255	2268	2295	rBV	177808	351622	86.47%	9.965%
17	9.414	2498	2511	2535	rBV	205097	350362	86.16%	9.929%
18	10.751	2914	2927	2944	rVB	72720	118596	29.16%	3.361%
19	10.893	2958	2971	2979	rBV3	3772	5644	1.39%	0.160%
20	11.806	3241	3255	3276	rBV	215199	351890	86.53%	9.972%
21	12.188	3361	3374	3388	rBV	183292	297816	73.24%	8.440%




Sum of corrected areas: 3528682

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053860.D
Acq On : 24 Apr 2023 22:33
Operator : JC/MD
Sample : 02433-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

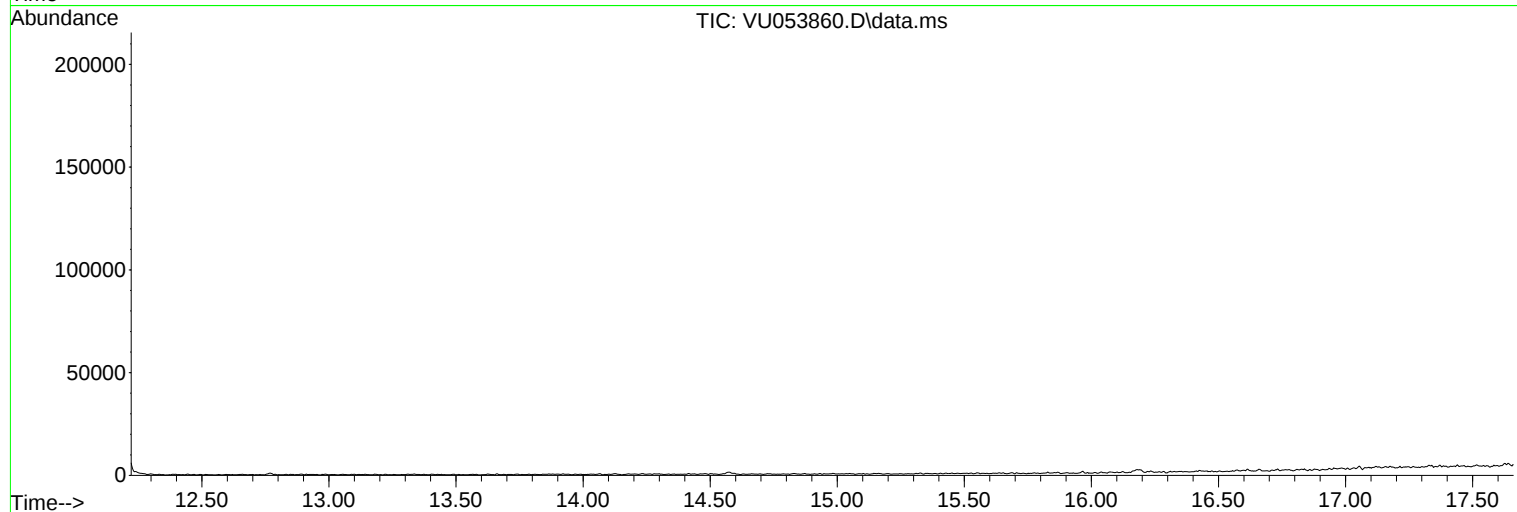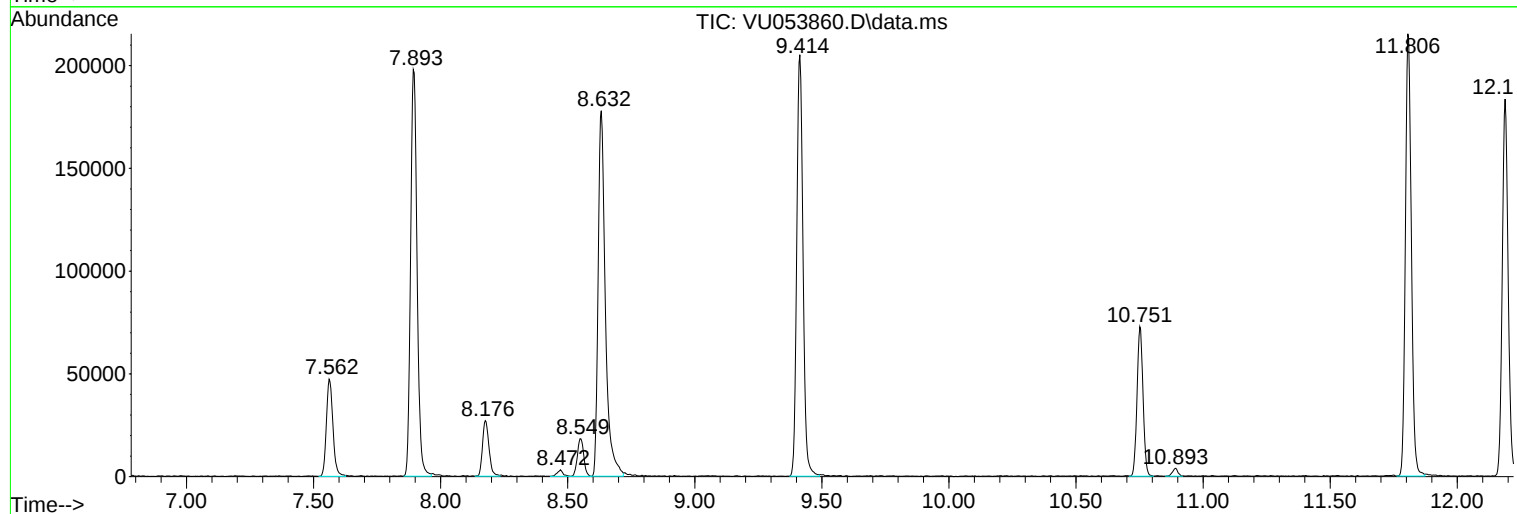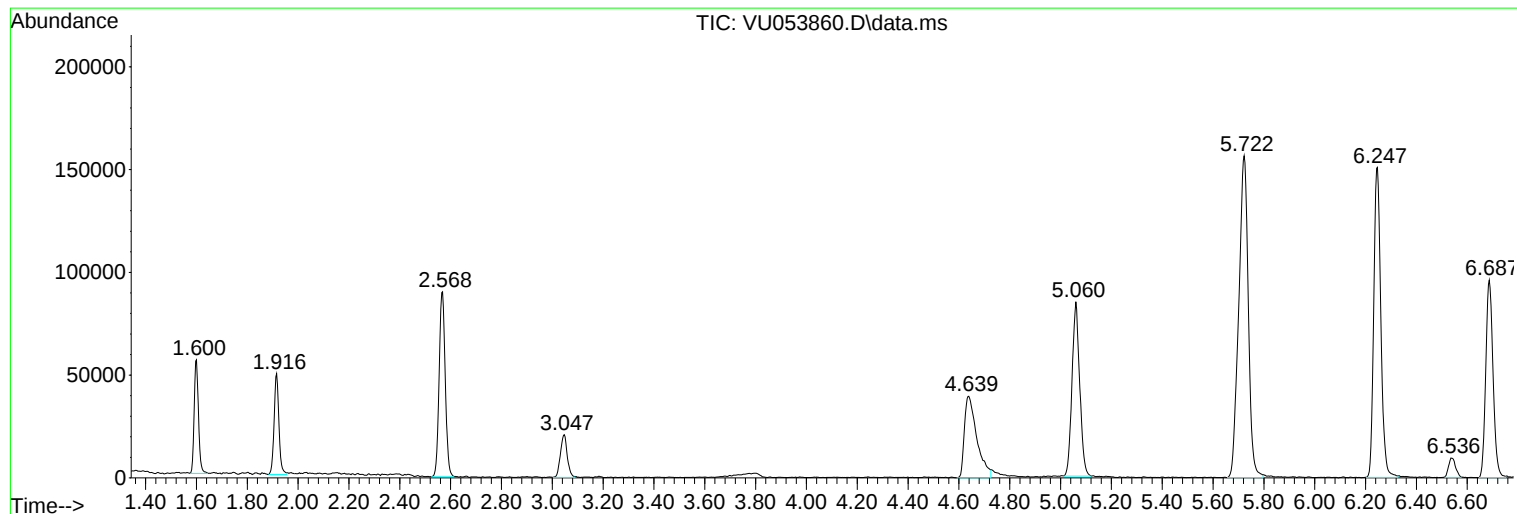

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053860.D
Acq On : 24 Apr 2023 22:33
Operator : JC/MD
Sample : 02433-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053860.D
Acq On : 24 Apr 2023 22:33
Operator : JC/MD
Sample : 02433-04 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE40

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------