

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053861.D
 Acq On : 24 Apr 2023 22:57
 Operator : JC/MD
 Sample : 02433-05 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE41

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053861.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	96	rVB	51508	61085	16.13%	1.805%
2	1.916	170	179	191	rBV	42933	56343	14.88%	1.665%
3	2.568	369	382	395	rBV	86009	140436	37.08%	4.149%
4	3.044	518	530	545	rBV	20352	37735	9.96%	1.115%
5	4.636	1014	1025	1056	rBV	38488	129422	34.17%	3.824%
6	5.060	1138	1157	1177	rBV	75933	167494	44.22%	4.948%
7	5.723	1344	1363	1387	rBV3	147120	378756	100.00%	11.190%
8	6.247	1513	1526	1546	rBV	158685	306876	81.02%	9.066%
9	6.539	1607	1617	1634	rVB2	14370	27834	7.35%	0.822%
10	6.687	1647	1663	1685	rBV2	90264	176875	46.70%	5.226%
11	7.562	1920	1935	1958	rBV	43419	78188	20.64%	2.310%
12	7.893	2025	2038	2060	rBV	180558	325535	85.95%	9.618%
13	8.176	2116	2126	2145	rBV	25292	45471	12.01%	1.343%
14	8.468	2204	2217	2224	rBV3	2477	4064	1.07%	0.120%
15	8.632	2257	2268	2299	rBV2	160952	323715	85.47%	9.564%
16	9.414	2496	2511	2533	rBV	216825	373032	98.49%	11.021%
17	10.751	2916	2927	2942	rBV	67034	109366	28.88%	3.231%
18	10.890	2962	2970	2983	rBV3	2562	3811	1.01%	0.113%
19	11.809	3242	3256	3274	rBV	223940	367043	96.91%	10.844%
20	12.189	3360	3374	3393	rBV2	159114	271710	71.74%	8.027%




Sum of corrected areas: 3384791

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053861.D
Acq On : 24 Apr 2023 22:57
Operator : JC/MD
Sample : 02433-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

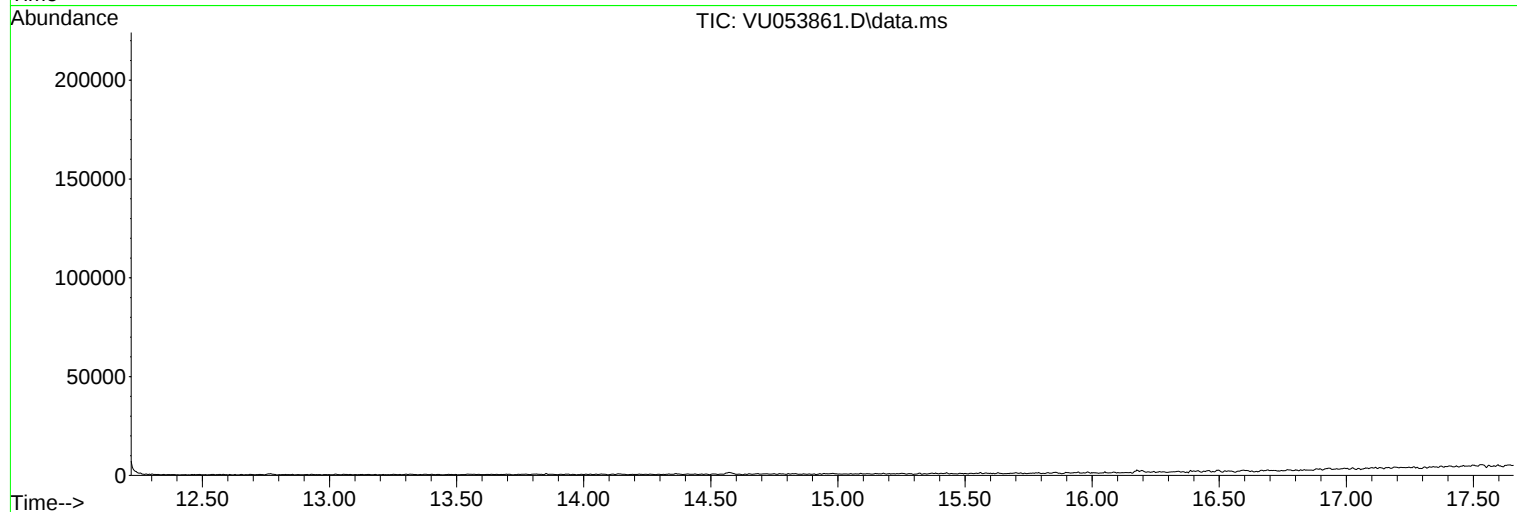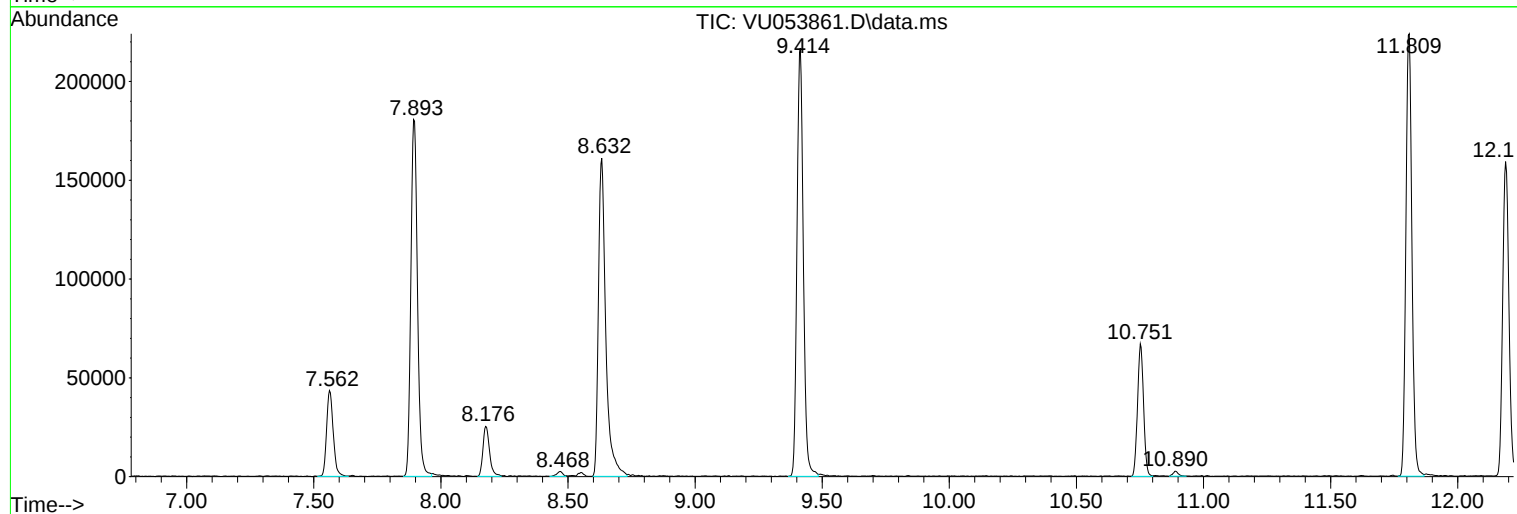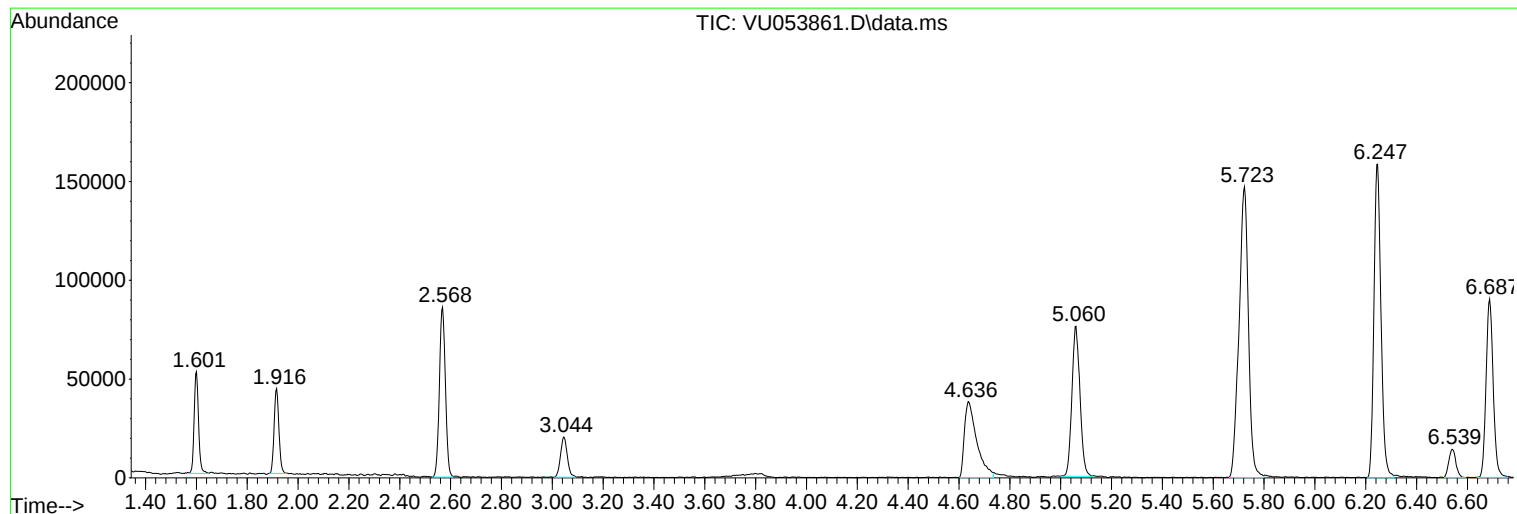

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053861.D
Acq On : 24 Apr 2023 22:57
Operator : JC/MD
Sample : 02433-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053861.D
Acq On : 24 Apr 2023 22:57
Operator : JC/MD
Sample : 02433-05 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE41

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc