

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053862.D
 Acq On : 24 Apr 2023 23:22
 Operator : JC/MD
 Sample : 02433-06 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE42

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	72	81	97	rBV	51384	62575	11.92%	1.617%
2	1.916	170	179	189	rBV	42838	54974	10.47%	1.420%
3	2.569	370	382	401	rVB	85900	139592	26.58%	3.606%
4	3.044	519	530	544	rBV2	16312	31645	6.03%	0.818%
5	4.639	1013	1026	1056	rBV	38379	128768	24.52%	3.327%
6	5.060	1142	1157	1181	rVB2	76276	167869	31.97%	4.337%
7	5.723	1343	1363	1384	rBV2	146385	378864	72.14%	9.788%
8	6.247	1510	1526	1547	rBV	156927	303046	57.71%	7.829%
9	6.543	1605	1618	1631	rVB4	13073	25061	4.77%	0.647%
10	6.687	1646	1663	1682	rBV2	90459	176871	33.68%	4.569%
11	7.562	1924	1935	1953	rBV	43191	77431	14.74%	2.000%
12	7.893	2026	2038	2060	rBV	183021	322745	61.46%	8.338%
13	8.176	2113	2126	2142	rBV2	24920	44018	8.38%	1.137%
14	8.549	2230	2242	2257	rBV	313077	525146	100.00%	13.567%
15	8.633	2257	2268	2298	rVB2	161022	317804	60.52%	8.210%
16	9.414	2499	2511	2536	rBV	219970	369579	70.38%	9.548%
17	10.752	2915	2927	2943	rBV2	68157	111272	21.19%	2.875%
18	11.806	3244	3255	3278	rBV	222719	361974	68.93%	9.351%
19	12.189	3362	3374	3389	rBV	165815	271539	51.71%	7.015%




Sum of corrected areas: 3870773

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053862.D
Acq On : 24 Apr 2023 23:22
Operator : JC/MD
Sample : 02433-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

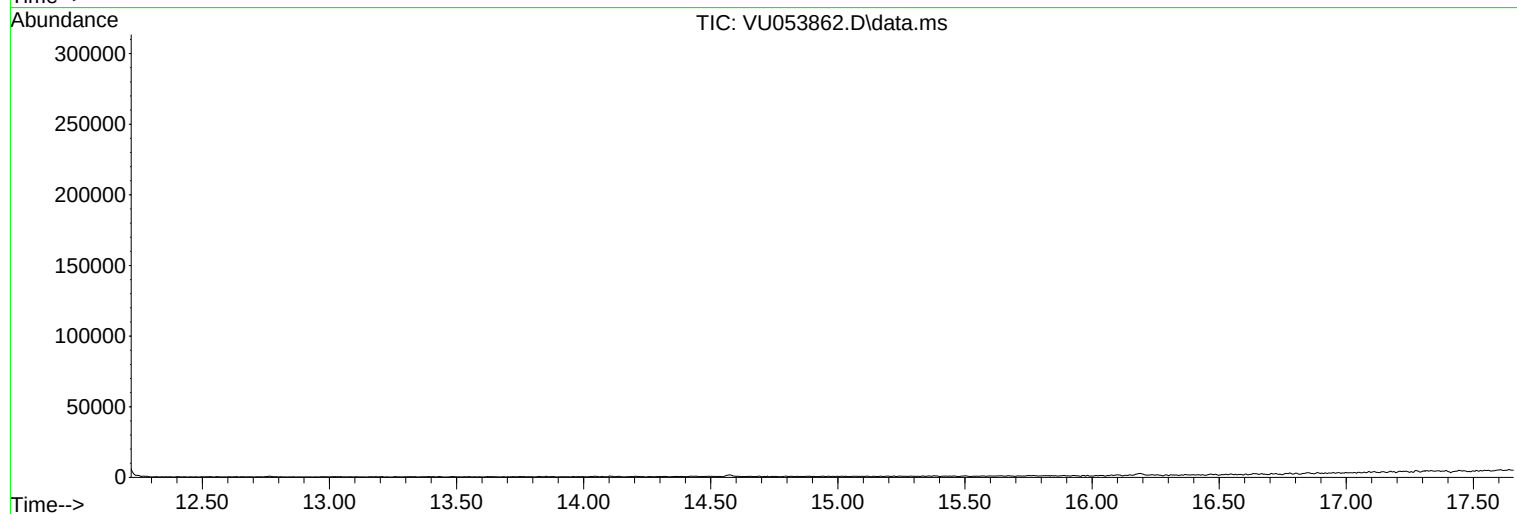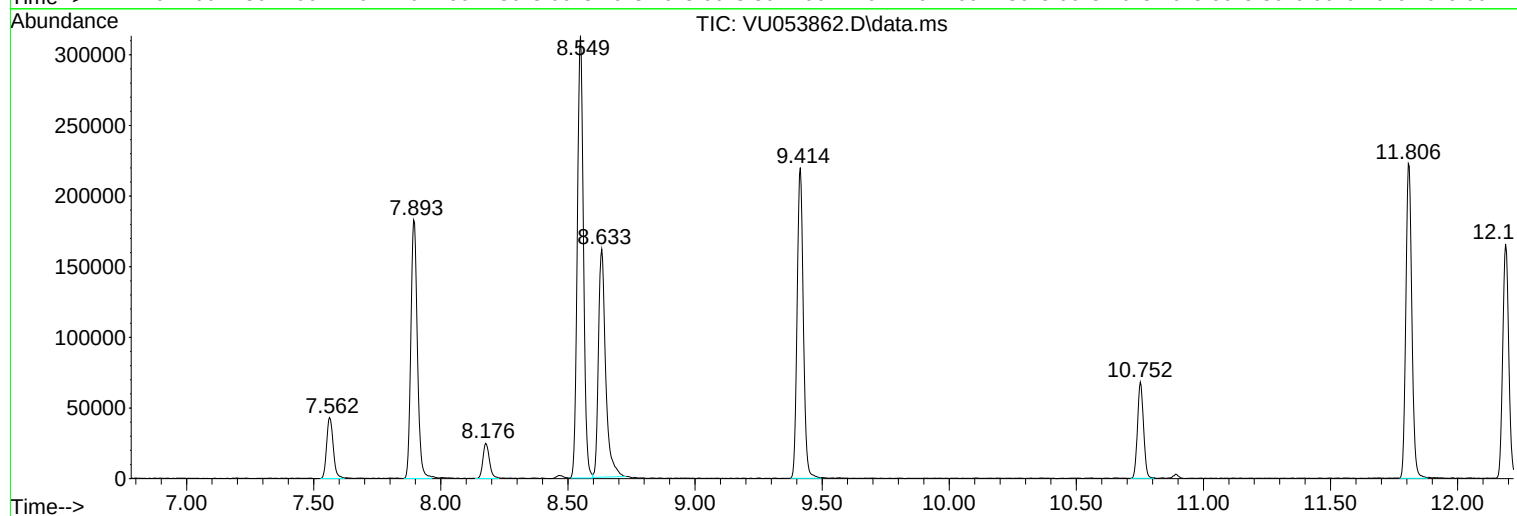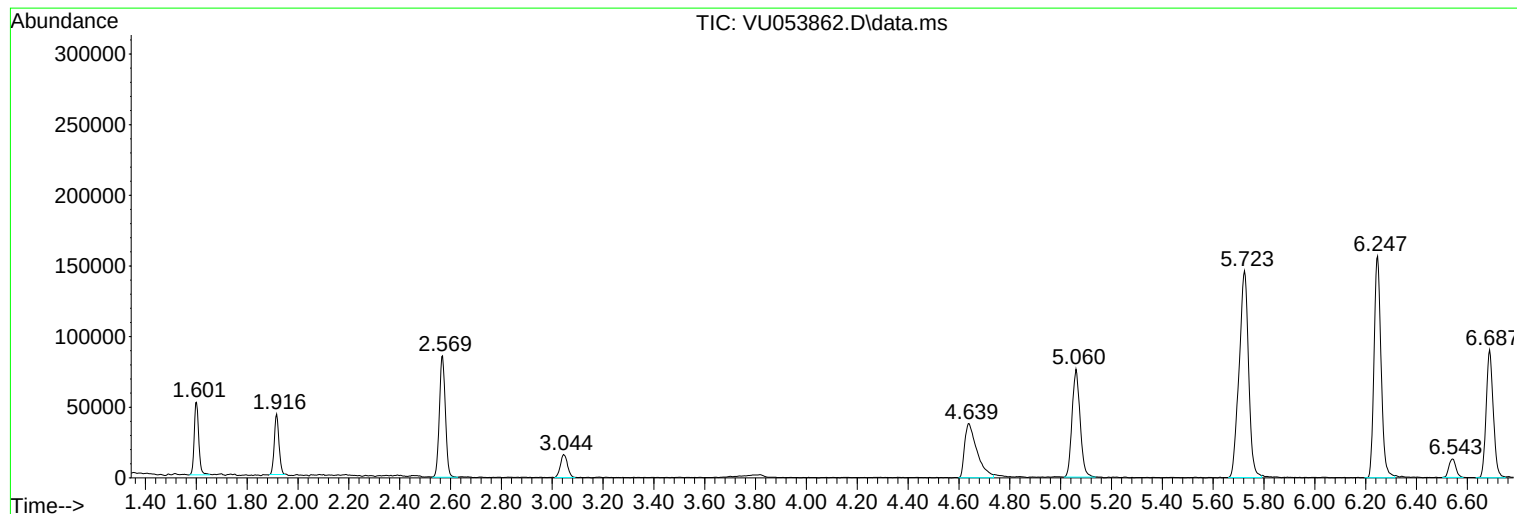

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053862.D
Acq On : 24 Apr 2023 23:22
Operator : JC/MD
Sample : 02433-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053862.D
Acq On : 24 Apr 2023 23:22
Operator : JC/MD
Sample : 02433-06 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE42

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc