

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053864.D
 Acq On : 25 Apr 2023 00:10
 Operator : JC/MD
 Sample : 02433-12 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE47

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	92	rBV	53698	62002	5.04%	1.276%
2	1.916	171	179	191	rVB	40749	55307	4.49%	1.138%
3	2.568	370	382	399	rVB2	90405	156624	12.72%	3.222%
4	3.044	518	530	545	rBV2	19483	35863	2.91%	0.738%
5	4.639	1013	1026	1027	rBV	41005	56765	4.61%	1.168%
6	5.060	1140	1157	1180	rBV2	79651	189966	15.43%	3.908%
7	5.523	1284	1301	1318	rBV3	39064	83950	6.82%	1.727%
8	5.723	1344	1363	1390	rBV2	147814	378048	30.70%	7.777%
9	6.247	1512	1526	1545	rBV	156826	304335	24.72%	6.261%
10	6.539	1600	1617	1650	rBV	647315	1231261	100.00%	25.330%
11	6.687	1650	1663	1682	rVB	90196	178642	14.51%	3.675%
12	7.562	1924	1935	1953	rBV2	44882	77798	6.32%	1.600%
13	7.896	2025	2039	2071	rBV	185533	329774	26.78%	6.784%
14	8.176	2117	2126	2147	rVB2	24945	43443	3.53%	0.894%
15	8.549	2230	2242	2257	rBV2	135987	231020	18.76%	4.753%
16	8.632	2257	2268	2296	rVV	163279	321960	26.15%	6.623%
17	9.414	2499	2511	2536	rBV	225642	375269	30.48%	7.720%
18	10.751	2913	2927	2945	rBV	67576	111106	9.02%	2.286%
19	11.809	3244	3256	3275	rBV	228273	365485	29.68%	7.519%
20	12.188	3362	3374	3398	rBV	164861	272258	22.11%	5.601%




Sum of corrected areas: 4860876

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053864.D
Acq On : 25 Apr 2023 00:10
Operator : JC/MD
Sample : 02433-12 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

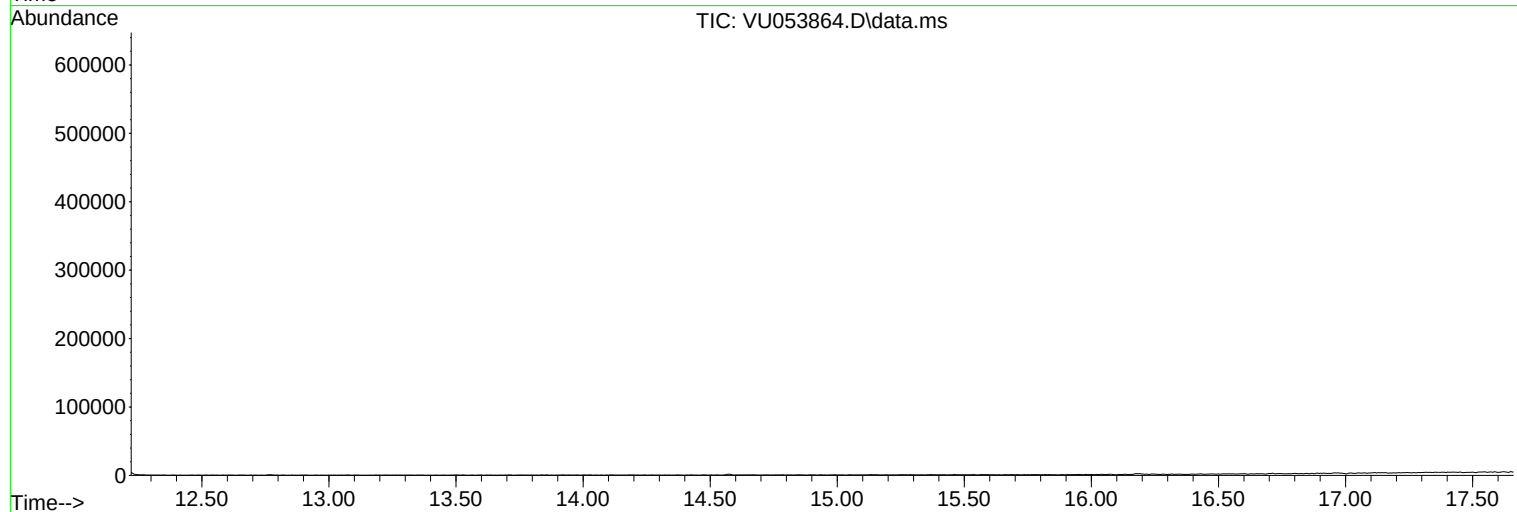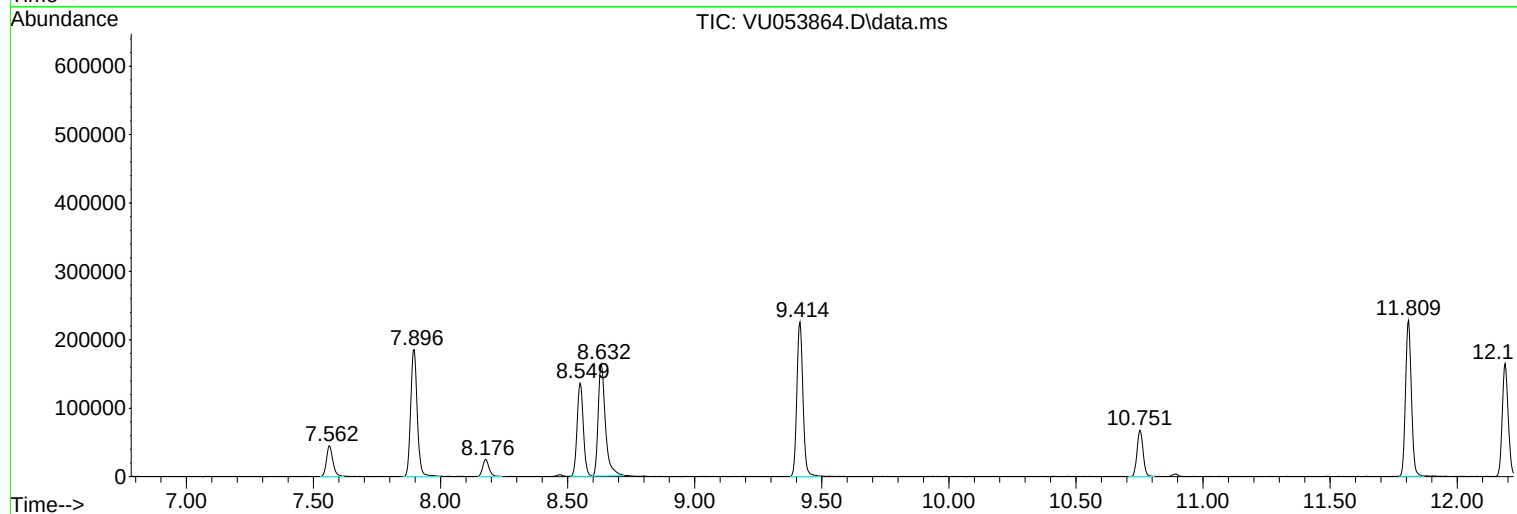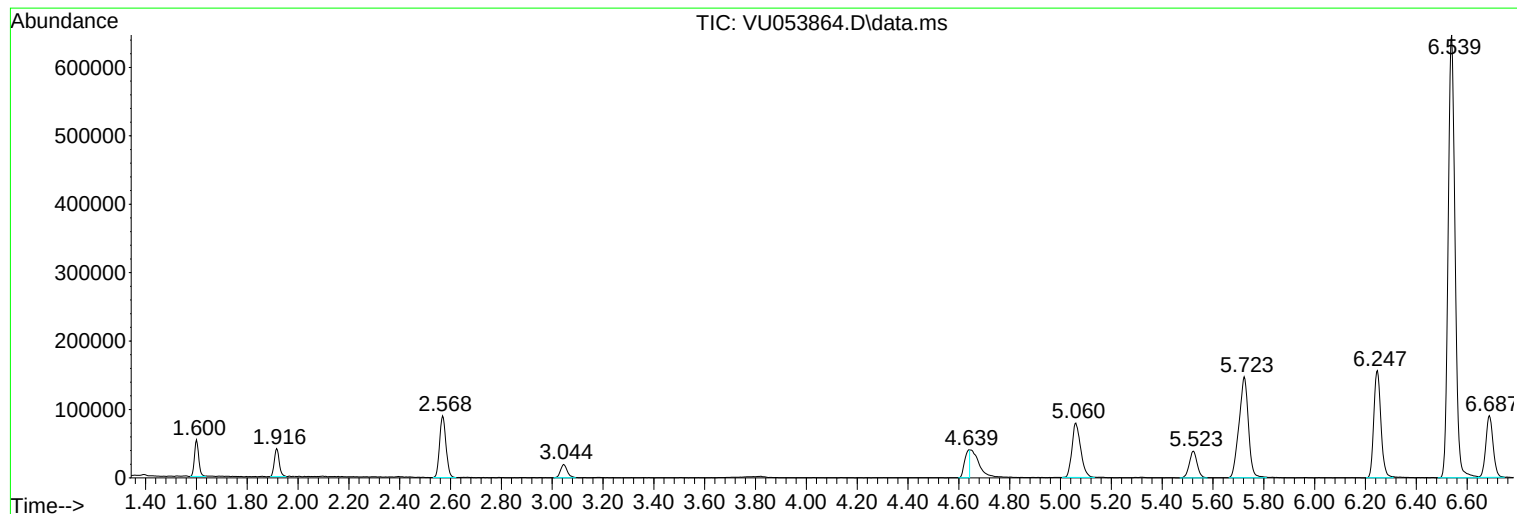

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053864.D
Acq On : 25 Apr 2023 00:10
Operator : JC/MD
Sample : 02433-12 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053864.D
Acq On : 25 Apr 2023 00:10
Operator : JC/MD
Sample : 02433-12 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 34 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE47

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc