

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053865.D
 Acq On : 25 Apr 2023 00:34
 Operator : JC/MD
 Sample : 02433-13 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE48

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053865.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	94	rVB	52243	59940	3.01%	1.112%
2	1.916	169	179	192	rBV	43287	56890	2.86%	1.056%
3	2.568	369	382	400	rVB	80573	135788	6.83%	2.520%
4	3.047	518	531	549	rVB2	16770	32413	1.63%	0.601%
5	4.639	1013	1026	1059	rBV	38819	132764	6.68%	2.464%
6	5.060	1141	1157	1183	rVB	77512	167849	8.44%	3.115%
7	5.723	1340	1363	1387	rBV2	142814	370564	18.64%	6.877%
8	6.247	1510	1526	1545	rBV	159527	303876	15.28%	5.639%
9	6.539	1606	1617	1632	rBV	41743	79905	4.02%	1.483%
10	6.687	1649	1663	1684	rBV	87693	172043	8.65%	3.193%
11	7.562	1922	1935	1959	rBV2	42998	77069	3.88%	1.430%
12	7.893	2026	2038	2060	rBV	179626	320339	16.11%	5.945%
13	8.176	2116	2126	2142	rBV	24574	42207	2.12%	0.783%
14	8.549	2228	2242	2258	rBV	1180748	1988176	100.00%	36.895%
15	8.632	2258	2268	2304	rVB	163568	331527	16.67%	6.152%
16	9.414	2499	2511	2532	rBV	220413	374710	18.85%	6.954%
17	10.751	2916	2927	2950	rBV	67629	107634	5.41%	1.997%
18	11.806	3244	3255	3273	rBV	224828	364132	18.31%	6.757%
19	12.189	3361	3374	3392	rBV	166328	270873	13.62%	5.027%




Sum of corrected areas: 5388699

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053865.D
Acq On : 25 Apr 2023 00:34
Operator : JC/MD
Sample : 02433-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

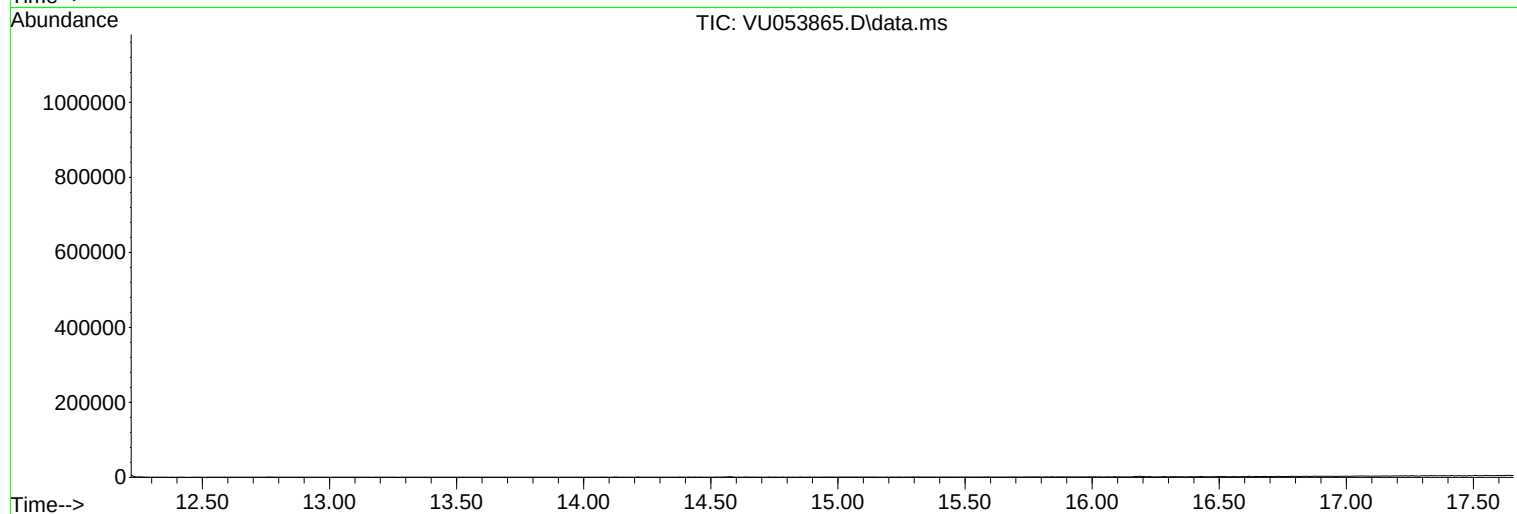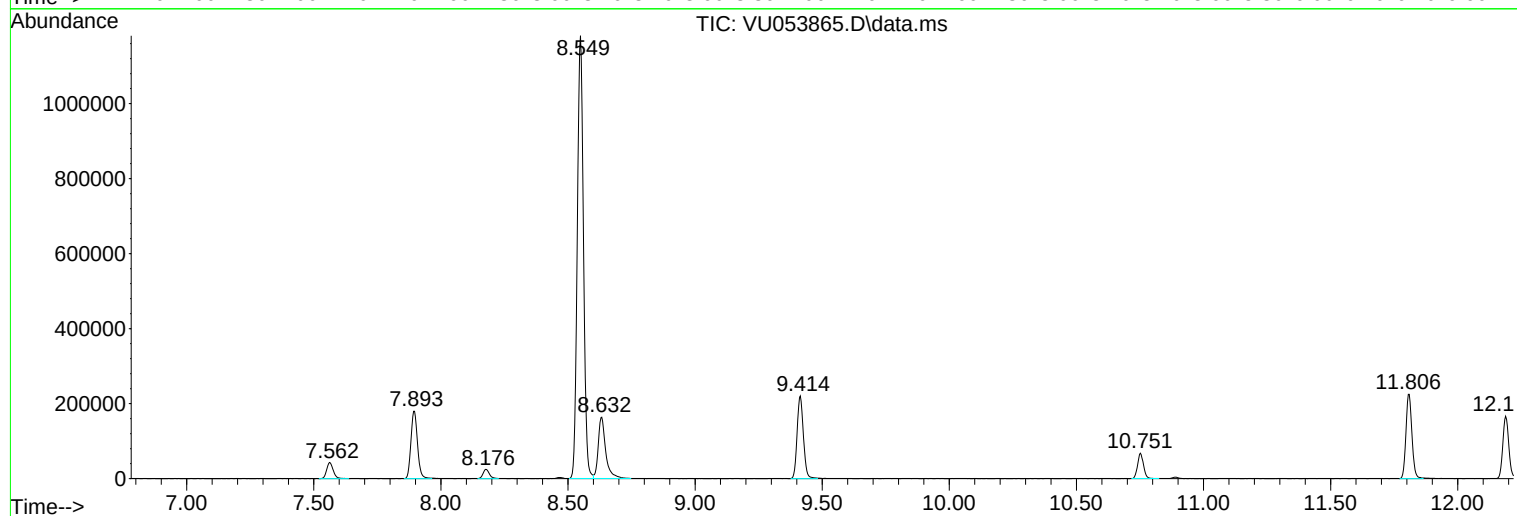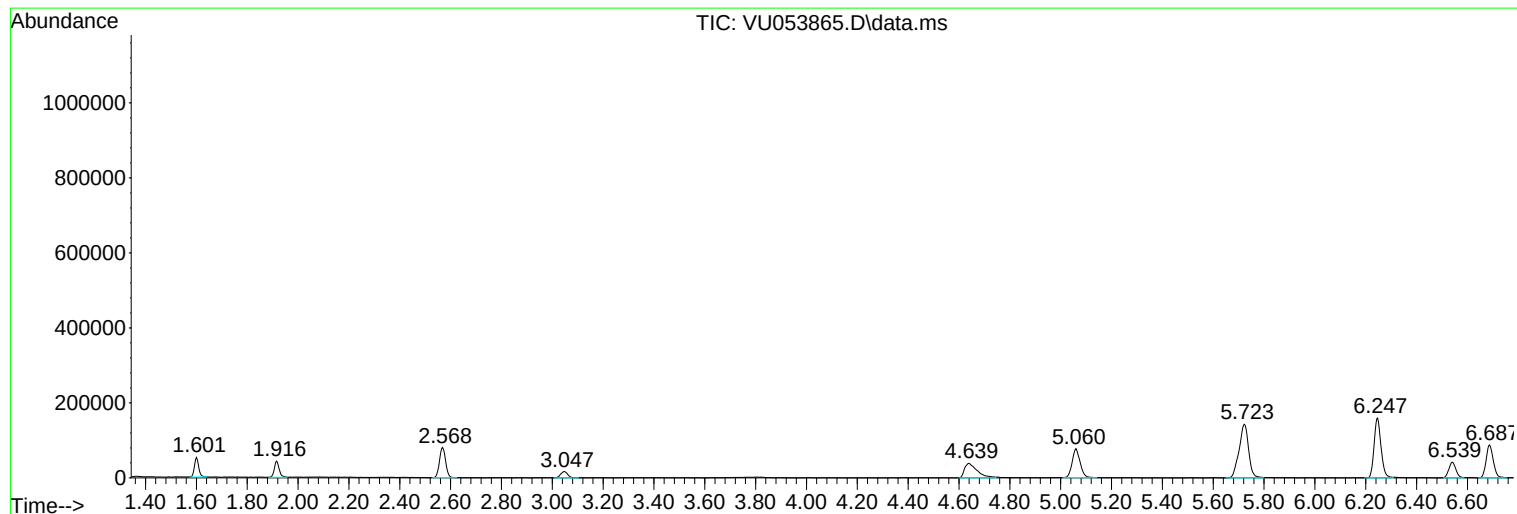

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053865.D
Acq On : 25 Apr 2023 00:34
Operator : JC/MD
Sample : 02433-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053865.D
Acq On : 25 Apr 2023 00:34
Operator : JC/MD
Sample : 02433-13 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE48

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc