

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
 Data File : VU053869.D
 Acq On : 25 Apr 2023 02:35
 Operator : JC/MD
 Sample : 02433-18 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE53

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053869.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	72	81	93	rBV	52200	59858	15.82%	1.762%
2	1.916	170	179	192	rVB	43758	56631	14.97%	1.667%
3	2.568	370	382	396	rBV2	88087	149644	39.55%	4.406%
4	3.044	517	530	545	rBV3	15295	30892	8.16%	0.910%
5	3.864	781	785	802	rVB2	4191	8481	2.24%	0.250%
6	4.639	1013	1026	1058	rBV	38777	127625	33.73%	3.758%
7	5.060	1141	1157	1179	rBV2	75503	170354	45.02%	5.016%
8	5.722	1343	1363	1382	rBV2	147245	378364	100.00%	11.140%
9	6.247	1510	1526	1544	rBV	154878	297831	78.72%	8.769%
10	6.542	1606	1618	1631	rBV3	19322	36924	9.76%	1.087%
11	6.687	1650	1663	1688	rBV2	91966	178921	47.29%	5.268%
12	7.565	1923	1936	1956	rBV3	41334	75781	20.03%	2.231%
13	7.896	2026	2039	2062	rBV	182284	324333	85.72%	9.549%
14	8.176	2115	2126	2145	rBV2	24639	43848	11.59%	1.291%
15	8.465	2206	2216	2228	rBV3	3590	6365	1.68%	0.187%
16	8.549	2233	2242	2251	rBV3	6192	9707	2.57%	0.286%
17	8.632	2255	2268	2307	rBV	163797	325791	86.11%	9.592%
18	9.414	2496	2511	2535	rBV	212663	363489	96.07%	10.702%
19	10.751	2916	2927	2941	rBV	67365	108149	28.58%	3.184%
20	10.889	2958	2970	2984	rVB2	4621	7758	2.05%	0.228%
21	11.809	3240	3256	3275	rBV	219773	359246	94.95%	10.577%
22	12.188	3362	3374	3393	rBV	171703	276543	73.09%	8.142%




Sum of corrected areas: 3396535

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053869.D
Acq On : 25 Apr 2023 02:35
Operator : JC/MD
Sample : 02433-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

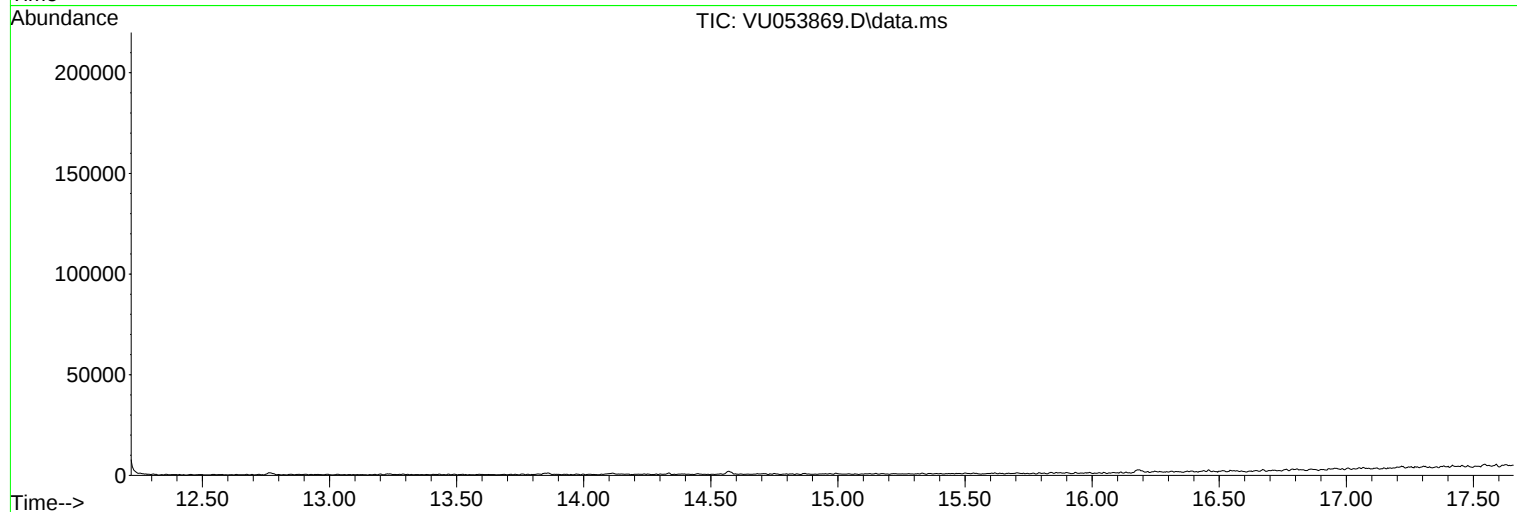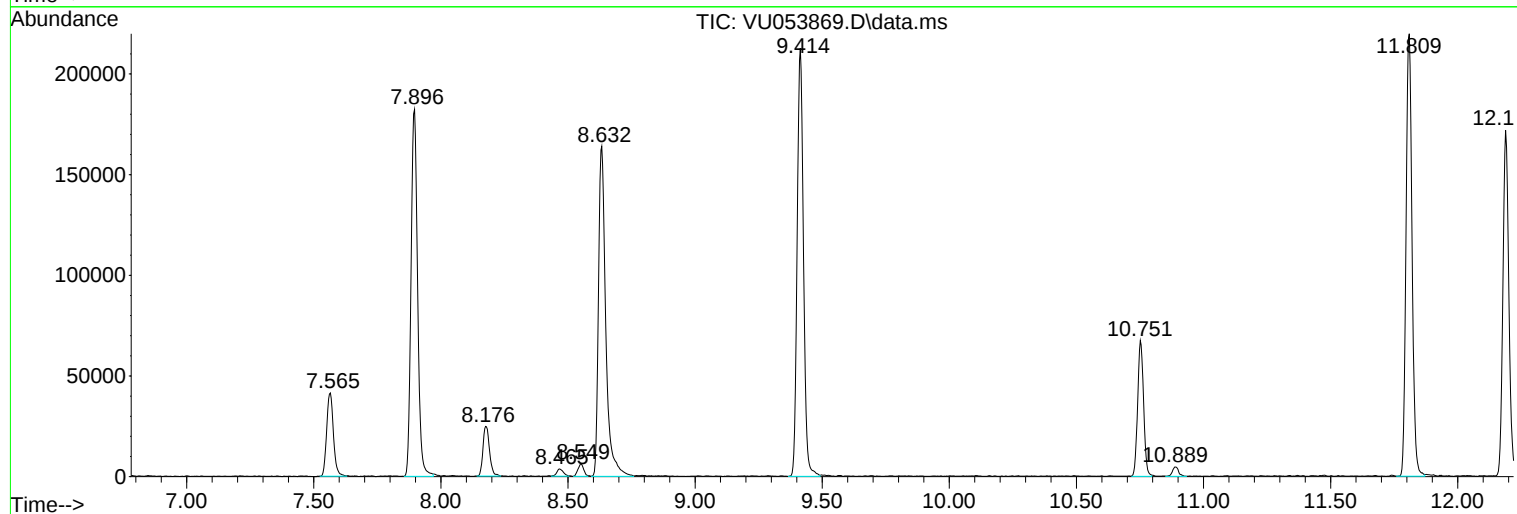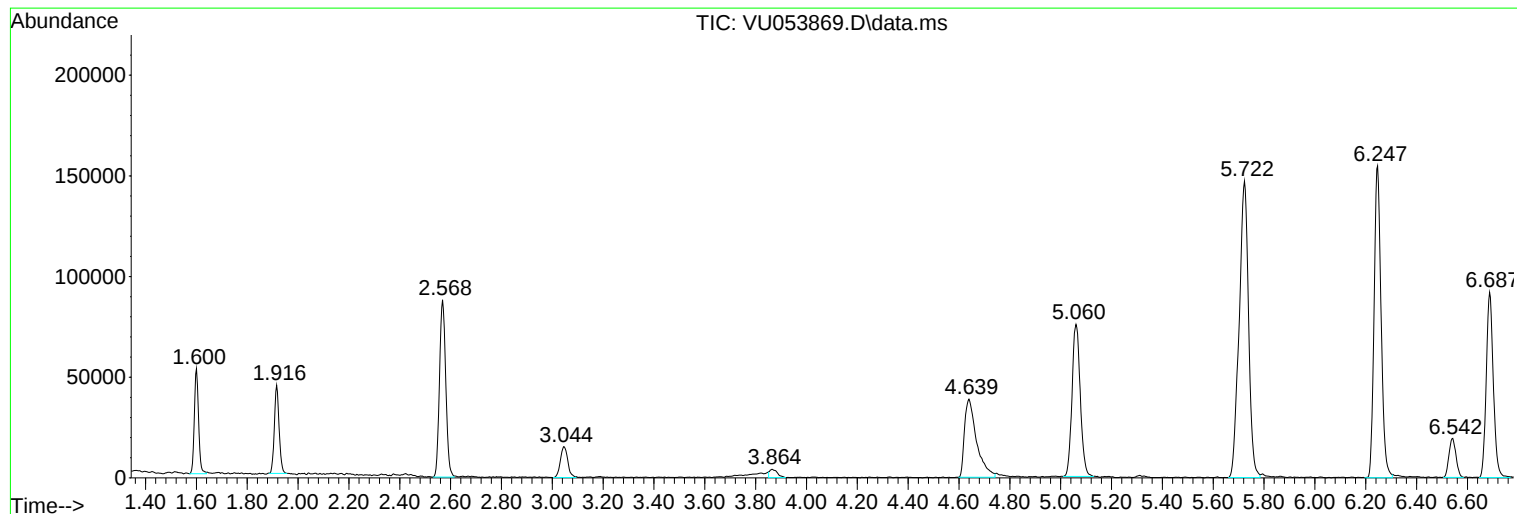

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053869.D
Acq On : 25 Apr 2023 02:35
Operator : JC/MD
Sample : 02433-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042423\
Data File : VU053869.D
Acq On : 25 Apr 2023 02:35
Operator : JC/MD
Sample : 02433-18 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE53

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc